

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035061.D
 Acq On : 08 Apr 2024 17:52
 Operator : SY/MD
 Sample : P2006-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	214487	225746	14.49%	2.007%
2	1.532	146	153	171	rVB	209676	239544	15.37%	2.129%
3	2.057	307	316	335	rBV	359135	530548	34.05%	4.716%
4	2.661	501	504	508	rBV3	479	315	0.02%	0.003%
5	2.677	508	509	512	rBV2	386	166	0.01%	0.001%
6	2.757	532	534	540	rVB3	355	224	0.01%	0.002%
7	2.796	540	546	549	rBV3	412	397	0.03%	0.004%
8	2.815	549	552	555	rBV2	405	256	0.02%	0.002%
9	2.886	572	574	576	rVB2	535	221	0.01%	0.002%
10	2.899	576	578	580	rBV	308	147	0.01%	0.001%
11	3.101	638	641	642	rBV	264	132	0.01%	0.001%
12	3.166	657	661	664	rBV2	492	411	0.03%	0.004%
13	3.246	684	686	689	rVB2	352	182	0.01%	0.002%
14	3.262	689	691	694	rBV2	275	189	0.01%	0.002%
15	3.288	697	699	702	rVV	308	177	0.01%	0.002%
16	3.388	724	730	733	rBV2	544	538	0.03%	0.005%
17	3.468	749	755	760	rVB3	454	532	0.03%	0.005%
18	3.510	760	768	770	rBV2	350	319	0.02%	0.003%
19	3.558	780	783	788	rVB3	350	332	0.02%	0.003%
20	3.616	796	801	803	rBV	353	263	0.02%	0.002%
21	3.671	813	818	821	rVB3	341	341	0.02%	0.003%
22	3.722	829	834	838	rBV3	370	292	0.02%	0.003%
23	3.751	841	843	845	rBV2	358	195	0.01%	0.002%
24	3.796	848	857	898	rBV	99160	318567	20.45%	2.832%
25	4.246	983	997	1034	rVB	237892	621005	39.86%	5.521%
26	4.632	1113	1117	1118	rBV	366	260	0.02%	0.002%
27	4.732	1145	1148	1150	rBV3	575	370	0.02%	0.003%
28	4.802	1166	1170	1172	rBV2	335	178	0.01%	0.002%
29	4.953	1201	1217	1254	rBV2	585268	1558020	100.00%	13.850%
30	5.326	1329	1333	1336	rBV5	838	562	0.04%	0.005%
31	5.449	1368	1371	1372	rBV2	366	174	0.01%	0.002%
32	5.458	1372	1374	1377	rBV3	426	256	0.02%	0.002%
33	5.532	1386	1397	1427	rBV	395328	825200	52.96%	7.336%
34	5.986	1525	1538	1568	rBV	344724	721527	46.31%	6.414%
35	6.259	1621	1623	1626	rBV3	385	192	0.01%	0.002%
36	6.371	1655	1658	1660	rBV3	371	189	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035061.D
 Acq On : 08 Apr 2024 17:52
 Operator : SY/MD
 Sample : P2006-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.500	1696	1698	1702	rBV	267	160	0.01%	0.001%
38	6.516	1702	1703	1706	rVV	350	135	0.01%	0.001%
39	6.542	1708	1711	1713	rVV	547	318	0.02%	0.003%
40	6.555	1713	1715	1718	rVV3	772	322	0.02%	0.003%
41	6.603	1727	1730	1733	rBV3	375	341	0.02%	0.003%
42	6.632	1737	1739	1742	rBV	517	384	0.02%	0.003%
43	6.786	1784	1787	1788	rBV2	343	137	0.01%	0.001%
44	6.828	1796	1800	1802	rVB2	307	218	0.01%	0.002%
45	6.912	1816	1826	1853	rBV	167756	332045	21.31%	2.952%
46	7.243	1917	1929	1966	rBV	657812	1174641	75.39%	10.442%
47	7.551	2016	2025	2059	rBV	115194	221720	14.23%	1.971%
48	7.834	2111	2113	2116	rVV3	497	308	0.02%	0.003%
49	7.873	2118	2125	2138	rVB5	2130	3712	0.24%	0.033%
50	7.950	2147	2149	2152	rBV3	316	135	0.01%	0.001%
51	7.986	2156	2160	2164	rBV3	401	347	0.02%	0.003%
52	8.027	2164	2173	2224	rBV2	307648	707405	45.40%	6.289%
53	8.651	2364	2367	2369	rBV2	589	435	0.03%	0.004%
54	8.728	2386	2391	2396	rBV4	311	278	0.02%	0.002%
55	8.783	2396	2408	2439	rBV	615254	1017991	65.34%	9.050%
56	9.053	2489	2492	2494	rBV3	454	292	0.02%	0.003%
57	9.098	2504	2506	2511	rVB3	631	519	0.03%	0.005%
58	9.124	2511	2514	2516	rBV2	371	231	0.01%	0.002%
59	9.191	2532	2535	2537	rBV	254	152	0.01%	0.001%
60	9.243	2547	2551	2552	rBV2	333	190	0.01%	0.002%
61	9.262	2554	2557	2561	rBV2	376	355	0.02%	0.003%
62	9.317	2571	2574	2576	rBV	367	240	0.02%	0.002%
63	9.420	2604	2606	2607	rBV	415	179	0.01%	0.002%
64	9.442	2611	2613	2615	rVV2	279	149	0.01%	0.001%
65	9.619	2666	2668	2672	rVB2	391	215	0.01%	0.002%
66	9.648	2672	2677	2678	rBV2	290	219	0.01%	0.002%
67	9.725	2699	2701	2702	rBV	458	206	0.01%	0.002%
68	9.908	2756	2758	2760	rBV	314	206	0.01%	0.002%
69	9.957	2770	2773	2774	rBV	252	132	0.01%	0.001%
70	10.149	2820	2833	2855	rBV	468401	741939	47.62%	6.596%
71	10.326	2880	2888	2896	rVB5	2685	4651	0.30%	0.041%
72	10.368	2899	2901	2904	rVB3	438	225	0.01%	0.002%
73	10.400	2910	2911	2915	rVB	361	163	0.01%	0.001%
74	10.468	2930	2932	2934	rBV2	275	133	0.01%	0.001%
75	10.516	2944	2947	2950	rVB2	280	169	0.01%	0.002%
76	10.535	2950	2953	2956	rBV2	459	228	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035061.D
 Acq On : 08 Apr 2024 17:52
 Operator : SY/MD
 Sample : P2006-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.577	2962	2966	2968	rBV2	411	337	0.02%	0.003%
78	10.619	2976	2979	2981	rBV3	214	135	0.01%	0.001%
79	10.651	2987	2989	2992	rVB2	342	137	0.01%	0.001%
80	10.677	2995	2997	3001	rVB2	499	231	0.01%	0.002%
81	10.722	3009	3011	3013	rBV2	315	166	0.01%	0.001%
82	10.764	3022	3024	3029	rVB2	327	167	0.01%	0.001%
83	10.792	3029	3033	3036	rBV2	456	294	0.02%	0.003%
84	10.860	3049	3054	3057	rBV2	355	355	0.02%	0.003%
85	11.027	3104	3106	3111	rVB2	347	225	0.01%	0.002%
86	11.127	3127	3137	3144	rBV5	6314	11177	0.72%	0.099%
87	11.185	3145	3155	3184	rVB	555707	884350	56.76%	7.862%
88	11.513	3248	3257	3259	rBV6	4589	6376	0.41%	0.057%
89	11.558	3261	3271	3298	rVB	636408	1015641	65.19%	9.029%
90	11.876	3367	3370	3374	rBV3	559	555	0.04%	0.005%
91	12.014	3411	3413	3416	rBV	476	218	0.01%	0.002%
92	12.426	3538	3541	3544	rBV2	302	271	0.02%	0.002%
93	12.490	3558	3561	3565	rBV2	459	324	0.02%	0.003%
94	12.522	3567	3571	3573	rVB	491	385	0.02%	0.003%
95	12.567	3583	3585	3588	rBV2	384	281	0.02%	0.002%
96	13.046	3732	3734	3740	rVB2	469	327	0.02%	0.003%
97	13.079	3740	3744	3751	rVB2	526	526	0.03%	0.005%
98	13.204	3775	3783	3794	rBV3	12931	19749	1.27%	0.176%
99	13.619	3910	3912	3916	rBV2	544	301	0.02%	0.003%
100	13.683	3922	3932	3945	rBV3	28028	46564	2.99%	0.414%




Sum of corrected areas: 11248884

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035061.D
Acq On : 08 Apr 2024 17:52
Operator : SY/MD
Sample : P2006-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

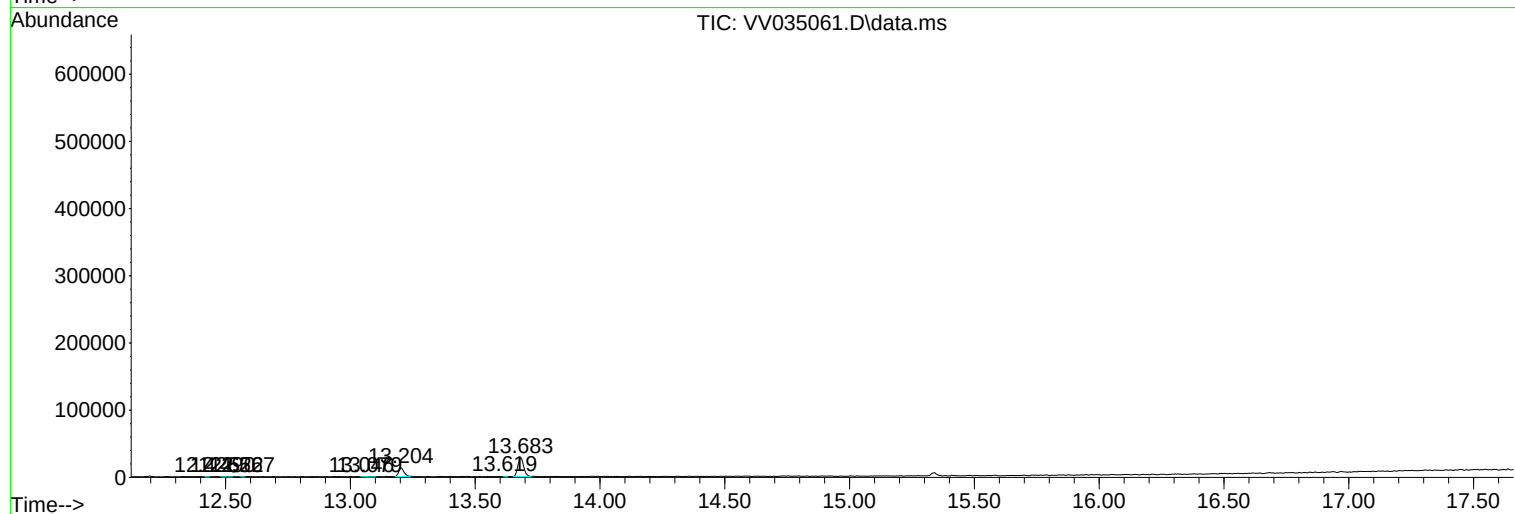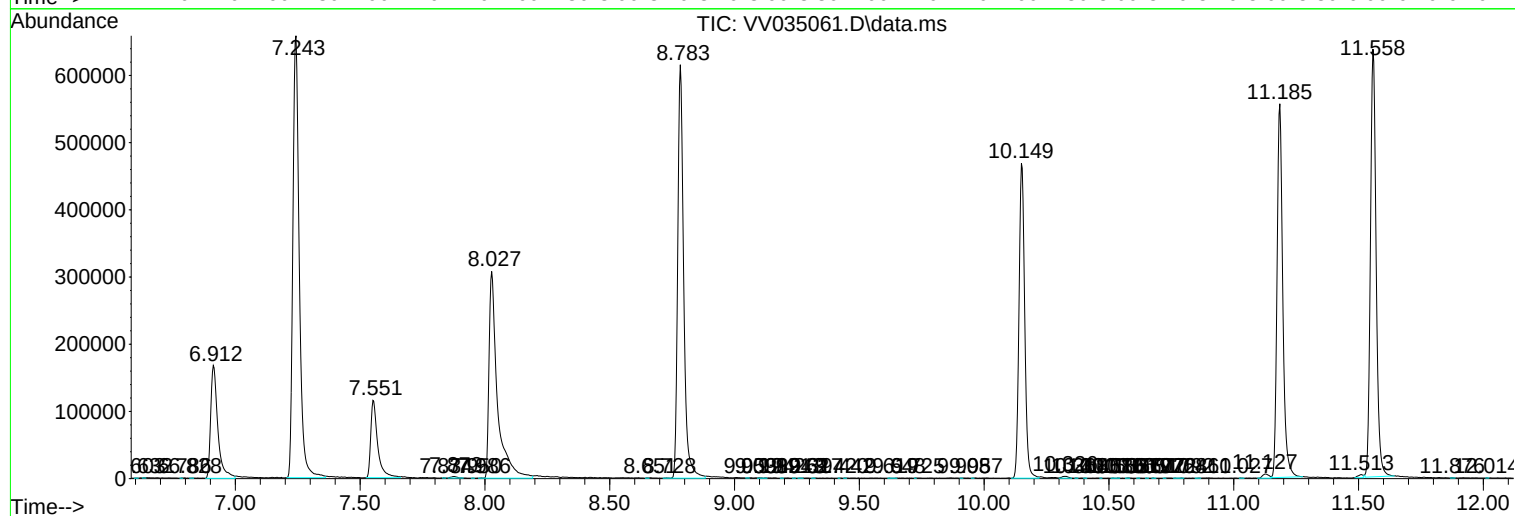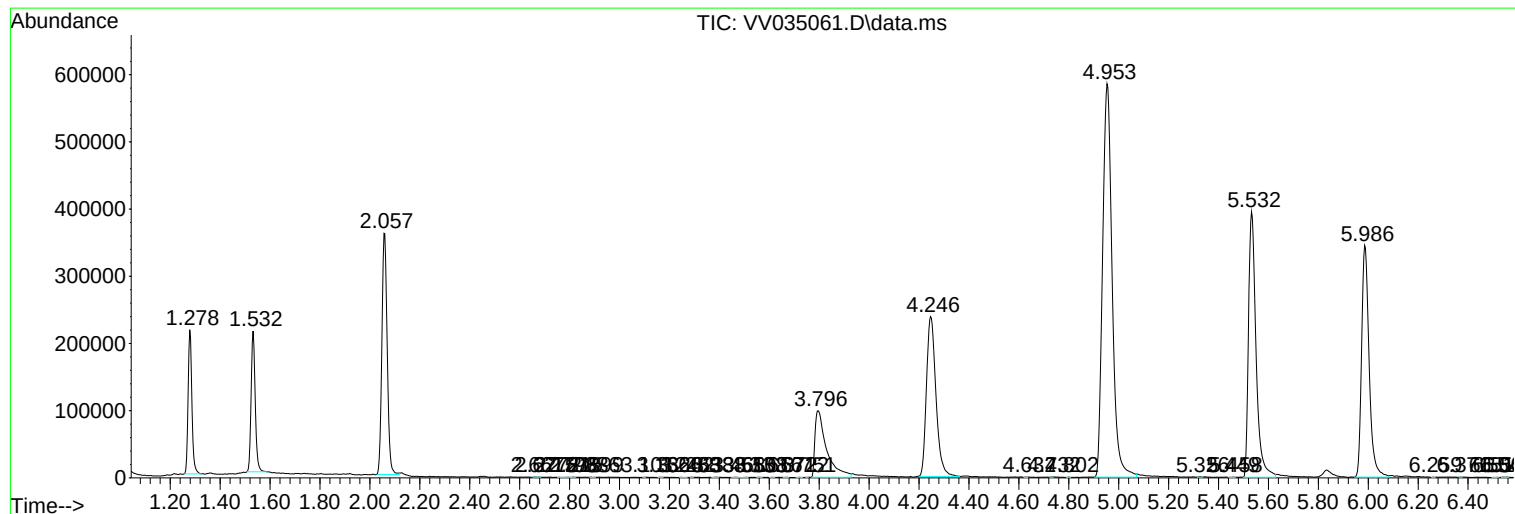

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035061.D
Acq On : 08 Apr 2024 17:52
Operator : SY/MD
Sample : P2006-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035061.D
Acq On : 08 Apr 2024 17:52
Operator : SY/MD
Sample : P2006-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------