

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035062.D
 Acq On : 08 Apr 2024 18:15
 Operator : SY/MD
 Sample : P2006-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rBV	226846	239212	14.73%	2.056%
2	1.532	146	153	168	rBV	225391	257461	15.86%	2.213%
3	2.056	307	316	333	rVB	379502	550846	33.92%	4.736%
4	2.610	486	488	490	rBV	286	159	0.01%	0.001%
5	2.687	510	512	516	rVB4	465	295	0.02%	0.003%
6	2.709	516	519	522	rBV2	631	539	0.03%	0.005%
7	2.799	543	547	552	rVB4	714	614	0.04%	0.005%
8	2.954	591	595	600	rVB2	492	334	0.02%	0.003%
9	2.989	603	606	607	rBV	328	164	0.01%	0.001%
10	3.040	619	622	627	rVB3	522	269	0.02%	0.002%
11	3.214	673	676	679	rBV3	291	202	0.01%	0.002%
12	3.233	679	682	686	rVV3	326	223	0.01%	0.002%
13	3.269	691	693	695	rBV	223	145	0.01%	0.001%
14	3.282	695	697	699	rBV3	264	164	0.01%	0.001%
15	3.365	721	723	726	rBV2	422	271	0.02%	0.002%
16	3.400	731	734	736	rBV2	255	167	0.01%	0.001%
17	3.417	737	739	743	rVB2	449	258	0.02%	0.002%
18	3.436	743	745	747	rBV2	307	172	0.01%	0.001%
19	3.516	767	770	773	rBV2	177	108	0.01%	0.001%
20	3.539	773	777	778	rBV2	493	275	0.02%	0.002%
21	3.609	795	799	801	rVB3	386	241	0.01%	0.002%
22	3.651	805	812	815	rBV	420	499	0.03%	0.004%
23	3.671	815	818	822	rBV2	330	172	0.01%	0.001%
24	3.693	822	825	829	rBV3	265	226	0.01%	0.002%
25	3.716	829	832	836	rVB3	222	181	0.01%	0.002%
26	3.735	836	838	840	rBV2	262	111	0.01%	0.001%
27	3.751	841	843	847	rVB3	425	211	0.01%	0.002%
28	3.793	848	856	908	rBV	108130	355830	21.91%	3.059%
29	4.246	982	997	1028	rBV	253804	650503	40.06%	5.592%
30	4.510	1074	1079	1081	rBV3	713	525	0.03%	0.005%
31	4.709	1139	1141	1146	rBV3	342	342	0.02%	0.003%
32	4.818	1173	1175	1179	rVB3	587	441	0.03%	0.004%
33	4.953	1201	1217	1252	rBV2	613092	1623754	100.00%	13.959%
34	5.394	1352	1354	1356	rBV2	543	252	0.02%	0.002%
35	5.455	1371	1373	1375	rBV	221	127	0.01%	0.001%
36	5.532	1386	1397	1434	rBV	407028	847951	52.22%	7.290%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035062.D
 Acq On : 08 Apr 2024 18:15
 Operator : SY/MD
 Sample : P2006-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1526	1538	1568	rBV	359017	746500	45.97%	6.418%
38	6.342	1648	1649	1655	rVB2	334	216	0.01%	0.002%
39	6.400	1663	1667	1671	rBV2	389	257	0.02%	0.002%
40	6.420	1671	1673	1674	rVB	351	119	0.01%	0.001%
41	6.433	1674	1677	1678	rBV	418	195	0.01%	0.002%
42	6.510	1697	1701	1702	rBV	227	128	0.01%	0.001%
43	6.542	1707	1711	1712	rBV	425	249	0.02%	0.002%
44	6.587	1723	1725	1726	rBV	341	118	0.01%	0.001%
45	6.712	1762	1764	1767	rBV4	391	214	0.01%	0.002%
46	6.815	1793	1796	1797	rBV	211	148	0.01%	0.001%
47	6.847	1803	1806	1811	rVB2	432	312	0.02%	0.003%
48	6.912	1814	1826	1850	rBV	176339	343103	21.13%	2.950%
49	7.243	1918	1929	1959	rBV	680792	1226573	75.54%	10.545%
50	7.551	2016	2025	2050	rBV	120226	227878	14.03%	1.959%
51	7.770	2089	2093	2094	rBV4	616	422	0.03%	0.004%
52	7.847	2114	2117	2118	rBV2	469	238	0.01%	0.002%
53	7.912	2134	2137	2138	rBV3	734	273	0.02%	0.002%
54	7.941	2143	2146	2147	rBV	279	146	0.01%	0.001%
55	7.992	2159	2162	2164	rBV2	210	176	0.01%	0.002%
56	8.027	2164	2173	2221	rBV2	333430	760924	46.86%	6.542%
57	8.609	2352	2354	2359	rVB3	653	462	0.03%	0.004%
58	8.645	2361	2365	2367	rBV3	607	369	0.02%	0.003%
59	8.690	2375	2379	2384	rVB2	603	461	0.03%	0.004%
60	8.722	2386	2389	2391	rVV2	386	222	0.01%	0.002%
61	8.783	2397	2408	2437	rBV	625267	1036104	63.81%	8.907%
62	9.108	2505	2509	2512	rBV3	455	292	0.02%	0.003%
63	9.153	2519	2523	2524	rBV2	324	216	0.01%	0.002%
64	9.188	2532	2534	2537	rBV3	445	219	0.01%	0.002%
65	9.272	2558	2560	2563	rVB	381	134	0.01%	0.001%
66	9.304	2566	2570	2572	rBV2	338	300	0.02%	0.003%
67	9.349	2582	2584	2588	rBV2	424	189	0.01%	0.002%
68	9.468	2616	2621	2626	rBV2	430	432	0.03%	0.004%
69	9.600	2660	2662	2664	rBV2	360	196	0.01%	0.002%
70	9.670	2681	2684	2692	rVB3	456	548	0.03%	0.005%
71	9.706	2692	2695	2697	rBV	303	193	0.01%	0.002%
72	9.793	2720	2722	2724	rBV	372	158	0.01%	0.001%
73	9.844	2733	2738	2745	rBV2	495	531	0.03%	0.005%
74	9.889	2750	2752	2753	rBV	244	127	0.01%	0.001%
75	9.921	2760	2762	2765	rBV2	233	156	0.01%	0.001%
76	9.969	2774	2777	2779	rBV2	294	212	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035062.D
 Acq On : 08 Apr 2024 18:15
 Operator : SY/MD
 Sample : P2006-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.998	2784	2786	2789	rBV2	421	287	0.02%	0.002%
78	10.024	2792	2794	2797	rBV	239	174	0.01%	0.001%
79	10.149	2821	2833	2859	rBV	488245	779093	47.98%	6.698%
80	10.468	2929	2932	2936	rVB3	777	463	0.03%	0.004%
81	10.561	2958	2961	2962	rBV	291	189	0.01%	0.002%
82	10.664	2990	2993	2995	rBV3	525	370	0.02%	0.003%
83	10.722	3008	3011	3017	rVB2	297	215	0.01%	0.002%
84	10.757	3020	3022	3023	rBV	394	134	0.01%	0.001%
85	10.873	3056	3058	3060	rBV	321	151	0.01%	0.001%
86	10.950	3080	3082	3084	rBV2	299	159	0.01%	0.001%
87	11.185	3144	3155	3183	rBV	560501	891574	54.91%	7.665%
88	11.436	3229	3233	3234	rBV	630	450	0.03%	0.004%
89	11.503	3245	3254	3259	rBV6	6831	12078	0.74%	0.104%
90	11.558	3261	3271	3298	rVB	665411	1056156	65.04%	9.080%
91	11.886	3369	3373	3375	rBV3	487	360	0.02%	0.003%
92	11.963	3395	3397	3399	rBV	285	143	0.01%	0.001%
93	12.091	3435	3437	3443	rBV3	532	518	0.03%	0.004%
94	12.188	3463	3467	3469	rBV2	445	415	0.03%	0.004%
95	12.371	3521	3524	3525	rBV	424	204	0.01%	0.002%
96	12.413	3533	3537	3540	rBV3	424	364	0.02%	0.003%
97	12.831	3664	3667	3668	rBV2	624	292	0.02%	0.003%
98	12.953	3703	3705	3707	rBV	446	165	0.01%	0.001%
99	13.210	3778	3785	3794	rBV6	3026	4935	0.30%	0.042%
100	13.423	3849	3851	3853	rBV2	458	176	0.01%	0.002%




Sum of corrected areas: 11632019

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035062.D
Acq On : 08 Apr 2024 18:15
Operator : SY/MD
Sample : P2006-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

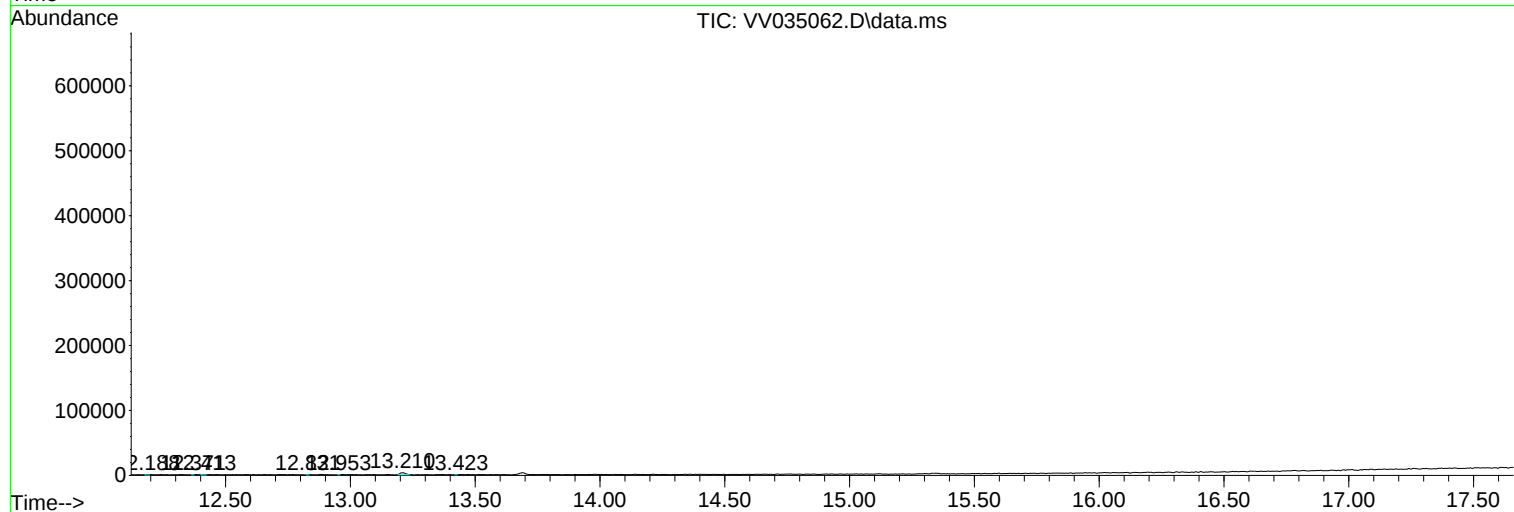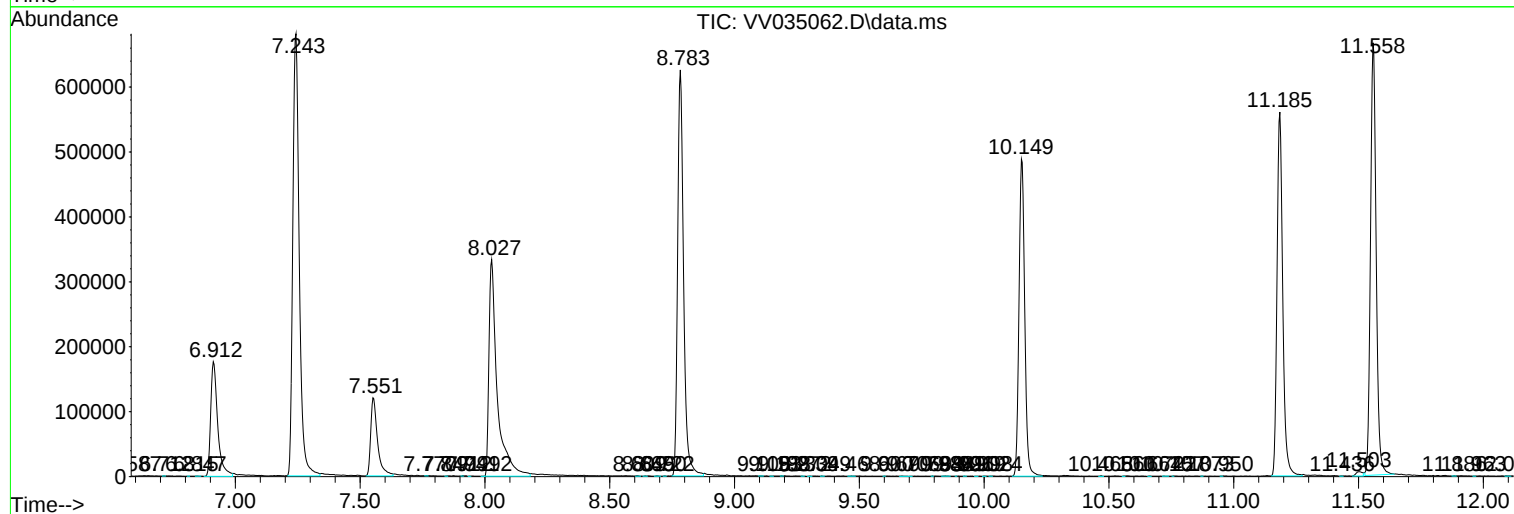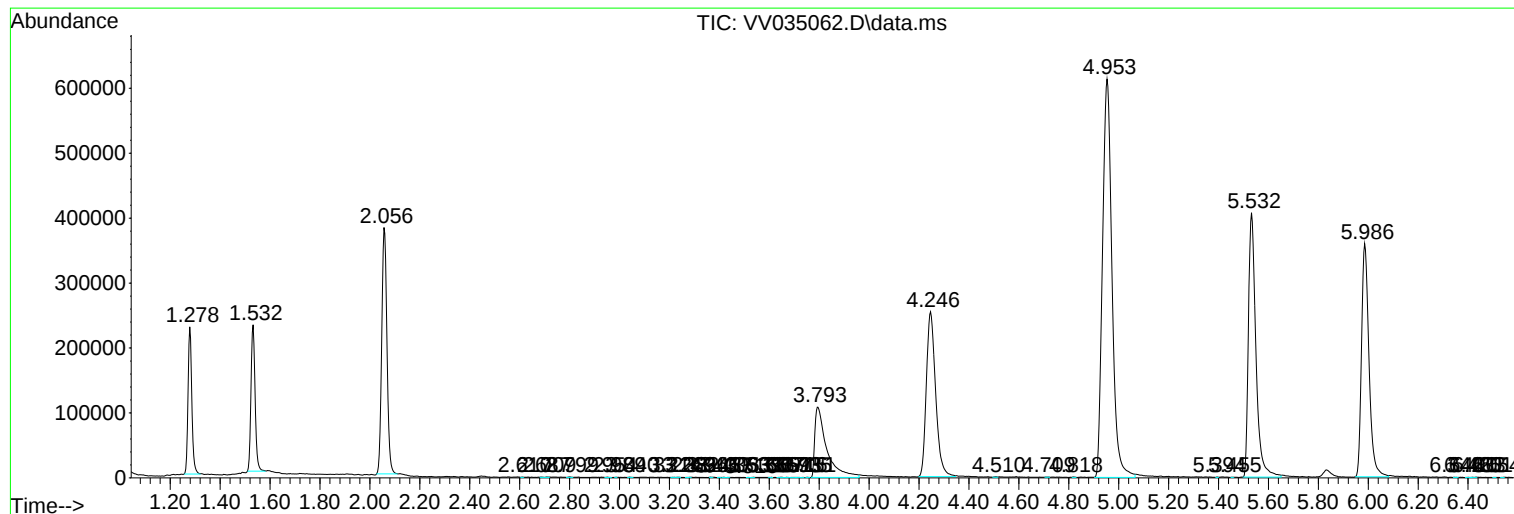

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035062.D
Acq On : 08 Apr 2024 18:15
Operator : SY/MD
Sample : P2006-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035062.D
Acq On : 08 Apr 2024 18:15
Operator : SY/MD
Sample : P2006-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------