

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035063.D
 Acq On : 08 Apr 2024 18:39
 Operator : SY/MD
 Sample : P2006-15DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RH3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	219240	233248	3.02%	0.859%
2	1.532	146	153	178	rVB	222354	261794	3.39%	0.964%
3	2.060	307	317	334	rVB	371006	539856	7.00%	1.988%
4	2.445	431	437	451	rVB4	5363	9384	0.12%	0.035%
5	2.513	454	458	465	rVB5	793	830	0.01%	0.003%
6	2.600	483	485	486	rBV	395	165	0.00%	0.001%
7	2.642	496	498	499	rBV	334	123	0.00%	0.000%
8	2.687	509	512	514	rBV2	432	271	0.00%	0.001%
9	2.712	518	520	526	rVB2	646	275	0.00%	0.001%
10	2.751	530	532	535	rBV	246	158	0.00%	0.001%
11	2.815	550	552	554	rVV	258	66	0.00%	0.000%
12	2.844	557	561	567	rBV4	443	456	0.01%	0.002%
13	2.873	568	570	574	rVB3	416	238	0.00%	0.001%
14	2.969	598	600	601	rBV	505	239	0.00%	0.001%
15	3.011	611	613	615	rBV2	313	158	0.00%	0.001%
16	3.047	621	624	631	rVB4	407	372	0.00%	0.001%
17	3.072	631	632	633	rBV4	225	74	0.00%	0.000%
18	3.092	634	638	642	rVB2	374	319	0.00%	0.001%
19	3.124	646	648	649	rBV	175	69	0.00%	0.000%
20	3.133	649	651	653	rBV	255	116	0.00%	0.000%
21	3.166	657	661	663	rBV2	479	394	0.01%	0.001%
22	3.291	698	700	703	rVB2	360	163	0.00%	0.001%
23	3.310	703	706	707	rBV2	300	161	0.00%	0.001%
24	3.362	720	722	726	rVB2	270	174	0.00%	0.001%
25	3.407	732	736	737	rBV2	312	147	0.00%	0.001%
26	3.526	771	773	777	rVB2	202	105	0.00%	0.000%
27	3.545	777	779	784	rVB3	346	201	0.00%	0.001%
28	3.609	796	799	800	rBV2	214	124	0.00%	0.000%
29	3.645	803	810	811	rBV3	492	423	0.01%	0.002%
30	3.764	845	847	848	rBV3	136	56	0.00%	0.000%
31	3.793	848	856	896	rBV	111227	344247	4.46%	1.268%
32	4.246	983	997	1029	rBV	248847	642111	8.32%	2.365%
33	4.738	1139	1150	1168	rVB6	4275	10545	0.14%	0.039%
34	4.953	1201	1217	1226	rBV2	620243	1571220	20.36%	5.786%
35	5.490	1382	1384	1386	rBV	327	161	0.00%	0.001%
36	5.532	1386	1397	1427	rBV	422973	874602	11.34%	3.221%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035063.D
 Acq On : 08 Apr 2024 18:39
 Operator : SY/MD
 Sample : P2006-15DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORH3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.918	1515	1517	1520	rBV4	549	321	0.00%	0.001%
38	5.985	1525	1538	1567	rBV	354606	746319	9.67%	2.749%
39	6.400	1664	1667	1669	rBV	366	213	0.00%	0.001%
40	6.452	1680	1683	1685	rBV4	582	269	0.00%	0.001%
41	6.484	1689	1693	1694	rBV	398	246	0.00%	0.001%
42	6.754	1773	1777	1784	rBV5	611	843	0.01%	0.003%
43	6.815	1793	1796	1797	rVB	245	122	0.00%	0.000%
44	6.834	1797	1802	1806	rBV3	355	426	0.01%	0.002%
45	6.911	1816	1826	1855	rBV	174084	340306	4.41%	1.253%
46	7.243	1918	1929	1963	rBV	684798	1216070	15.76%	4.478%
47	7.551	2016	2025	2063	rBV	117958	226177	2.93%	0.833%
48	7.889	2127	2130	2133	rBV2	482	315	0.00%	0.001%
49	7.931	2141	2143	2146	rBV2	376	174	0.00%	0.001%
50	7.960	2149	2152	2154	rVB2	390	220	0.00%	0.001%
51	7.972	2154	2156	2160	rBV3	244	177	0.00%	0.001%
52	8.027	2163	2173	2219	rBV2	335611	753765	9.77%	2.776%
53	8.644	2363	2365	2368	rBV2	239	150	0.00%	0.001%
54	8.689	2376	2379	2382	rBV3	533	369	0.00%	0.001%
55	8.741	2393	2395	2397	rBV2	410	210	0.00%	0.001%
56	8.808	2397	2416	2459	rVV2	4120637	7715684	100.00%	28.415%
57	9.378	2590	2593	2595	rBV2	477	304	0.00%	0.001%
58	9.525	2636	2639	2641	rBV2	418	301	0.00%	0.001%
59	9.603	2660	2663	2664	rBV	463	239	0.00%	0.001%
60	9.689	2688	2690	2691	rBV	252	102	0.00%	0.000%
61	9.715	2695	2698	2701	rBV	557	344	0.00%	0.001%
62	9.760	2709	2712	2714	rBV	268	170	0.00%	0.001%
63	9.808	2723	2727	2734	rBV3	368	391	0.01%	0.001%
64	9.982	2778	2781	2782	rBV	171	100	0.00%	0.000%
65	9.992	2782	2784	2790	rVB3	268	173	0.00%	0.001%
66	10.030	2794	2796	2802	rVB4	469	414	0.01%	0.002%
67	10.149	2819	2833	2856	rBV	490859	778754	10.09%	2.868%
68	10.429	2919	2920	2921	rBV	308	103	0.00%	0.000%
69	10.496	2938	2941	2942	rBV	359	169	0.00%	0.001%
70	10.734	3013	3015	3016	rBV	268	102	0.00%	0.000%
71	10.847	3048	3050	3054	rVB2	566	251	0.00%	0.001%
72	10.879	3056	3060	3064	rBV3	446	399	0.01%	0.001%
73	10.927	3073	3075	3077	rBV2	338	191	0.00%	0.001%
74	11.062	3116	3117	3120	rBV2	283	174	0.00%	0.001%
75	11.117	3123	3134	3145	rBV	268581	426856	5.53%	1.572%
76	11.204	3146	3161	3191	rVB2	2365736	4599103	59.61%	16.937%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035063.D
Acq On : 08 Apr 2024 18:39
Operator : SY/MD
Sample : P2006-15DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	11.574	3258	3276	3305	rBV2	2540058	4825150	62.54%	17.770%
78	12.156	3455	3457	3458	rBV2	254	106	0.00%	0.000%
79	12.693	3618	3624	3635	rBV7	2180	3060	0.04%	0.011%
80	12.773	3647	3649	3653	rBV2	468	195	0.00%	0.001%
81	12.792	3653	3655	3659	rVB	511	232	0.00%	0.001%
82	12.956	3703	3706	3711	rBV2	462	348	0.00%	0.001%
83	13.197	3769	3781	3801	rBV	498200	790580	10.25%	2.912%
84	13.680	3920	3931	3952	rVB2	138558	222805	2.89%	0.821%
85	15.336	4441	4446	4457	rVB6	4739	7048	0.09%	0.026%




Sum of corrected areas: 27153585

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035063.D
Acq On : 08 Apr 2024 18:39
Operator : SY/MD
Sample : P2006-15DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

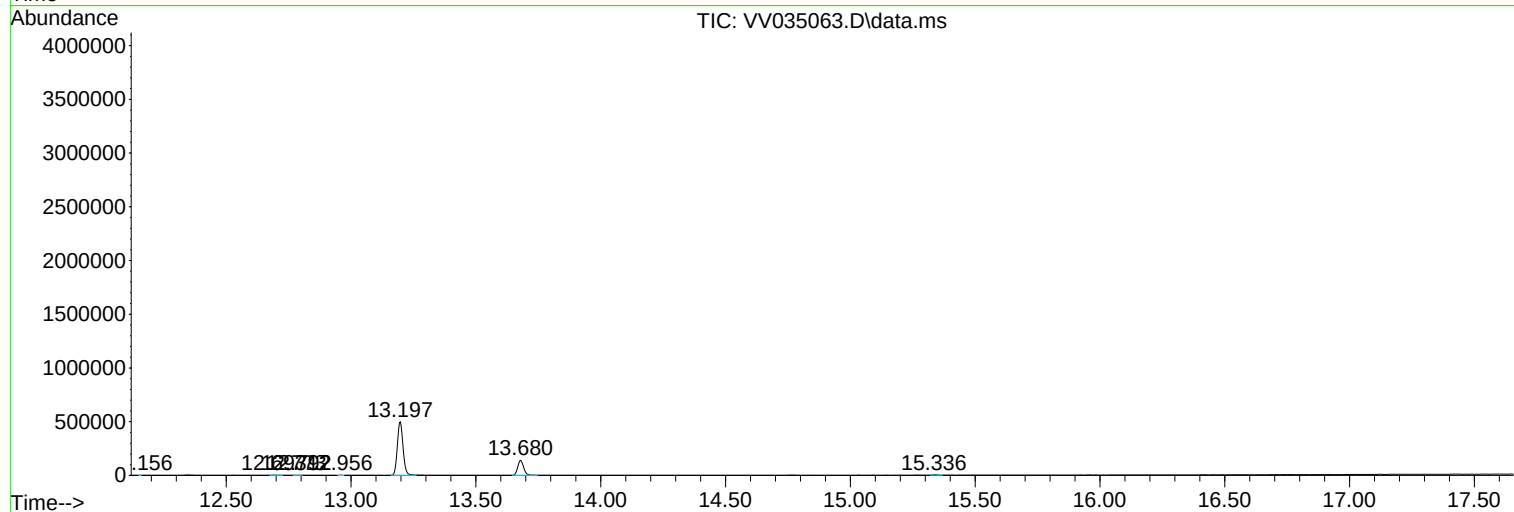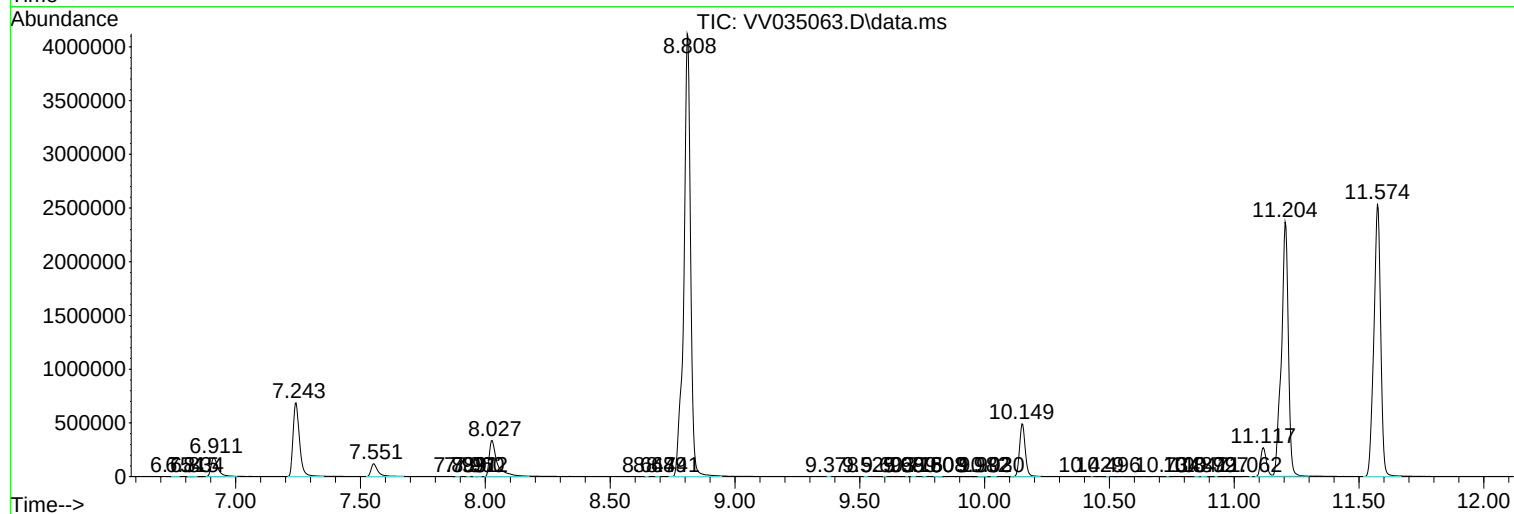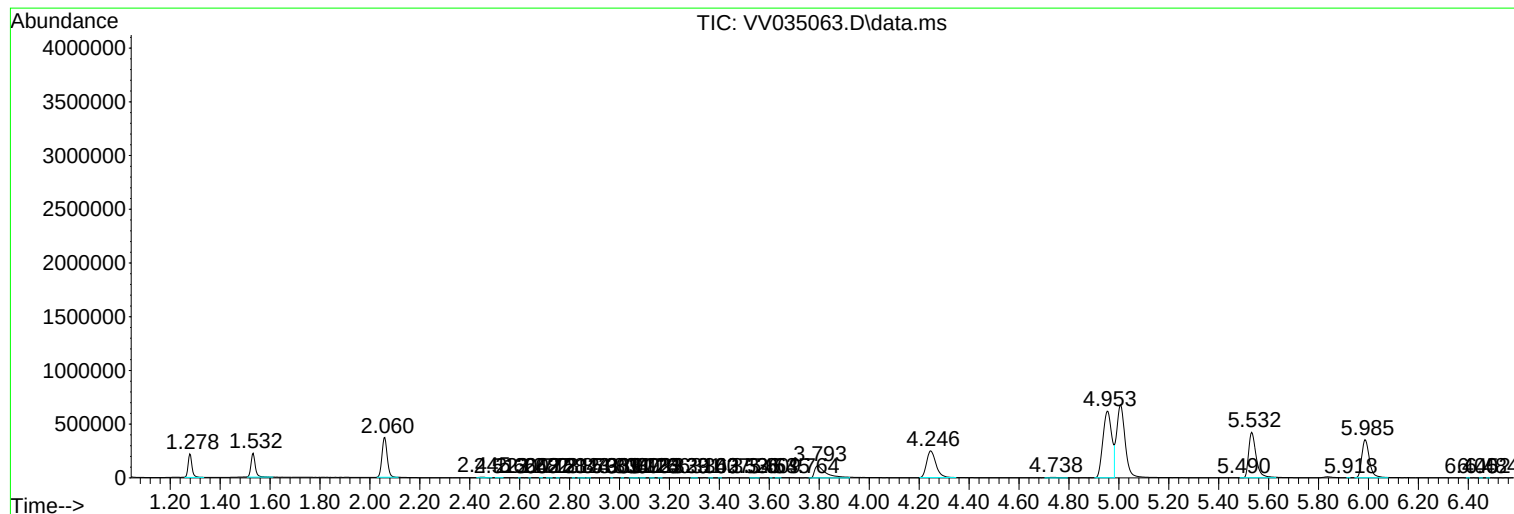

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035063.D
Acq On : 08 Apr 2024 18:39
Operator : SY/MD
Sample : P2006-15DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035063.D
Acq On : 08 Apr 2024 18:39
Operator : SY/MD
Sample : P2006-15DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc