

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035064.D
 Acq On : 08 Apr 2024 19:03
 Operator : SY/MD
 Sample : P2006-11DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	217224	226900	4.97%	1.006%
2	1.532	146	153	171	rVB	226237	261437	5.73%	1.159%
3	2.056	307	316	333	rVB	360022	522998	11.46%	2.319%
4	2.449	430	438	452	rBV6	3341	5759	0.13%	0.026%
5	2.706	515	518	520	rVB3	435	205	0.00%	0.001%
6	2.748	528	531	535	rBV3	338	321	0.01%	0.001%
7	2.806	546	549	550	rBV	277	135	0.00%	0.001%
8	2.854	562	564	566	rVV2	384	135	0.00%	0.001%
9	2.912	577	582	585	rBV5	314	379	0.01%	0.002%
10	2.941	589	591	596	rVB4	405	314	0.01%	0.001%
11	3.005	608	611	614	rBV2	437	343	0.01%	0.002%
12	3.053	623	626	627	rBV	241	146	0.00%	0.001%
13	3.063	627	629	634	rVB4	364	244	0.01%	0.001%
14	3.089	634	637	640	rVB	299	196	0.00%	0.001%
15	3.117	640	646	647	rBV3	481	388	0.01%	0.002%
16	3.146	653	655	659	rVB3	206	116	0.00%	0.001%
17	3.207	670	674	676	rVB3	367	210	0.00%	0.001%
18	3.298	698	702	703	rBV	225	142	0.00%	0.001%
19	3.336	711	714	716	rVB2	353	181	0.00%	0.001%
20	3.349	716	718	721	rVB	324	182	0.00%	0.001%
21	3.365	721	723	726	rBV	494	297	0.01%	0.001%
22	3.420	738	740	743	rVV2	288	161	0.00%	0.001%
23	3.487	759	761	766	rVB2	278	156	0.00%	0.001%
24	3.516	766	770	771	rBV	247	184	0.00%	0.001%
25	3.613	796	800	806	rBV3	418	513	0.01%	0.002%
26	3.648	807	811	812	rBV3	302	198	0.00%	0.001%
27	3.719	827	833	835	rBV3	328	257	0.01%	0.001%
28	3.793	847	856	901	rBV	114195	366129	8.03%	1.624%
29	4.246	983	997	1023	rBV	247317	630014	13.81%	2.794%
30	4.735	1134	1149	1158	rBV8	1828	4384	0.10%	0.019%
31	4.793	1164	1167	1169	rBV2	331	259	0.01%	0.001%
32	4.953	1201	1217	1227	rBV2	614947	1565793	34.32%	6.944%
33	5.410	1357	1359	1361	rBV2	431	140	0.00%	0.001%
34	5.423	1361	1363	1365	rBV	481	241	0.01%	0.001%
35	5.532	1386	1397	1432	rBV	420313	878453	19.26%	3.896%
36	5.831	1481	1490	1506	rBV2	8668	19762	0.43%	0.088%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035064.D
 Acq On : 08 Apr 2024 19:03
 Operator : SY/MD
 Sample : P2006-11DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.905	1512	1513	1514	rBV2	379	143	0.00%	0.001%
38	5.986	1524	1538	1572	rBV	351552	745401	16.34%	3.306%
39	6.291	1631	1633	1635	rBV2	386	141	0.00%	0.001%
40	6.365	1654	1656	1658	rVB	378	138	0.00%	0.001%
41	6.403	1664	1668	1670	rBV2	450	288	0.01%	0.001%
42	6.522	1702	1705	1706	rBV2	233	129	0.00%	0.001%
43	6.532	1706	1708	1710	rVB2	352	114	0.00%	0.001%
44	6.612	1728	1733	1735	rBV2	438	374	0.01%	0.002%
45	6.683	1753	1755	1758	rVB2	515	266	0.01%	0.001%
46	6.715	1758	1765	1770	rBV5	871	969	0.02%	0.004%
47	6.738	1770	1772	1775	rVB3	473	297	0.01%	0.001%
48	6.760	1777	1779	1785	rBV4	511	434	0.01%	0.002%
49	6.783	1785	1786	1789	rVB4	365	161	0.00%	0.001%
50	6.799	1789	1791	1792	rBV	284	124	0.00%	0.001%
51	6.828	1797	1800	1802	rVB3	359	171	0.00%	0.001%
52	6.850	1805	1807	1811	rBV2	447	382	0.01%	0.002%
53	6.912	1816	1826	1859	rBV	174245	340331	7.46%	1.509%
54	7.243	1918	1929	1964	rBV	677896	1208005	26.48%	5.357%
55	7.551	2017	2025	2048	rBV	118290	219839	4.82%	0.975%
56	7.780	2093	2096	2099	rBV4	678	601	0.01%	0.003%
57	7.879	2125	2127	2130	rBV3	270	111	0.00%	0.000%
58	7.956	2149	2151	2154	rVB	334	114	0.00%	0.001%
59	7.989	2158	2161	2162	rVB2	376	160	0.00%	0.001%
60	8.027	2163	2173	2220	rBV2	336869	765144	16.77%	3.393%
61	8.455	2304	2306	2309	rBV3	579	212	0.00%	0.001%
62	8.651	2364	2367	2368	rBV	202	99	0.00%	0.000%
63	8.809	2397	2416	2455	rBV2	1923098	4206978	92.22%	18.656%
64	9.352	2582	2585	2593	rVB4	603	670	0.01%	0.003%
65	9.429	2604	2609	2611	rBV	415	313	0.01%	0.001%
66	9.442	2611	2613	2614	rBV	356	122	0.00%	0.001%
67	9.487	2625	2627	2634	rBV3	579	615	0.01%	0.003%
68	9.577	2653	2655	2658	rBV	478	351	0.01%	0.002%
69	9.677	2684	2686	2691	rBV2	255	147	0.00%	0.001%
70	9.722	2698	2700	2703	rVB	395	198	0.00%	0.001%
71	9.860	2738	2743	2746	rVB2	338	327	0.01%	0.001%
72	9.879	2746	2749	2752	rBV3	479	424	0.01%	0.002%
73	9.895	2752	2754	2756	rVV2	314	130	0.00%	0.001%
74	9.995	2783	2785	2791	rVB2	248	184	0.00%	0.001%
75	10.037	2797	2798	2801	rVB2	296	135	0.00%	0.001%
76	10.063	2801	2806	2808	rBV2	433	370	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035064.D
 Acq On : 08 Apr 2024 19:03
 Operator : SY/MD
 Sample : P2006-11DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.111	2818	2821	2822	rBV	329	165	0.00%	0.001%
78	10.149	2822	2833	2859	rVV	496878	781745	17.14%	3.467%
79	10.577	2963	2966	2972	rBV3	424	389	0.01%	0.002%
80	10.606	2972	2975	2977	rBV2	354	256	0.01%	0.001%
81	10.677	2993	2997	3000	rBV3	256	234	0.01%	0.001%
82	10.886	3056	3062	3064	rBV3	448	484	0.01%	0.002%
83	10.905	3065	3068	3071	rVV2	244	217	0.00%	0.001%
84	10.966	3085	3087	3090	rVB	294	184	0.00%	0.001%
85	10.992	3091	3095	3098	rBV	324	275	0.01%	0.001%
86	11.034	3103	3108	3109	rBV2	454	351	0.01%	0.002%
87	11.120	3124	3135	3145	rBV	111879	181981	3.99%	0.807%
88	11.204	3145	3161	3189	rVB2	2072199	4096692	89.80%	18.167%
89	11.574	3259	3276	3308	rBV2	2368641	4562132	100.00%	20.231%
90	11.895	3375	3376	3379	rVB2	630	183	0.00%	0.001%
91	12.027	3415	3417	3421	rBV4	512	381	0.01%	0.002%
92	12.214	3473	3475	3479	rBV2	642	355	0.01%	0.002%
93	12.403	3532	3534	3537	rBV3	569	278	0.01%	0.001%
94	12.451	3547	3549	3550	rBV	359	101	0.00%	0.000%
95	12.474	3554	3556	3558	rBV2	357	196	0.00%	0.001%
96	12.821	3661	3664	3667	rBV3	518	317	0.01%	0.001%
97	12.995	3716	3718	3721	rBV2	403	263	0.01%	0.001%
98	13.050	3731	3735	3737	rBV2	466	359	0.01%	0.002%
99	13.197	3770	3781	3811	rBV	514153	804131	17.63%	3.566%
100	13.680	3921	3931	3946	rBV2	83832	135268	2.97%	0.600%




Sum of corrected areas: 22549721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035064.D
Acq On : 08 Apr 2024 19:03
Operator : SY/MD
Sample : P2006-11DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

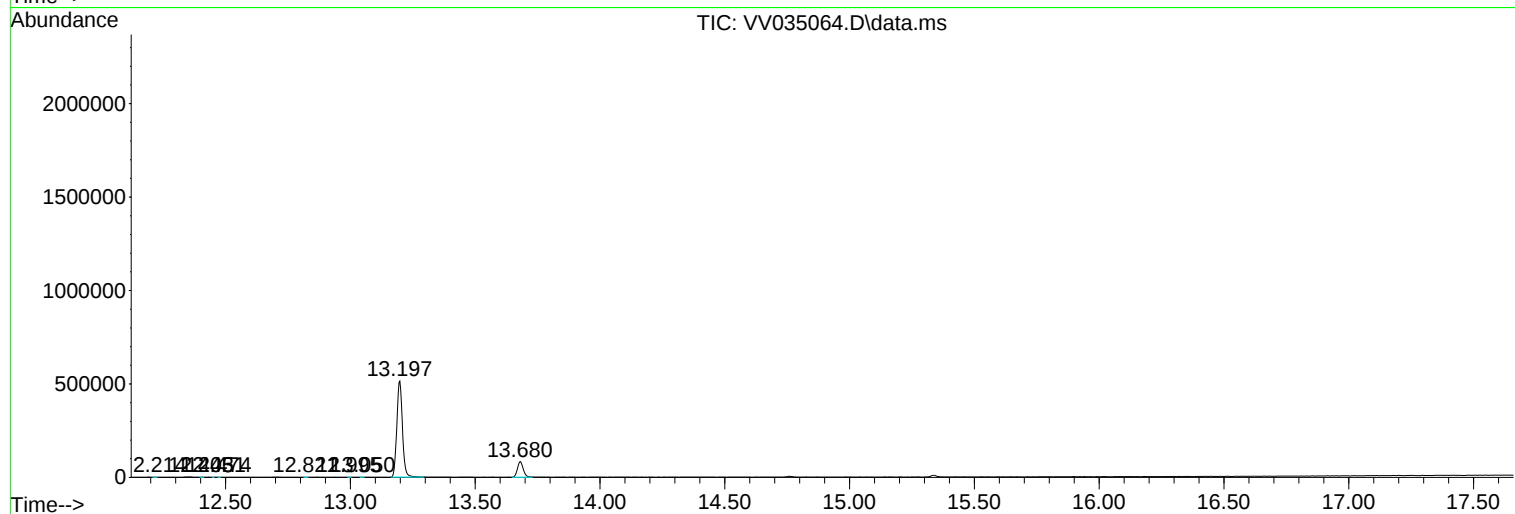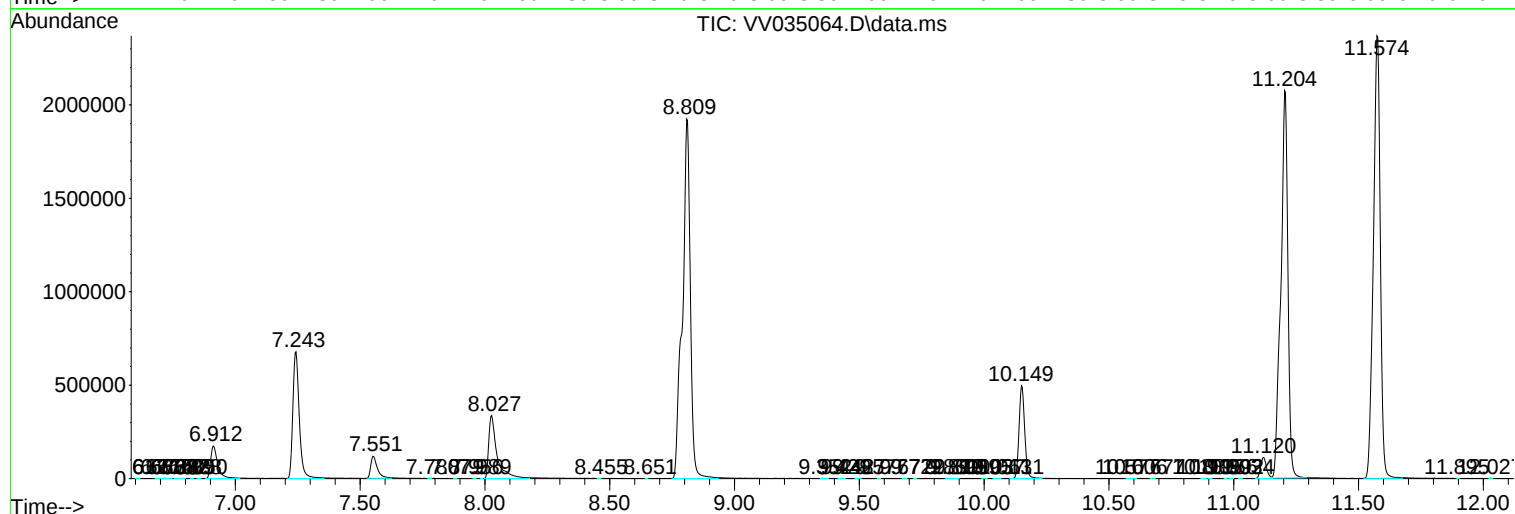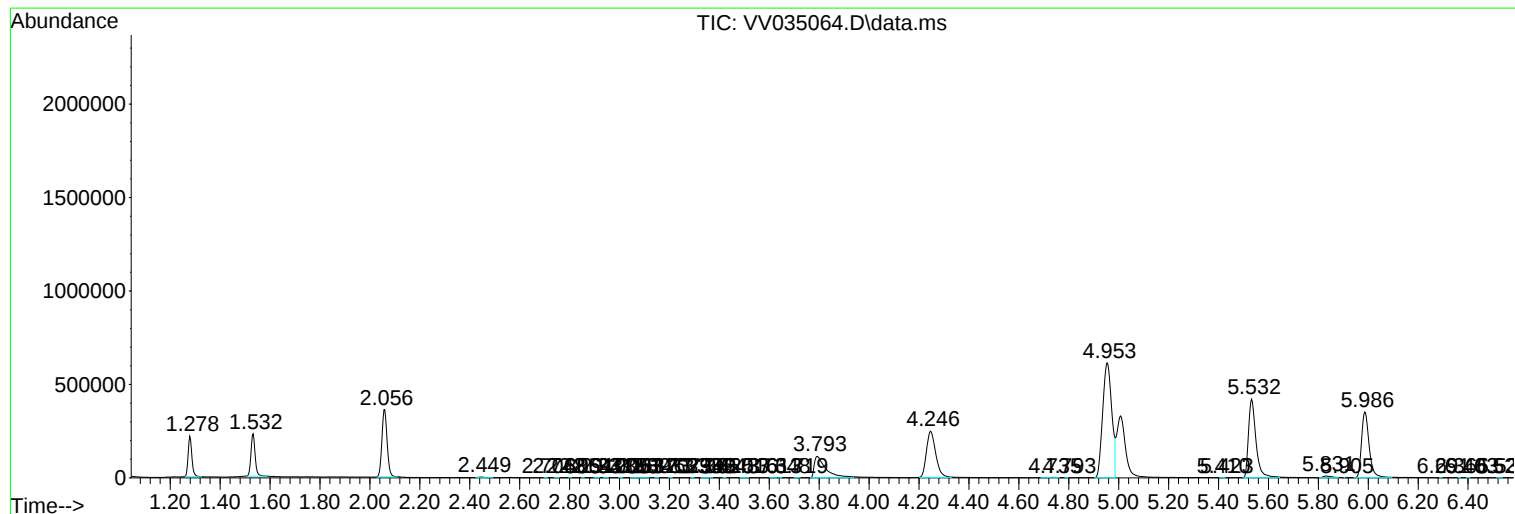

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035064.D
Acq On : 08 Apr 2024 19:03
Operator : SY/MD
Sample : P2006-11DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035064.D
Acq On : 08 Apr 2024 19:03
Operator : SY/MD
Sample : P2006-11DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc