

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035065.D
 Acq On : 08 Apr 2024 19:27
 Operator : SY/MD
 Sample : P2006-10DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	219027	232869	3.03%	0.854%
2	1.532	146	153	167	rBV	227289	253647	3.30%	0.930%
3	2.056	307	316	337	rVB	372409	550693	7.17%	2.019%
4	2.378	413	416	418	rBV	491	346	0.00%	0.001%
5	2.677	507	509	510	rBV	265	100	0.00%	0.000%
6	2.757	532	534	537	rVB2	474	251	0.00%	0.001%
7	2.773	537	539	542	rBV2	524	341	0.00%	0.001%
8	2.876	567	571	572	rBV3	359	279	0.00%	0.001%
9	2.899	575	578	579	rBV3	257	132	0.00%	0.000%
10	2.921	583	585	586	rBV	294	129	0.00%	0.000%
11	3.018	612	615	617	rBV3	395	280	0.00%	0.001%
12	3.101	637	641	642	rBV	364	277	0.00%	0.001%
13	3.166	659	661	665	rBV3	533	248	0.00%	0.001%
14	3.236	679	683	684	rBV	357	192	0.00%	0.001%
15	3.281	695	697	699	rBV2	399	222	0.00%	0.001%
16	3.323	708	710	714	rVB3	202	113	0.00%	0.000%
17	3.346	714	717	722	rVB2	190	115	0.00%	0.000%
18	3.371	722	725	728	rBV	230	229	0.00%	0.001%
19	3.404	733	735	737	rBV	159	103	0.00%	0.000%
20	3.477	755	758	761	rBV2	323	255	0.00%	0.001%
21	3.490	761	762	763	rVB	243	56	0.00%	0.000%
22	3.526	772	773	774	rBV	139	45	0.00%	0.000%
23	3.548	778	780	781	rBV	255	86	0.00%	0.000%
24	3.584	788	791	792	rBV	192	105	0.00%	0.000%
25	3.619	801	802	803	rBV	116	28	0.00%	0.000%
26	3.632	804	806	808	rBV	186	61	0.00%	0.000%
27	3.664	809	816	818	rBV3	1267	1393	0.02%	0.005%
28	3.715	830	832	833	rVB	226	77	0.00%	0.000%
29	3.725	833	835	838	rBV3	176	109	0.00%	0.000%
30	3.764	843	847	848	rBV	418	256	0.00%	0.001%
31	3.796	848	857	907	rBV	113709	375137	4.89%	1.375%
32	4.246	981	997	1032	rBV	251525	654216	8.52%	2.398%
33	4.651	1121	1123	1126	rBV	462	203	0.00%	0.001%
34	4.738	1137	1150	1164	rVB5	4155	10300	0.13%	0.038%
35	4.838	1179	1181	1185	rBV3	280	175	0.00%	0.001%
36	4.953	1201	1217	1226	rBV2	626047	1583436	20.62%	5.805%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035065.D
 Acq On : 08 Apr 2024 19:27
 Operator : SY/MD
 Sample : P2006-10DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1426	rBV	434596	903916	11.77%	3.314%
38	5.834	1481	1491	1510	rBV6	8506	19044	0.25%	0.070%
39	5.985	1522	1538	1570	rBV	360747	753131	9.81%	2.761%
40	6.307	1636	1638	1644	rVB4	416	311	0.00%	0.001%
41	6.358	1651	1654	1655	rBV2	353	145	0.00%	0.001%
42	6.416	1670	1672	1676	rBV2	231	153	0.00%	0.001%
43	6.439	1677	1679	1680	rBV	248	74	0.00%	0.000%
44	6.510	1700	1701	1703	rBV2	168	85	0.00%	0.000%
45	6.535	1706	1709	1712	rVB2	211	133	0.00%	0.000%
46	6.567	1718	1719	1723	rVB	383	177	0.00%	0.001%
47	6.590	1723	1726	1730	rVB4	515	327	0.00%	0.001%
48	6.616	1730	1734	1735	rBV2	621	425	0.01%	0.002%
49	6.686	1752	1756	1761	rBV3	767	761	0.01%	0.003%
50	6.751	1772	1776	1779	rBV3	801	636	0.01%	0.002%
51	6.805	1790	1793	1797	rVB2	298	248	0.00%	0.001%
52	6.854	1805	1808	1811	rBV2	315	228	0.00%	0.001%
53	6.911	1816	1826	1851	rBV	177967	343365	4.47%	1.259%
54	7.243	1918	1929	1961	rBV	690967	1231365	16.04%	4.514%
55	7.551	2015	2025	2056	rBV	119671	233241	3.04%	0.855%
56	7.776	2093	2095	2101	rVV5	488	418	0.01%	0.002%
57	7.815	2104	2107	2111	rVV3	583	436	0.01%	0.002%
58	7.837	2112	2114	2119	rVB4	764	575	0.01%	0.002%
59	7.866	2119	2123	2129	rBV6	662	679	0.01%	0.002%
60	8.027	2164	2173	2212	rBV2	344035	772567	10.06%	2.832%
61	8.632	2359	2361	2362	rBV	311	92	0.00%	0.000%
62	8.670	2371	2373	2374	rVB	377	109	0.00%	0.000%
63	8.808	2397	2416	2451	rBV2	4065024	7678875	100.00%	28.149%
64	9.506	2631	2633	2637	rVB5	647	394	0.01%	0.001%
65	9.632	2670	2672	2674	rBV	183	108	0.00%	0.000%
66	9.648	2674	2677	2679	rBV3	377	244	0.00%	0.001%
67	9.661	2679	2681	2683	rBV2	354	176	0.00%	0.001%
68	9.712	2694	2697	2699	rBV	271	129	0.00%	0.000%
69	9.738	2701	2705	2708	rBV2	361	326	0.00%	0.001%
70	9.770	2713	2715	2716	rBV2	362	124	0.00%	0.000%
71	9.808	2724	2727	2732	rBV3	346	325	0.00%	0.001%
72	9.847	2736	2739	2742	rVV2	329	205	0.00%	0.001%
73	9.902	2754	2756	2760	rBV2	294	205	0.00%	0.001%
74	9.992	2782	2784	2785	rBV2	126	34	0.00%	0.000%
75	10.014	2790	2791	2792	rVB2	209	40	0.00%	0.000%
76	10.149	2821	2833	2858	rBV	492660	787276	10.25%	2.886%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035065.D
 Acq On : 08 Apr 2024 19:27
 Operator : SY/MD
 Sample : P2006-10DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.352	2895	2896	2899	rVB	559	175	0.00%	0.001%
78	10.496	2937	2941	2942	rBV	263	195	0.00%	0.001%
79	10.570	2956	2964	2967	rBV4	694	964	0.01%	0.004%
80	10.590	2967	2970	2972	rVV	204	159	0.00%	0.001%
81	10.622	2976	2980	2981	rBV2	320	267	0.00%	0.001%
82	10.773	3024	3027	3029	rVB	638	375	0.00%	0.001%
83	10.789	3029	3032	3038	rVB4	583	399	0.01%	0.001%
84	10.943	3075	3080	3084	rBV3	333	381	0.00%	0.001%
85	10.963	3084	3086	3090	rVV2	213	168	0.00%	0.001%
86	11.005	3096	3099	3101	rBV2	347	192	0.00%	0.001%
87	11.056	3110	3115	3118	rBV	383	414	0.01%	0.002%
88	11.117	3123	3134	3145	rBV	261303	411837	5.36%	1.510%
89	11.204	3145	3161	3190	rVB2	2372105	4590050	59.78%	16.826%
90	11.574	3260	3276	3301	rBV2	2508794	4789152	62.37%	17.556%
91	12.349	3511	3517	3526	rBV6	2535	4235	0.06%	0.016%
92	12.506	3563	3566	3568	rBV3	513	353	0.00%	0.001%
93	12.812	3658	3661	3665	rBV2	290	291	0.00%	0.001%
94	13.197	3769	3781	3798	rBV	543774	836889	10.90%	3.068%
95	13.680	3920	3931	3949	rBV	146154	234221	3.05%	0.859%
96	15.336	4440	4446	4454	rBV5	7171	10662	0.14%	0.039%




Sum of corrected areas: 27278985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035065.D
Acq On : 08 Apr 2024 19:27
Operator : SY/MD
Sample : P2006-10DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

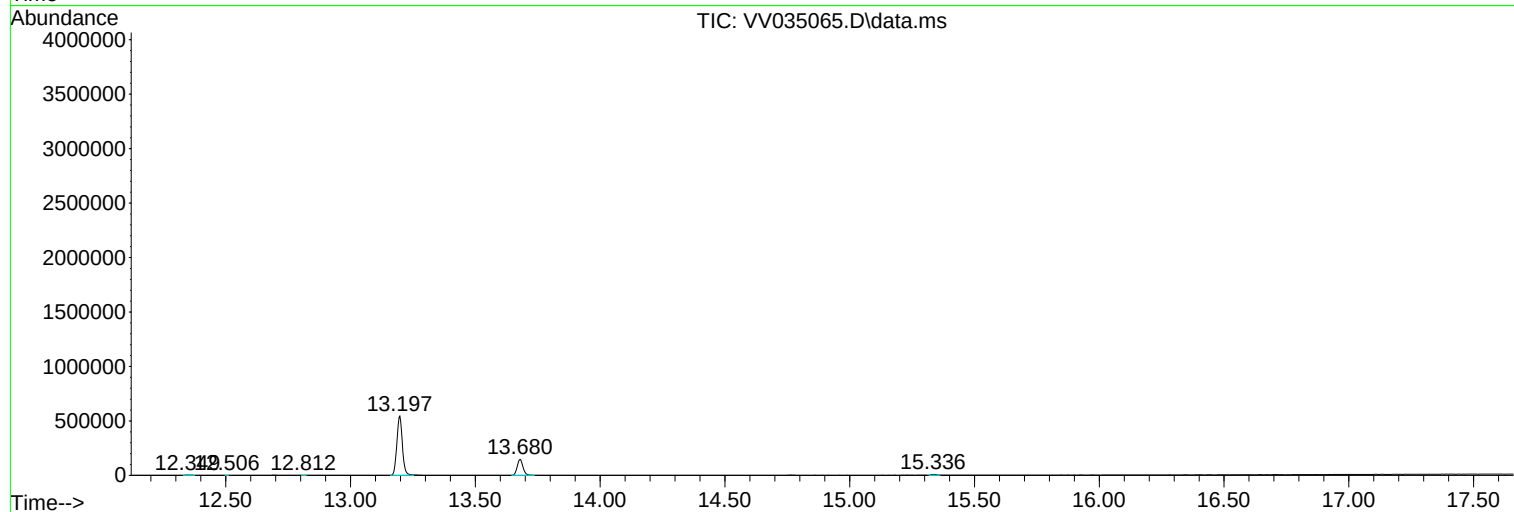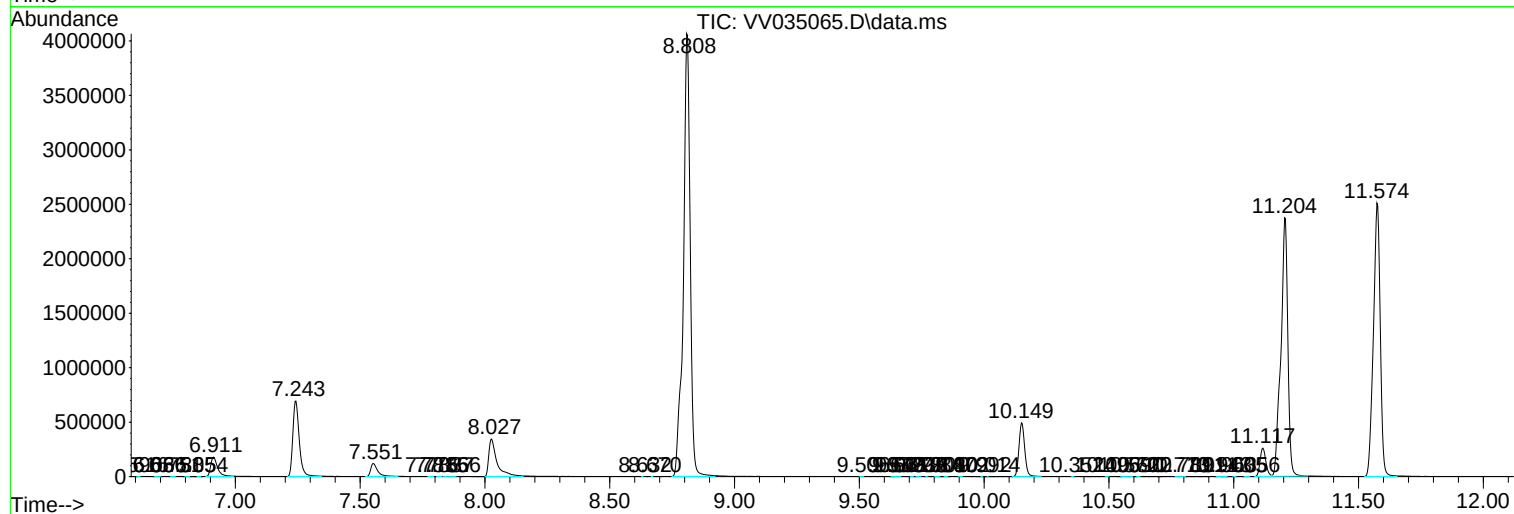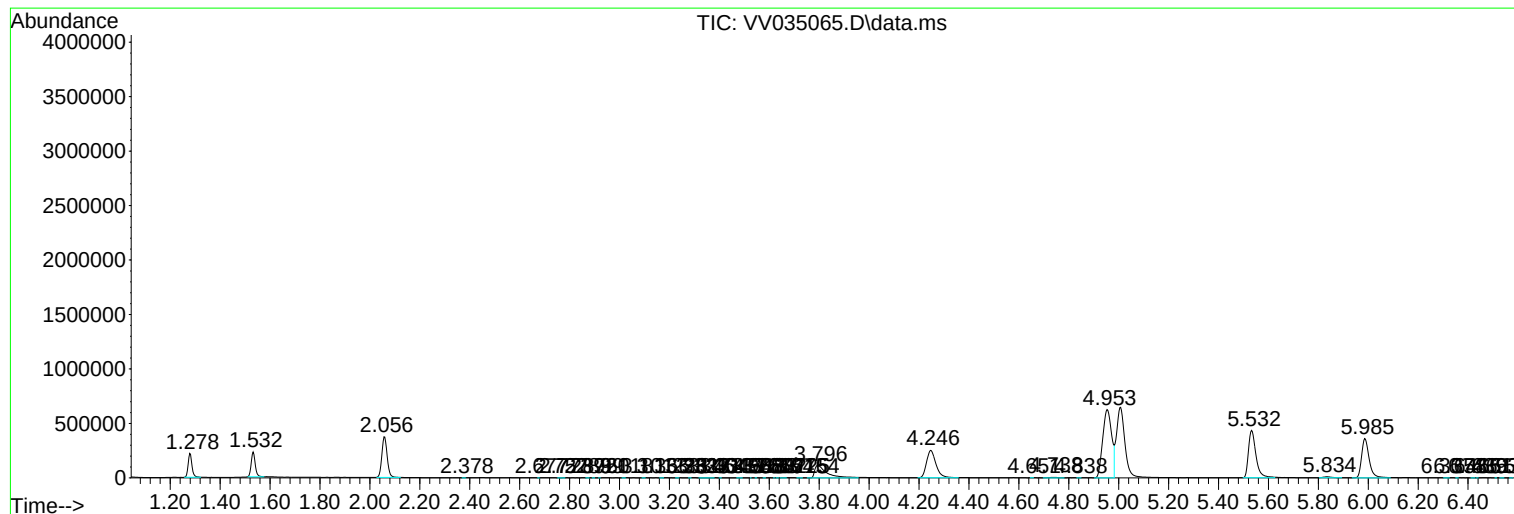

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035065.D
Acq On : 08 Apr 2024 19:27
Operator : SY/MD
Sample : P2006-10DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035065.D
Acq On : 08 Apr 2024 19:27
Operator : SY/MD
Sample : P2006-10DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc