
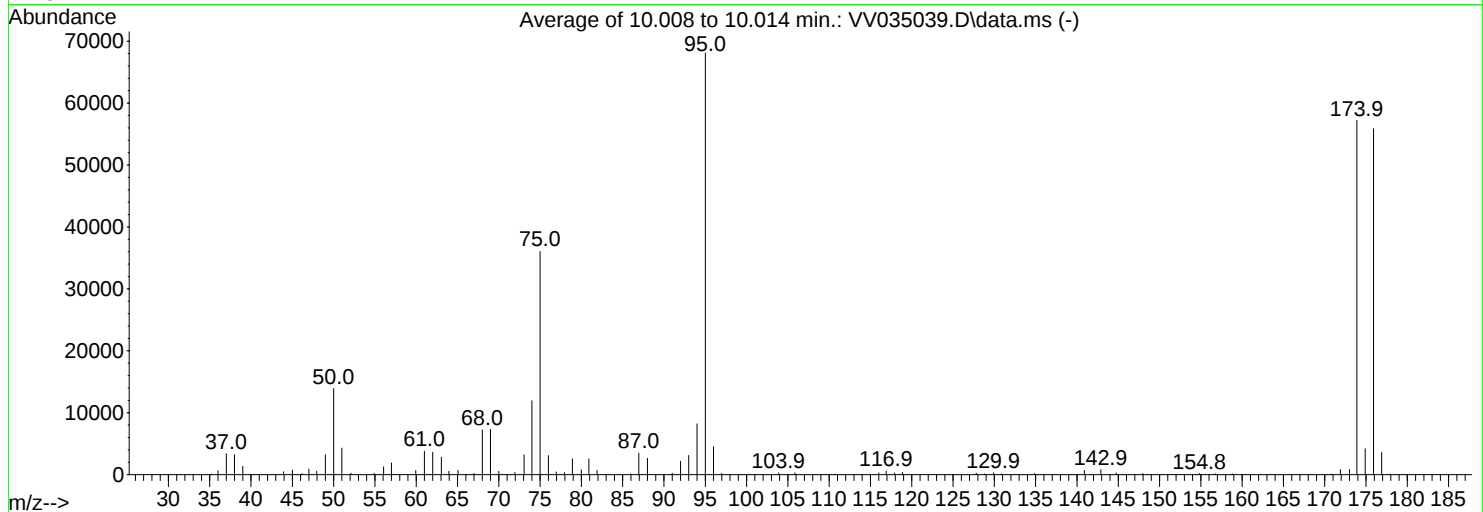


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035039.D
Acq On : 08 Apr 2024 08:17
Operator : SY/MD
Sample : BFB282
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB282

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Wed Apr 10 04:53:36 2024

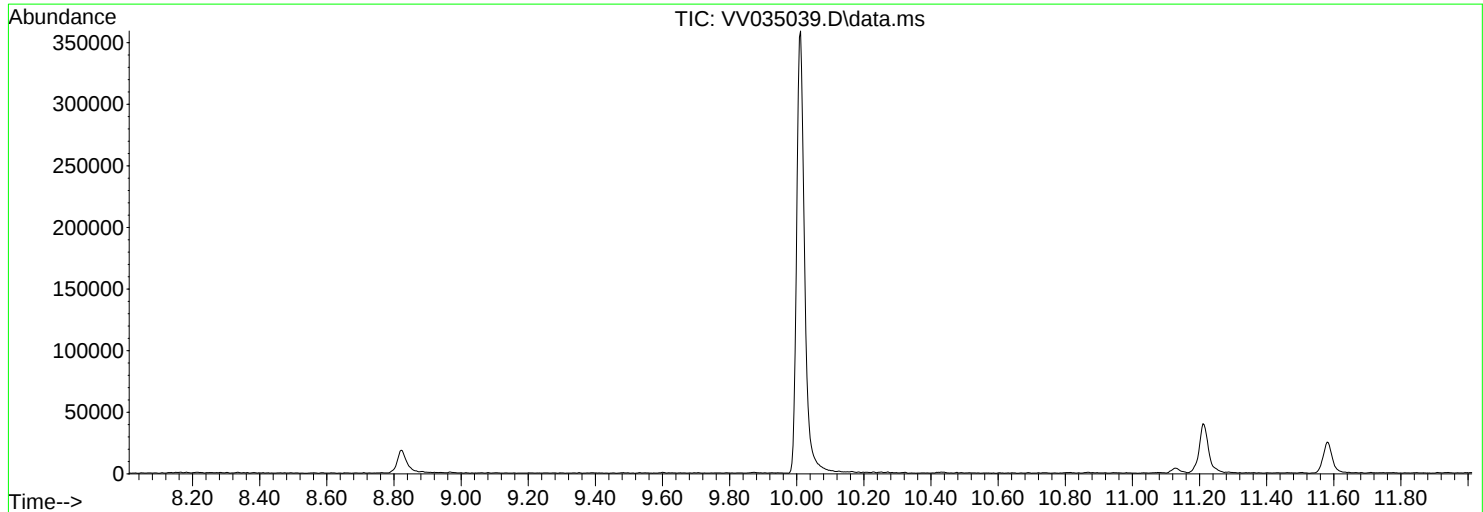

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	13915	PASS
75	95	30	80	52.9	36053	PASS
95	95	100	100	100.0	68117	PASS
96	95	5	9	6.7	4531	PASS
173	174	0.00	2	1.5	835	PASS
174	95	50	120	84.0	57200	PASS
175	174	5	9	7.3	4179	PASS
176	174	95	105	97.7	55864	PASS
177	176	5	10	6.5	3607	PASS

m/z	Abundance
39.90	308.0
43.90	317.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
35.30	117.0
36.00	659.0
37.00	3532.0
38.00	3307.0
39.00	1391.0
40.00	274.0
44.00	814.0
45.00	708.0
46.10	153.0
47.00	937.0
48.00	557.0
49.00	3307.0
50.00	14273.0
51.00	4474.0
52.20	219.0
54.90	273.0
56.00	1314.0
57.00	2082.0
60.00	647.0
61.00	3879.0
62.00	3673.0
63.00	2915.0
64.00	504.0
65.10	830.0
66.10	135.0
67.00	244.0
68.00	7508.0
69.00	7810.0
70.00	590.0
71.90	366.0
73.10	3313.0
74.00	12070.0
75.00	36888.0
76.00	3203.0
77.00	517.0
78.00	331.0
78.90	2620.0
80.00	758.0
80.90	2622.0
81.90	739.0
83.00	104.0
86.00	129.0
87.00	3486.0
88.00	2730.0
91.00	281.0
92.00	2254.0
93.00	3092.0
94.00	8587.0
95.00	70088.0
96.00	4754.0
97.00	175.0
103.90	298.0
105.80	272.0
114.90	101.0
116.00	298.0
116.90	578.0
117.90	279.0
118.80	314.0
127.80	244.0
128.80	125.0
129.90	313.0
130.90	133.0
134.80	176.0
140.90	705.0
141.90	125.0
142.90	851.0
144.80	279.0
145.90	125.0
148.00	166.0
154.80	173.0
156.70	129.0
158.90	140.0
170.80	113.0
171.90	655.0
173.00	790.0
173.90	57144.0
174.90	4222.0
175.90	55776.0
176.90	3590.0
177.80	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
35.20	110.0
36.00	659.0
37.00	3461.0
38.00	3336.0
39.00	1396.0
40.00	384.0
44.00	790.0
45.00	741.0
46.10	167.0
47.00	894.0
48.00	589.0
49.00	3327.0
50.00	14211.0
51.00	4424.0
52.10	249.0
54.90	219.0
56.00	1332.0
57.00	1941.0
59.90	681.0
61.00	3942.0
62.00	3714.0
63.10	2919.0
63.90	575.0
65.00	714.0
66.10	134.0
67.00	217.0
68.00	7448.0
69.00	7472.0
70.00	549.0
71.90	367.0
73.00	3303.0
74.00	12322.0
75.00	37328.0
76.00	3159.0
76.90	443.0
77.90	336.0
78.90	2638.0
80.00	787.0
80.90	2677.0
81.90	693.0
85.90	126.0
86.90	3584.0
88.00	2664.0
91.10	234.0
92.00	2297.0
93.00	3173.0
94.00	8467.0
95.00	70320.0
96.00	4727.0
97.00	164.0
103.90	281.0
105.90	291.0
110.70	102.0
114.90	103.0
116.00	295.0
116.90	624.0
117.90	284.0
118.80	373.0
127.80	232.0
128.80	122.0
129.90	293.0
130.80	132.0
134.80	178.0
140.90	699.0
141.80	122.0
142.90	819.0
144.70	276.0
145.80	101.0
148.00	183.0
154.80	198.0
156.70	124.0
158.80	121.0
170.90	116.0
171.90	840.0
173.00	880.0
173.90	59200.0
174.90	4300.0
175.90	57976.0
176.90	3728.0
177.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
36.00	653.0
37.00	3183.0
38.00	2992.0
39.00	1255.0
40.00	431.0
41.00	102.0
44.00	739.0
45.00	699.0
46.20	127.0
47.00	772.0
47.90	491.0
49.00	3017.0
50.00	13260.0
51.00	3964.0
52.00	243.0
52.90	102.0
54.90	213.0
56.10	1145.0
57.00	1658.0
59.90	734.0
61.00	3503.0
62.00	3493.0
63.10	2595.0
63.90	535.0
65.00	560.0
67.00	175.0
68.00	6729.0
69.00	6671.0
70.00	479.0
72.00	386.0
73.00	3038.0
74.00	11409.0
75.00	33944.0
76.00	2863.0
76.90	384.0
77.90	308.0
78.90	2422.0
80.00	747.0
80.90	2414.0
81.90	592.0
85.90	141.0
86.90	3318.0
88.00	2498.0
90.90	212.0
92.00	1980.0
93.00	3026.0
94.00	7582.0
95.00	63944.0
96.00	4113.0
96.90	182.0
103.90	290.0
105.90	278.0
110.70	114.0
116.00	245.0
116.90	547.0
117.90	263.0
118.90	436.0
127.80	239.0
128.80	138.0
129.90	257.0
130.80	101.0
134.90	161.0
140.90	606.0
142.90	757.0
144.70	230.0
147.90	160.0
154.90	198.0
156.80	126.0
158.70	124.0
171.90	885.0
173.00	836.0
173.90	55256.0
174.90	4016.0
175.90	53840.0
176.90	3503.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282