

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040920\
 Data File : VV015420.D
 Acq On : 09 Apr 2020 15:31
 Operator : SY/MD
 Sample : L2216-06
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y12

Manual Integrations
 APPROVED

apatel
 4/10/2020 11:13:24 AM

Quant Time: Apr 10 05:02:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 10 04:24:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	125224	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	118602	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	57308	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	29259	4.50	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.00%
7) Chloroethane-d5	1.57	69	26935	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.00%
11) 1,1-Dichloroethene-d2	2.12	63	43408	3.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.40%
20) 2-Butanone-d5	3.96	46	86083	47.19	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.38%
24) Chloroform-d	4.38	84	66102	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
26) 1,2-Dichloroethane-d4	5.06	65	37259	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
32) Benzene-d6	5.07	84	125827	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.10	67	40051	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	7.34	98	113816	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.64	79	16152	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
46) 2-Hexanone-d5	8.12	63	83244	48.43	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.86%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	30314	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
64) 1,2-Dichlorobenzene-d4	11.65	152	44279	4.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.20%

Target Compounds				Ovalue
13) Acetone	2.24	43	8105m	6.288 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040920\
Data File : VV015420.D
Acq On : 09 Apr 2020 15:31
Operator : SY/MD
Sample : L2216-06
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0Y12

Manual Integrations
APPROVED

apatel
4/10/2020 11:13:24 AM

Quant Time: Apr 10 05:02:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 10 04:24:06 2020
Response via : Initial Calibration

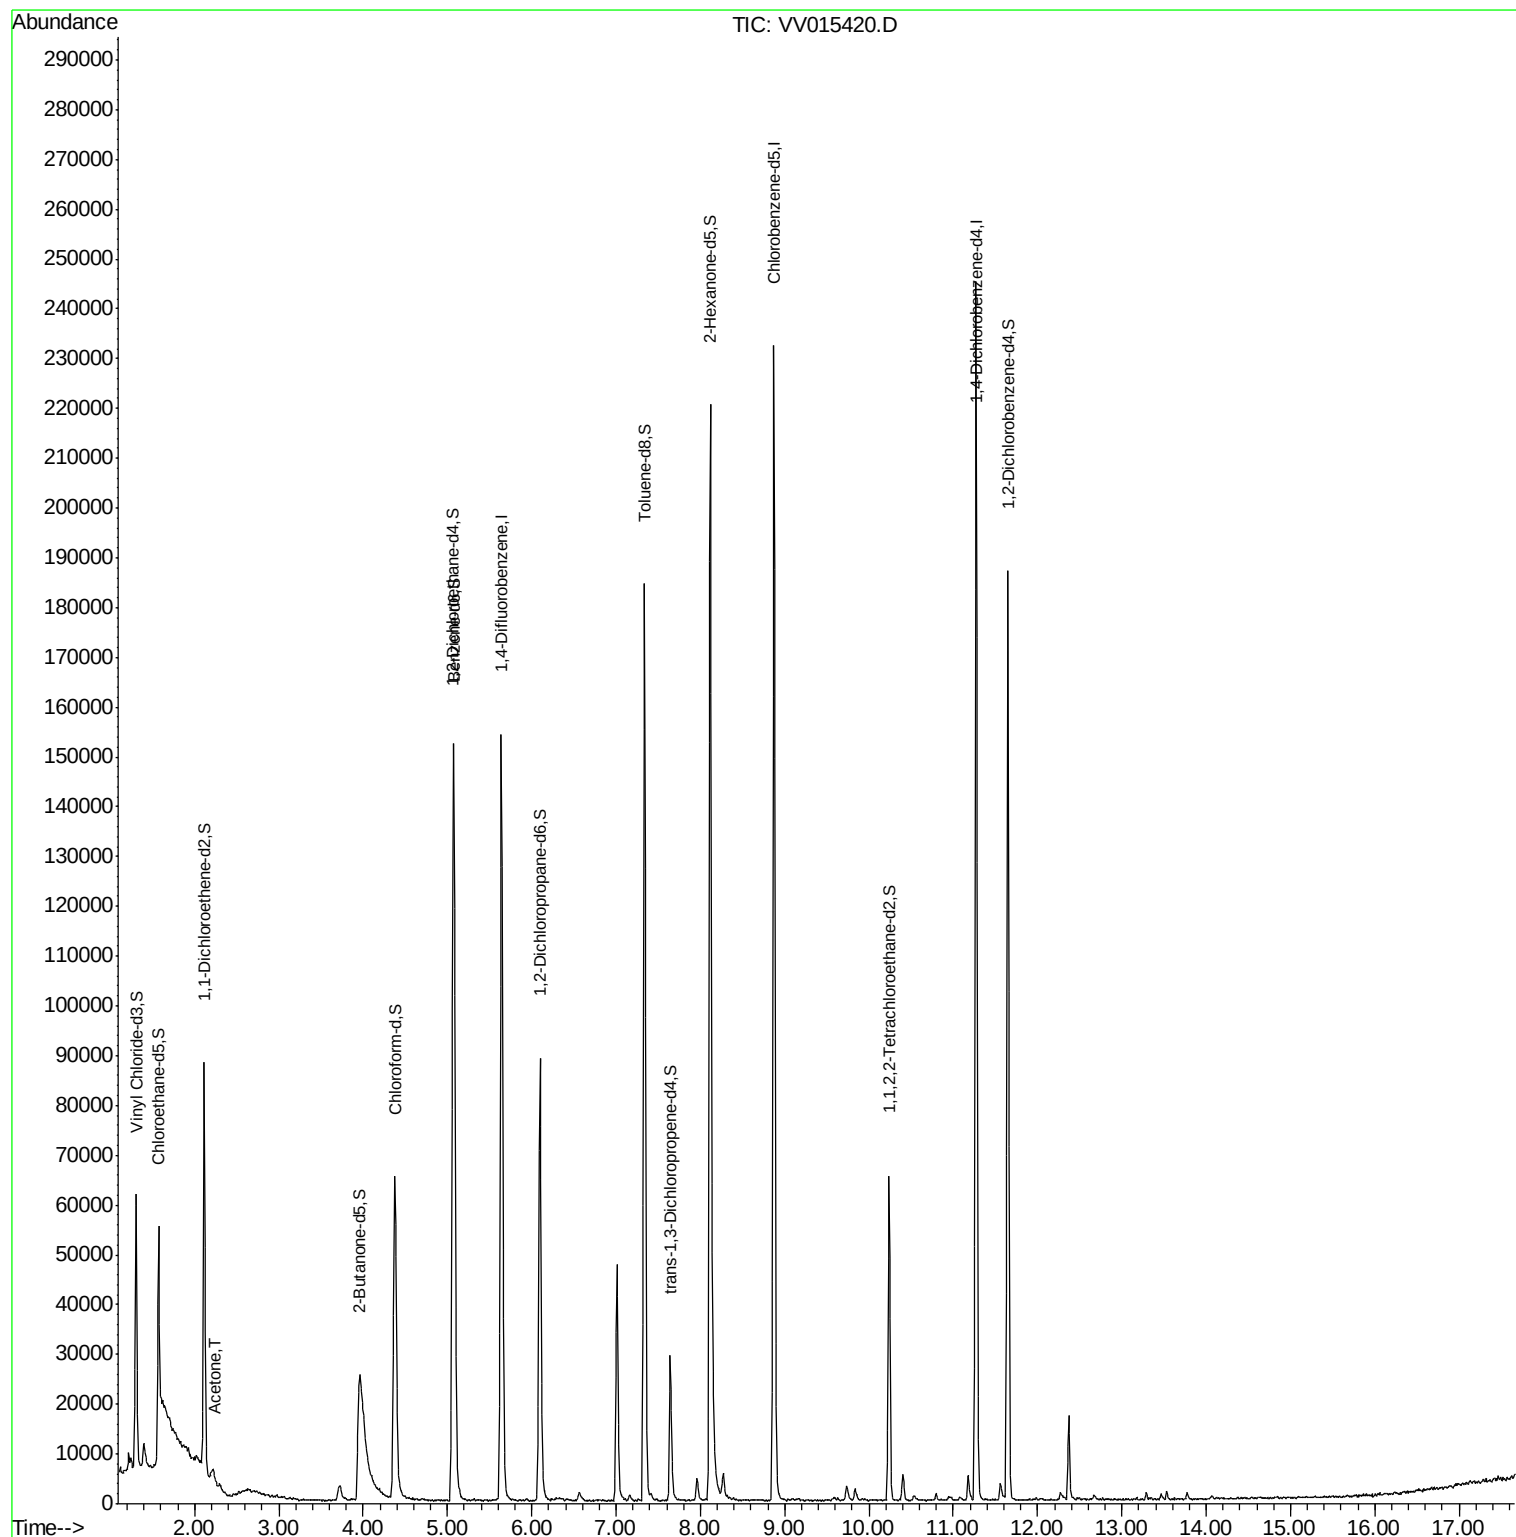

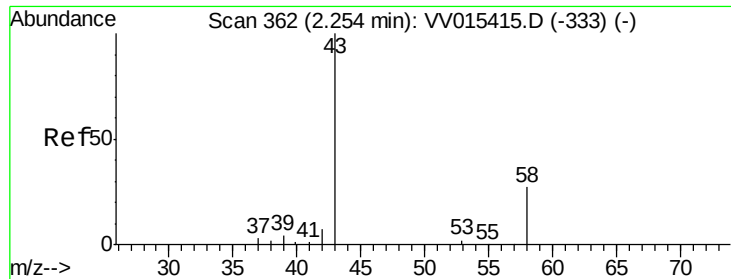

#13

Acetone

Concen: 6.288 ug/L m

RT: 2.24 min Scan# 359

Delta R.T. -0.01 min

Lab File: VV015420.D

Acq: 09 Apr 2020 15:31

Tot Ion: 43 Resp: 8105

Ion Ratio Lower Upper

43 100

58 4.4 0.0 22.2

Instrument :

MSVOA_V

ClientSampleId :

C0Y12

Manual Integrations

APPROVED

apatel

4/10/2020 11:13:24 AM

