

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040920\
 Data File : VV015421.D
 Acq On : 09 Apr 2020 15:55
 Operator : SY/MD
 Sample : L2216-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0Y13

Quant Time: Apr 10 05:07:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 10 04:24:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	122082	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	116372	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	56846	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	30727	4.85	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.00%
7) Chloroethane-d5	1.58	69	28243	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.80%
11) 1,1-Dichloroethene-d2	2.12	63	45269	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	3.94	46	103676	58.29	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.58%
24) Chloroform-d	4.38	84	67365	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.06	65	39208	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.80%
32) Benzene-d6	5.08	84	130184	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.10	67	41722	5.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.80%
41) Toluene-d8	7.34	98	120023	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
43) trans-1,3-Dichloropropene-	7.64	79	17249	4.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.60%
46) 2-Hexanone-d5	8.11	63	83988	49.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.60%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	31195	4.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	45471	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%


Target Compounds					Ovalue
13) Acetone	2.23	43	6985	5.559 ug/L	# 50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV040920\
Data File : VV015421.D
Acq On : 09 Apr 2020 15:55
Operator : SY/MD
Sample : L2216-07
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0Y13

Quant Time: Apr 10 05:07:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 10 04:24:06 2020
Response via : Initial Calibration

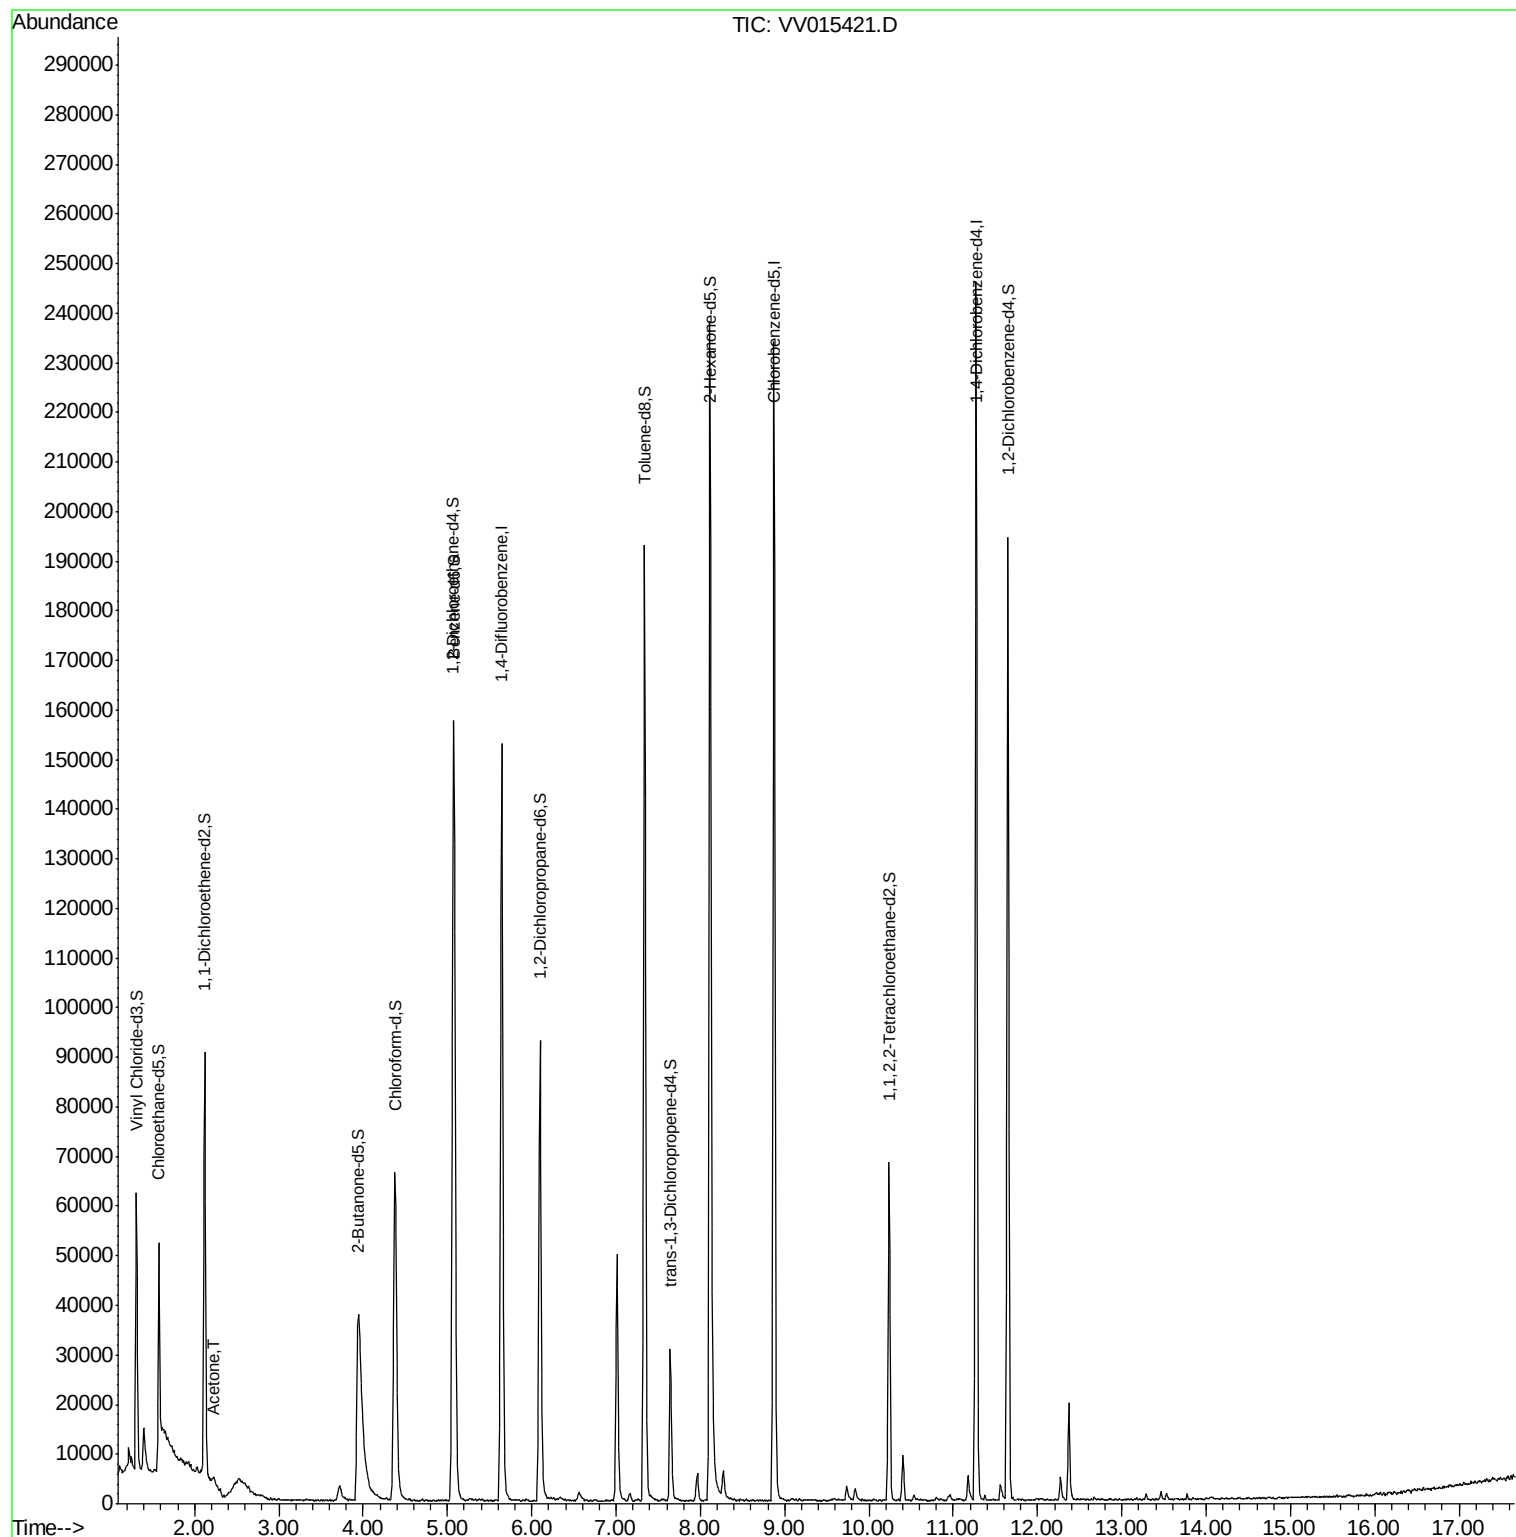

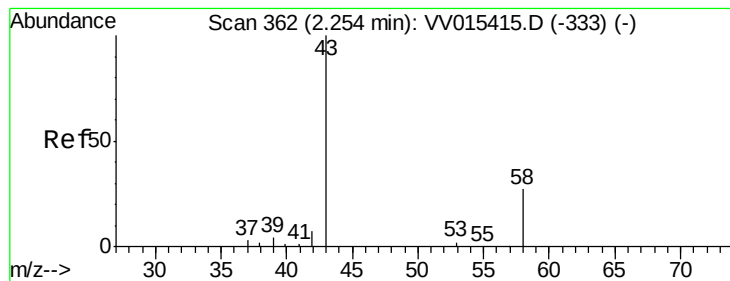

#13

Acetone

Concen: 5.559 ug/L

RT: 2.23 min Scan# 354

Delta R.T. -0.03 min

Lab File: VV015421.D

Acq: 09 Apr 2020 15:55

Instrument :
MSVOA_V
ClientSampleId :
C0Y13

Tot Ion: 43 Resp: 6985

Ion Ratio Lower Upper

43 100

58 30.0 0.0 22.2#

