


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV040920\
 Data File : VV015412.D
 Acq On : 09 Apr 2020 08:52
 Operator : SY/MD
 Sample : BFB32
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB32

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Apr 10 05:37:21 2020

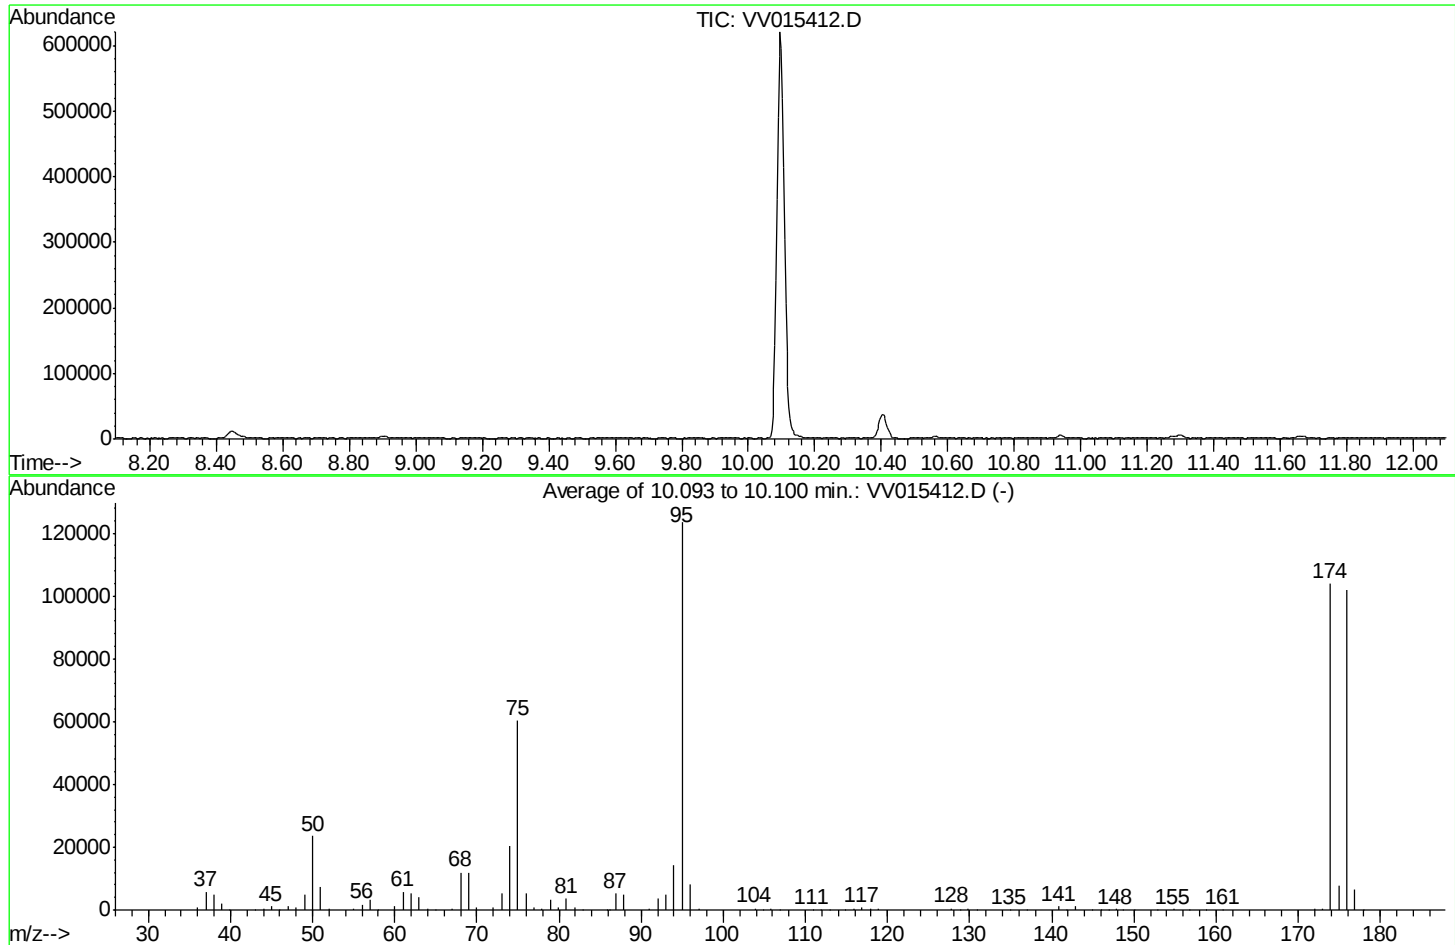

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	23538	PASS
75	95	30	80	48.8	60224	PASS
95	95	100	100	100.0	123445	PASS
96	95	5	9	6.6	8106	PASS
173	174	0.00	2	0.3	323	PASS
174	95	50	120	84.1	103861	PASS
175	174	5	9	7.5	7781	PASS
176	174	95	101	98.0	101832	PASS
177	176	5	9	6.5	6646	PASS

m/z	Abundance
36.00	983.0
37.00	5883.0
38.00	4864.0
39.00	2141.0
39.90	460.0
42.90	136.0
44.00	1187.0
45.00	1125.0
46.00	158.0
47.00	1333.0
47.90	710.0
49.00	4881.0
50.00	23008.0
51.00	7054.0
51.90	365.0
55.00	313.0
56.00	1761.0
57.00	3098.0
58.00	161.0
60.00	1038.0
61.00	5611.0
62.00	5466.0
63.00	4197.0
64.00	390.0
65.00	210.0
66.90	312.0
68.00	11663.0
69.00	11728.0
70.00	897.0
72.00	726.0
73.00	5261.0
74.00	20064.0
75.00	58720.0
76.00	5411.0
76.90	695.0
77.80	564.0
78.90	3198.0
79.90	971.0
80.90	3393.0
81.90	620.0
82.90	118.0
85.90	118.0
86.90	5135.0
87.90	4761.0
91.00	378.0
92.00	3571.0
93.00	4966.0
94.00	13990.0
95.00	120504.0
96.00	8216.0
97.00	264.0
103.90	476.0
104.90	166.0
105.80	498.0
106.80	106.0
112.90	103.0
114.80	132.0
115.90	464.0
116.80	701.0
117.90	409.0
118.80	618.0
127.80	412.0
128.80	181.0
129.80	413.0
130.80	183.0
134.90	216.0
137.00	173.0
140.90	1181.0
141.80	139.0
142.90	1082.0
144.90	134.0
145.90	142.0
146.90	105.0
147.80	261.0
152.80	110.0
154.80	301.0
156.80	199.0
158.80	169.0
160.80	138.0
172.10	303.0
173.00	969.0
173.90	98712.0
174.90	7473.0
175.90	97200.0
176.90	6308.0
177.90	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
36.00	1039.0
37.00	6019.0
38.00	5003.0
39.00	2237.0
39.90	491.0
43.00	126.0
44.00	1236.0
45.00	1230.0
46.00	167.0
47.00	1444.0
47.90	659.0
49.00	4968.0
50.00	24464.0
51.00	7593.0
52.00	353.0
55.00	317.0
56.00	1823.0
57.00	3240.0
58.00	132.0
60.00	1088.0
61.00	6063.0
62.00	5557.0
63.00	4261.0
64.00	435.0
65.00	198.0
66.90	309.0
68.00	12473.0
69.00	12175.0
70.00	948.0
71.90	717.0
73.00	5506.0
74.00	21112.0
75.00	62296.0
76.00	5537.0
76.90	714.0
77.80	600.0
78.90	3410.0
79.90	1051.0
80.90	3628.0
81.90	685.0
86.10	113.0
86.90	5290.0
87.90	5059.0
91.00	375.0
92.00	3726.0
93.00	5159.0
94.00	14844.0
95.00	128040.0
96.00	8294.0
97.00	260.0
103.90	514.0
104.90	160.0
105.80	492.0
106.80	124.0
110.90	109.0
111.90	102.0
114.80	165.0
115.90	497.0
116.80	714.0
117.90	435.0
118.80	629.0
127.80	454.0
128.90	181.0
129.90	454.0
130.80	188.0
134.90	207.0
136.90	173.0
140.90	1254.0
141.80	163.0
142.90	1142.0
144.90	138.0
146.00	162.0
147.80	272.0
150.00	104.0
152.80	121.0
154.80	331.0
156.80	192.0
158.80	193.0
160.80	131.0
172.10	287.0
173.90	107352.0
174.90	8035.0
175.90	105360.0
176.90	6923.0
177.90	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

m/z	Abundance
36.00	1002.0
37.00	5611.0
38.00	4671.0
39.00	2096.0
39.90	532.0
42.90	126.0
44.00	1160.0
45.00	1176.0
46.00	129.0
47.00	1343.0
47.90	556.0
49.00	4596.0
50.00	23144.0
51.00	7210.0
52.00	320.0
55.00	303.0
56.00	1771.0
57.00	3167.0
57.90	107.0
60.00	1064.0
61.00	5835.0
62.00	5213.0
63.00	4019.0
64.00	446.0
65.00	191.0
66.90	272.0
68.00	11921.0
69.00	11583.0
70.00	923.0
71.90	663.0
73.00	5166.0
74.00	20064.0
75.00	59656.0
76.00	5120.0
76.90	684.0
77.90	564.0
78.90	3188.0
79.90	994.0
80.90	3425.0
81.90	691.0
86.10	109.0
86.90	5019.0
87.90	4840.0
90.90	363.0
92.00	3507.0
93.00	4790.0
94.00	14098.0
95.00	121792.0
96.00	7808.0
97.00	227.0
103.90	506.0
104.80	140.0
105.90	443.0
106.80	142.0
110.80	124.0
114.90	152.0
115.90	473.0
116.90	657.0
117.90	398.0
118.80	574.0
127.80	458.0
128.90	174.0
129.90	434.0
130.80	184.0
134.80	171.0
136.90	179.0
140.90	1184.0
141.80	152.0
142.90	1174.0
144.90	131.0
146.00	143.0
147.80	274.0
148.70	103.0
150.00	109.0
152.80	126.0
154.80	333.0
156.80	201.0
158.80	187.0
160.90	107.0
171.90	246.0
173.90	105520.0
174.90	7837.0
175.90	102936.0
176.90	6708.0
177.90	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32

Scan 2787 (10.051 min): VV015412.D
BFB32

m/z	Abundance
39.90	402.0
44.00	616.0

Instrument :
MSVOA_V
ClientSampleId :
BFB32