

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
 Data File : VV020977.D
 Acq On : 08 Apr 2021 17:47
 Operator : SY/MD
 Sample : VSTD0.132
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Apr 09 07:58:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 09 07:58:08 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	6392	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	6155	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	2670	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	581	0.08	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.066	65	407	0.10	ug/L	0.02
7) 1,2-Dichloropropane-d6	6.092	67	514	0.10	ug/L	0.02
8) Toluene-d8	7.332	98	1059	0.07	ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.216	84	343	0.13	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.310	62	1097	0.15	ug/L #	78
6) Trichloroethene	5.925	95	626	0.12	ug/L	87
9) 1,2-Dibromoethane	8.368	107	343	0.12	ug/L #	93
12) 1,2,3-Trichloropropane	10.267	75	303	0.14	ug/L #	91
13) 1,2-Dibromo-3-chloropr...	12.426	75	37	0.12	ug/L	94




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
Data File : VV020977.D
Acq On : 08 Apr 2021 17:47
Operator : SY/MD
Sample : VSTD0.132
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Apr 09 07:58:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 09 07:58:08 2021
Response via : Initial Calibration




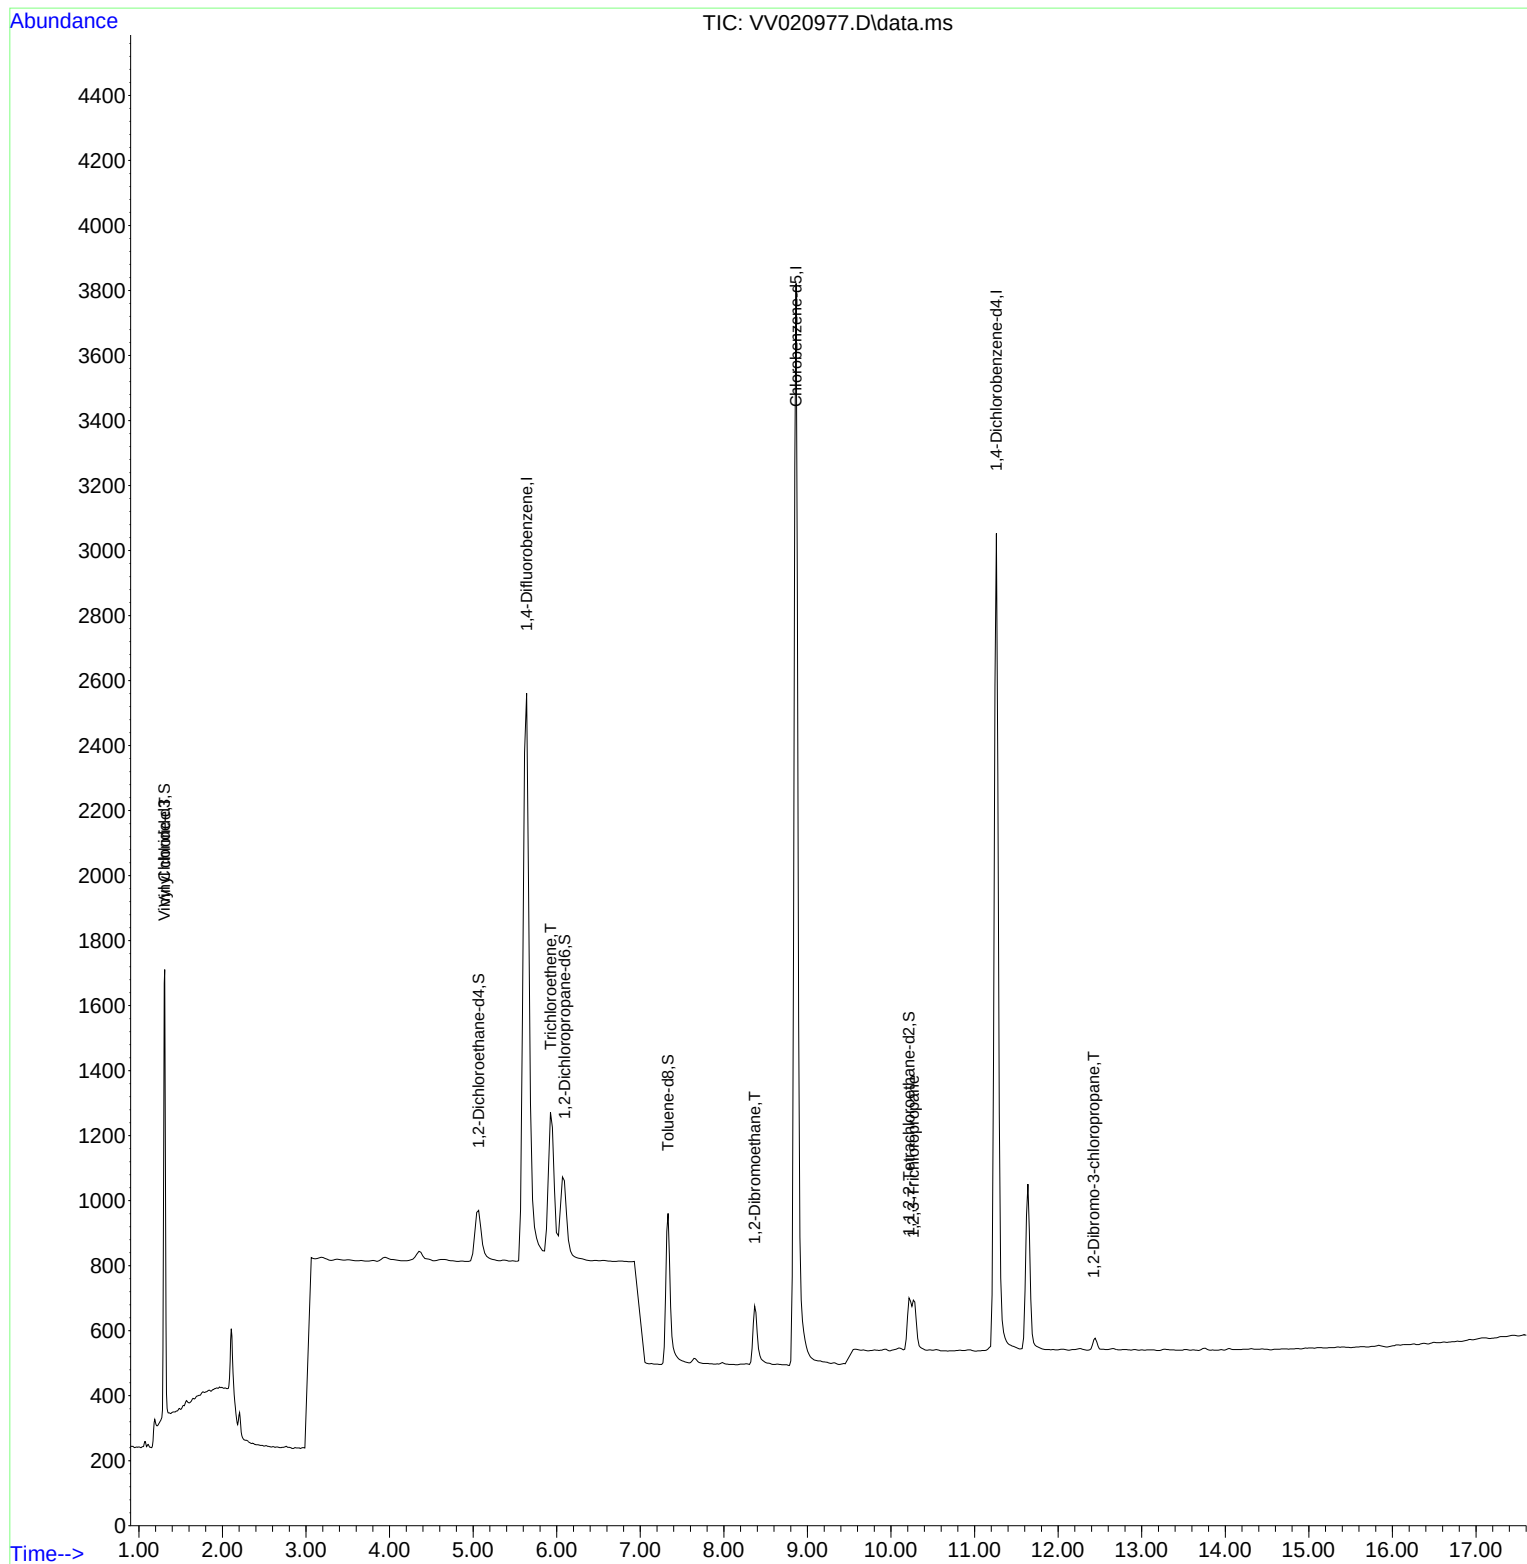


Abundance Scan 59 (1.310 min): VV020978.D\data.ms (-44)

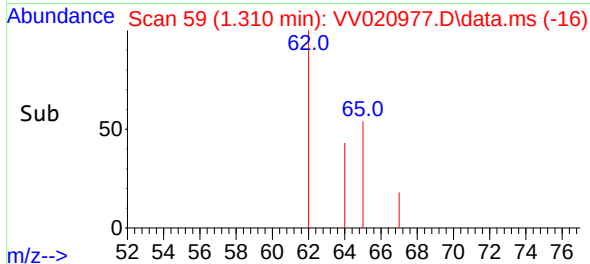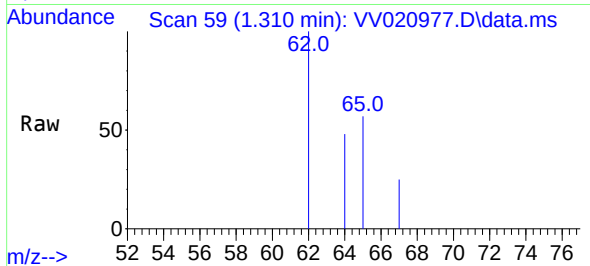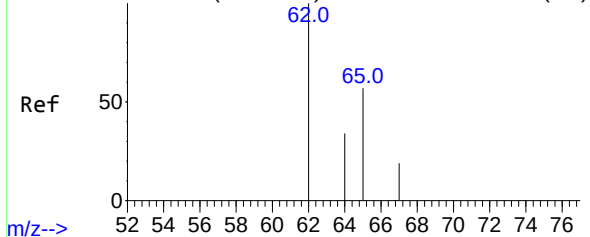


#3
Vinyl chloride
Concen: 0.15 ug/L
RT: 1.310 min Scan# 59
Delta R.T. -0.000 min
Lab File: VV020977.D
Acq: 08 Apr 2021 17:47


Tgt Ion: 62 Resp: 1097
Ion Ratio Lower Upper
62 100
64 47.7 24.3 45.1#

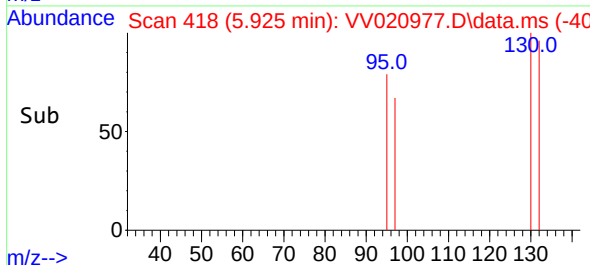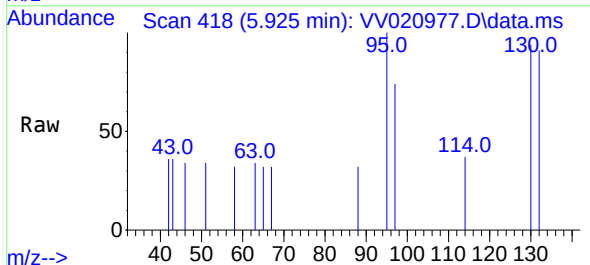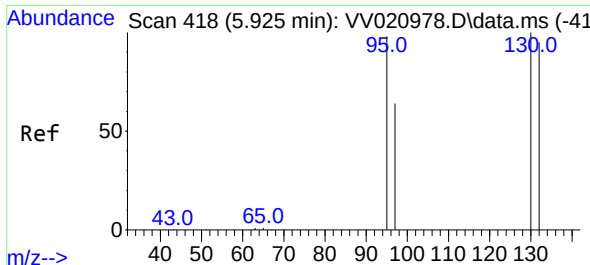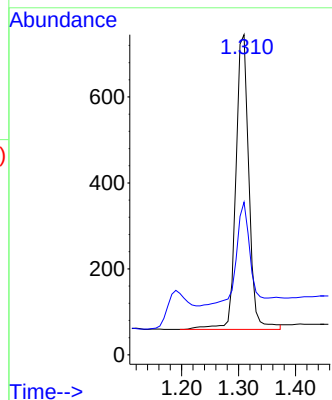

#6
Trichloroethene
Concen: 0.12 ug/L
RT: 5.925 min Scan# 418
Delta R.T. -0.000 min
Lab File: VV020977.D
Acq: 08 Apr 2021 17:47





Tgt Ion: 95 Resp: 626
Ion Ratio Lower Upper
95 100
97 73.6 47.2 87.6
132 91.2 73.6 136.6
130 94.0 77.1 143.3

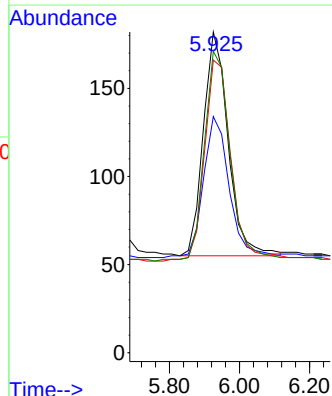

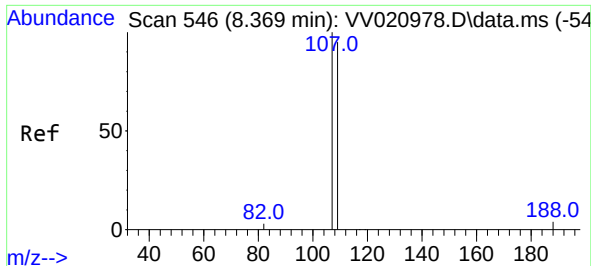




#9
1,2-Dibromoethane
Concen: 0.12 ug/L
RT: 8.368 min Scan# 546
Delta R.T. -0.000 min
Lab File: VV020977.D
Acq: 08 Apr 2021 17:47


Tgt Ion:107 Resp: 343
Ion Ratio Lower Upper
107 100
109 96.5 67.3 125.1
188 37.8 7.8 11.8#

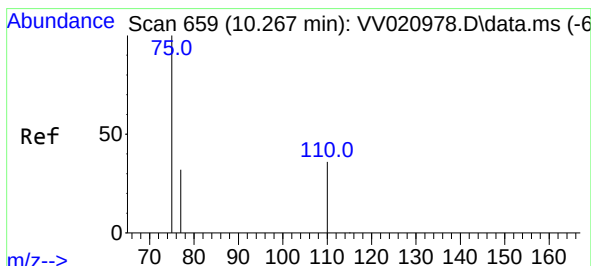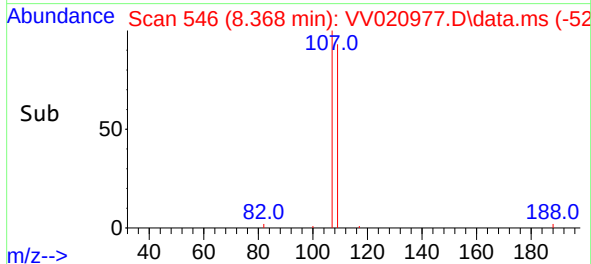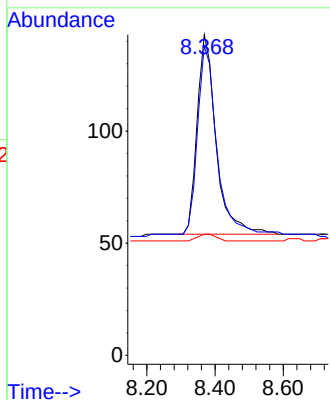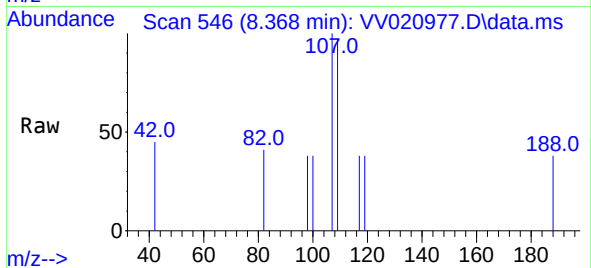

#12
1,2,3-Trichloropropane
Concen: 0.14 ug/L
RT: 10.267 min Scan# 659
Delta R.T. -0.000 min
Lab File: VV020977.D
Acq: 08 Apr 2021 17:47

Tgt Ion: 75 Resp: 303
Ion Ratio Lower Upper
75 100
110 44.9 33.5 50.3
77 39.9 25.4 38.2#

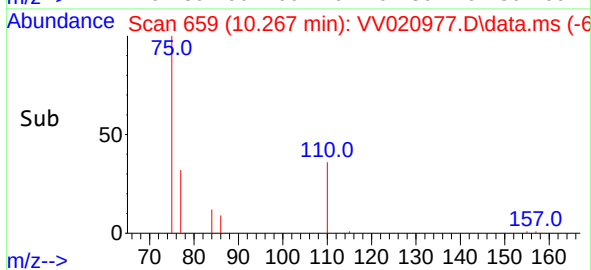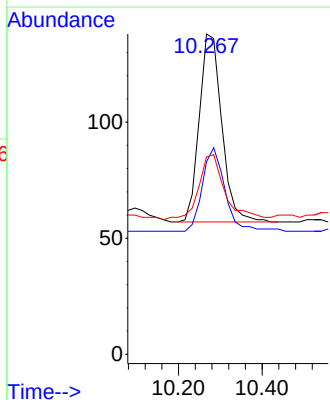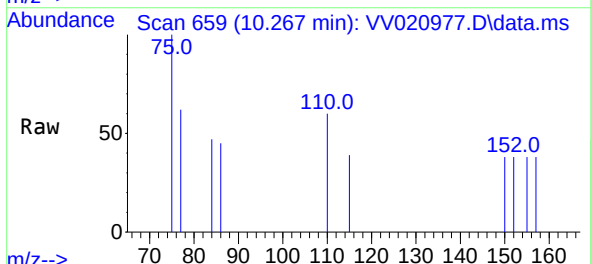

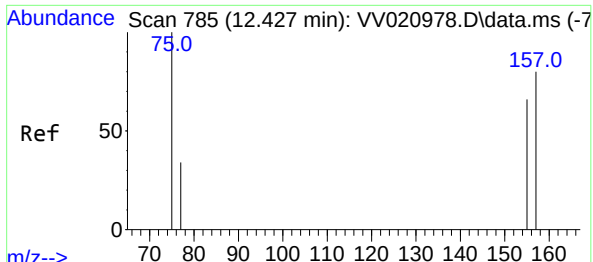

#13
1,2-Dibromo-3-chloropropane
Concen: 0.12 ug/L
RT: 12.426 min Scan# 785
Delta R.T. -0.000 min
Lab File: VV020977.D
Acq: 08 Apr 2021 17:47

Tgt Ion: 75 Resp: 37

Ion	Ratio	Lower	Upper
75	100		
157	88.2	74.3	111.5
155	88.2	65.4	98.2

