

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
 Data File : VV020978.D
 Acq On : 08 Apr 2021 18:10
 Operator : SY/MD
 Sample : VSTD0.533
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Apr 09 07:59:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 09 07:58:08 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	6236	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.864	117	6011	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	2642	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	2971	0.41	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	2145	0.52	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.069	67	2888	0.58	ug/L	0.00
8) Toluene-d8	7.317	98	5578	0.37	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	1762	0.66	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.310	62	5065	0.71	ug/L	97
6) Trichloroethene	5.925	95	2889	0.58	ug/L	93
9) 1,2-Dibromoethane	8.369	107	1673	0.59	ug/L #	98
12) 1,2,3-Trichloropropane	10.267	75	1495	0.67	ug/L	99
13) 1,2-Dibromo-3-chloropr...	12.427	75	198	0.65	ug/L	95




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
Data File : VV020978.D
Acq On : 08 Apr 2021 18:10
Operator : SY/MD
Sample : VSTD0.533
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Apr 09 07:59:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 09 07:58:08 2021
Response via : Initial Calibration




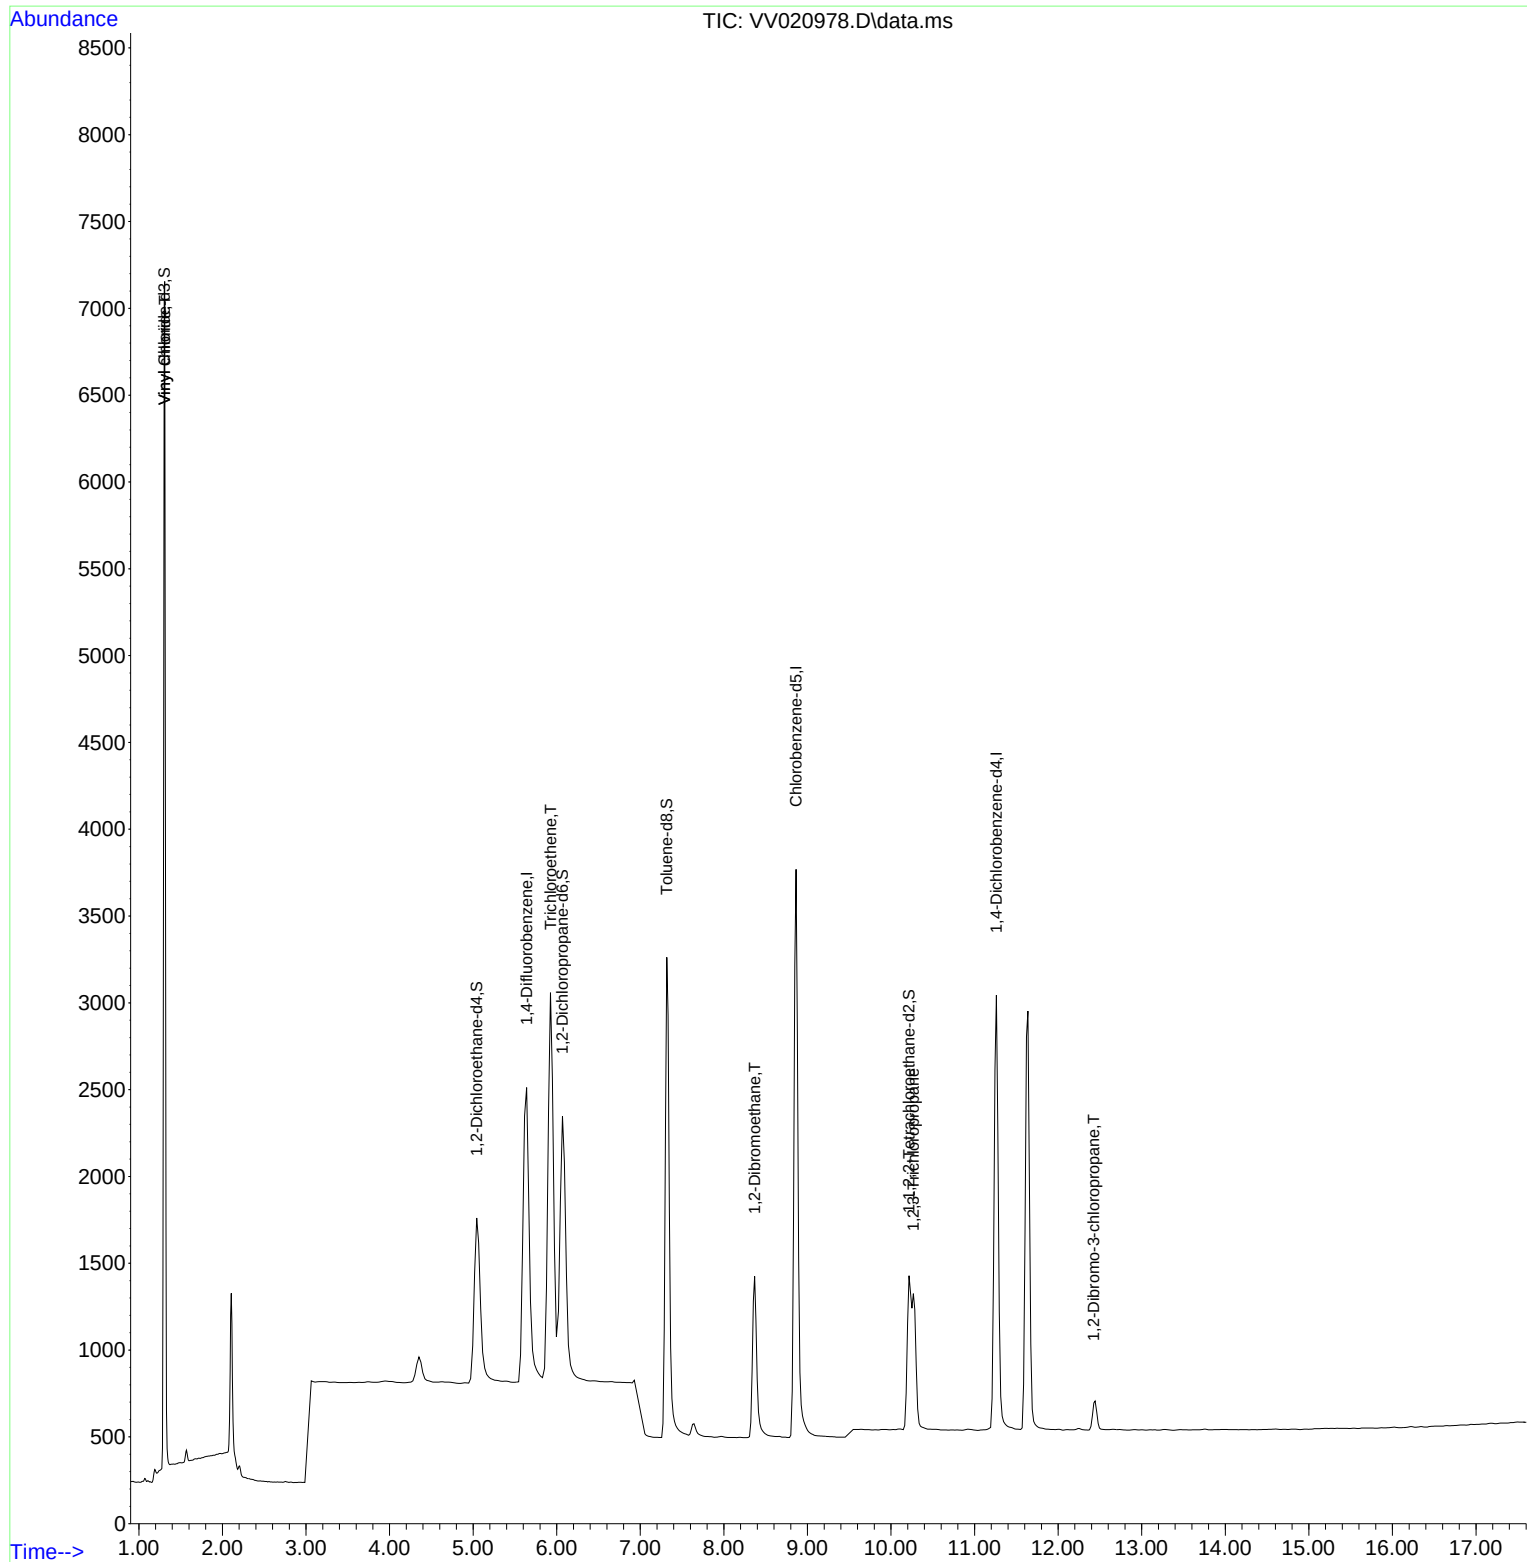


Abundance Scan 59 (1.310 min): VV020978.D\data.ms (-44)

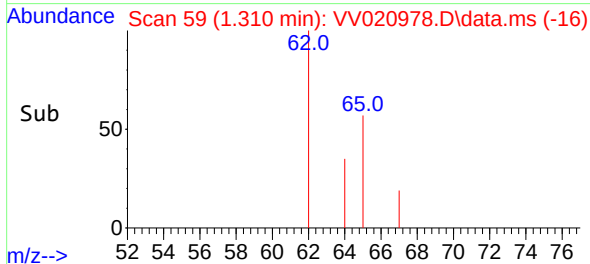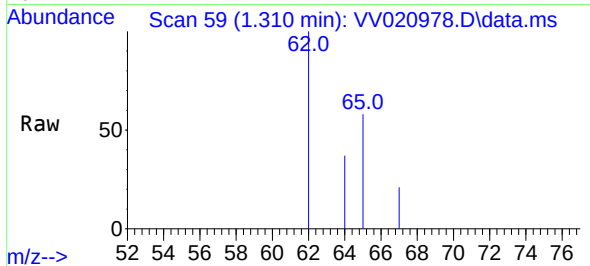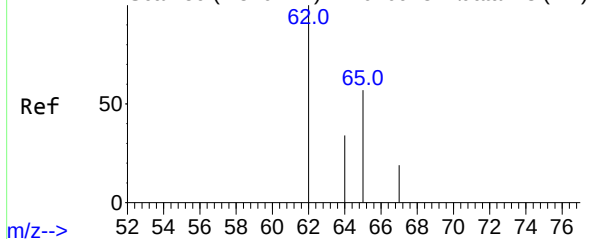


#3
Vinyl chloride
Concen: 0.71 ug/L
RT: 1.310 min Scan# 59
Delta R.T. 0.000 min
Lab File: VV020978.D
Acq: 08 Apr 2021 18:10


Tgt Ion: 62 Resp: 5065
Ion Ratio Lower Upper
62 100
64 36.5 24.3 45.1

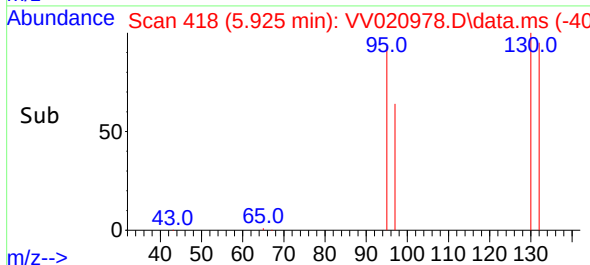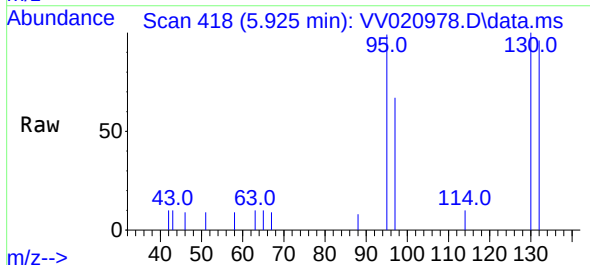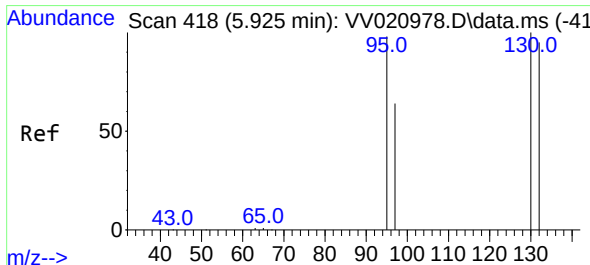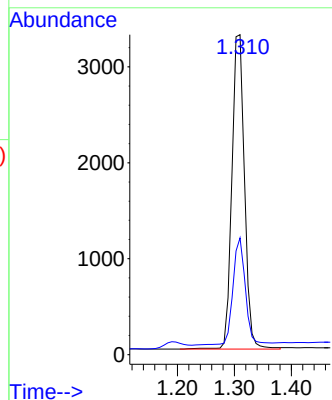

#6
Trichloroethene
Concen: 0.58 ug/L
RT: 5.925 min Scan# 418
Delta R.T. 0.000 min
Lab File: VV020978.D
Acq: 08 Apr 2021 18:10





Tgt Ion: 95 Resp: 2889
Ion Ratio Lower Upper
95 100
97 68.2 47.2 87.6
132 96.7 73.6 136.6
130 101.2 77.1 143.3

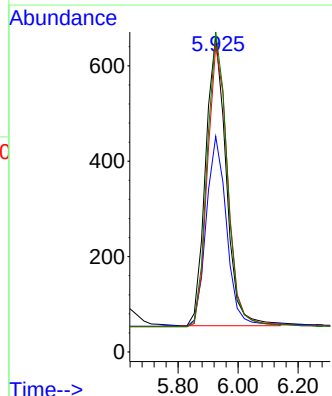

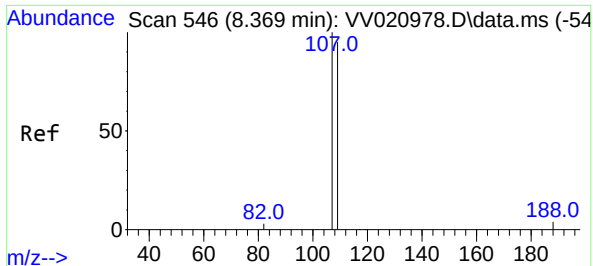




#9
1,2-Dibromoethane
Concen: 0.59 ug/L
RT: 8.369 min Scan# 546
Delta R.T. 0.000 min
Lab File: VV020978.D
Acq: 08 Apr 2021 18:10


Tgt Ion: 107 Resp: 1673
Ion Ratio Lower Upper
107 100
109 95.0 67.3 125.1
188 13.2 7.8 11.8#

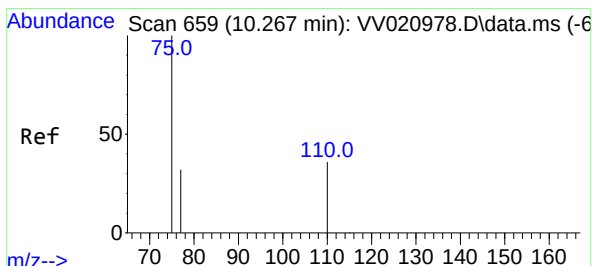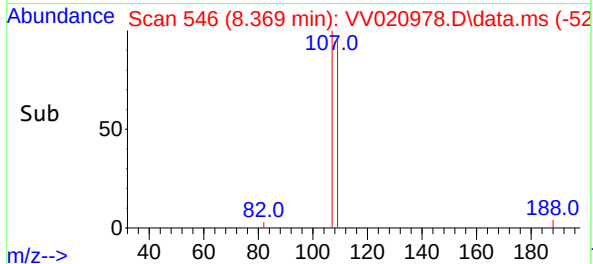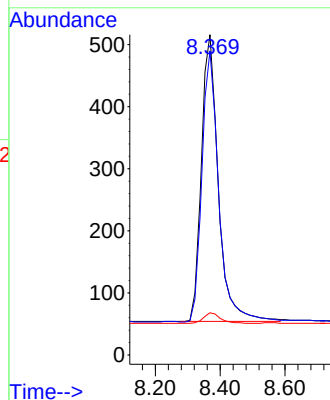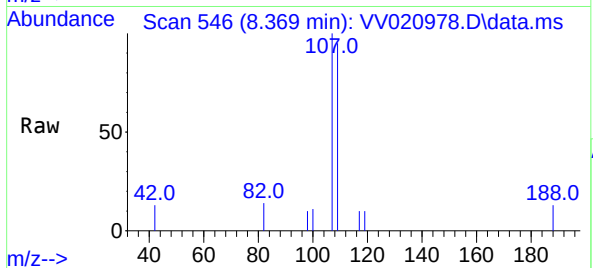

#12
1,2,3-Trichloropropane
Concen: 0.67 ug/L
RT: 10.267 min Scan# 659
Delta R.T. 0.000 min
Lab File: VV020978.D
Acq: 08 Apr 2021 18:10

Tgt Ion: 75 Resp: 1495
Ion Ratio Lower Upper
75 100
110 41.2 33.5 50.3
77 32.8 25.4 38.2

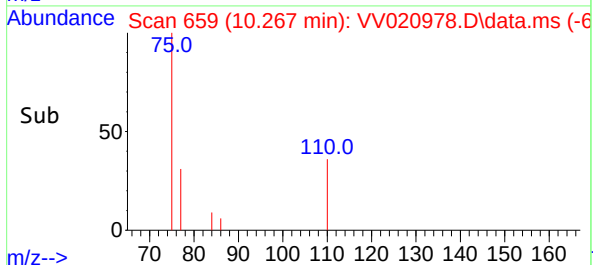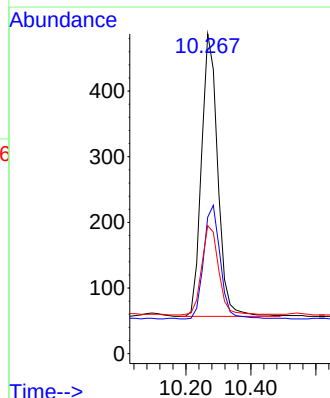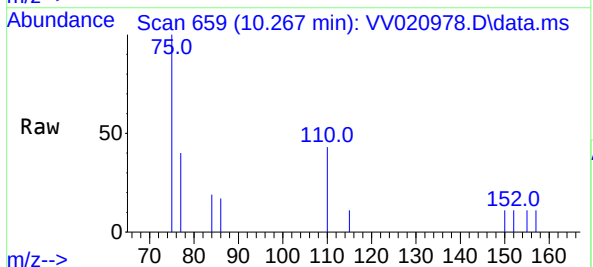

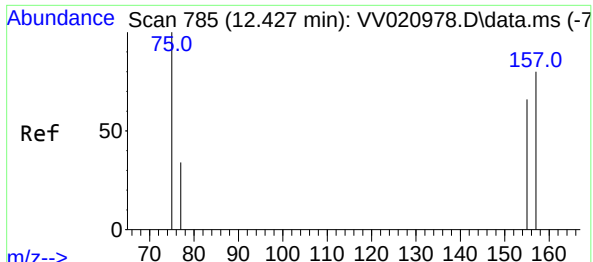

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.65 ug/L
 RT: 12.427 min Scan# 785
 Delta R.T. 0.000 min
 Lab File: VV020978.D
 Acq: 08 Apr 2021 18:10

Tgt Ion:	75	Resp:	198
Ion	Ratio	Lower	Upper
75	100		
157	85.7	74.3	111.5
155	79.5	65.4	98.2

