

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
 Data File : VV020979.D
 Acq On : 08 Apr 2021 18:34
 Operator : SY/MD
 Sample : VSTD00134
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Apr 09 07:59:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 09 07:58:08 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	6145	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	5932	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	2632	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	5591	0.79	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.042	65	4160	1.02	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.068	67	5668	1.15	ug/L	0.00
8) Toluene-d8	7.317	98	10860	0.74	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.216	84	3433	1.31	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.310	62	9515	1.34	ug/L	100
6) Trichloroethene	5.925	95	5453	1.11	ug/L	94
9) 1,2-Dibromoethane	8.368	107	3274	1.18	ug/L	99
12) 1,2,3-Trichloropropane	10.267	75	2912	1.32	ug/L	97
13) 1,2-Dibromo-3-chloropr...	12.426	75	365	1.20	ug/L	94




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
Data File : VV020979.D
Acq On : 08 Apr 2021 18:34
Operator : SY/MD
Sample : VSTD00134
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Apr 09 07:59:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 09 07:58:08 2021
Response via : Initial Calibration




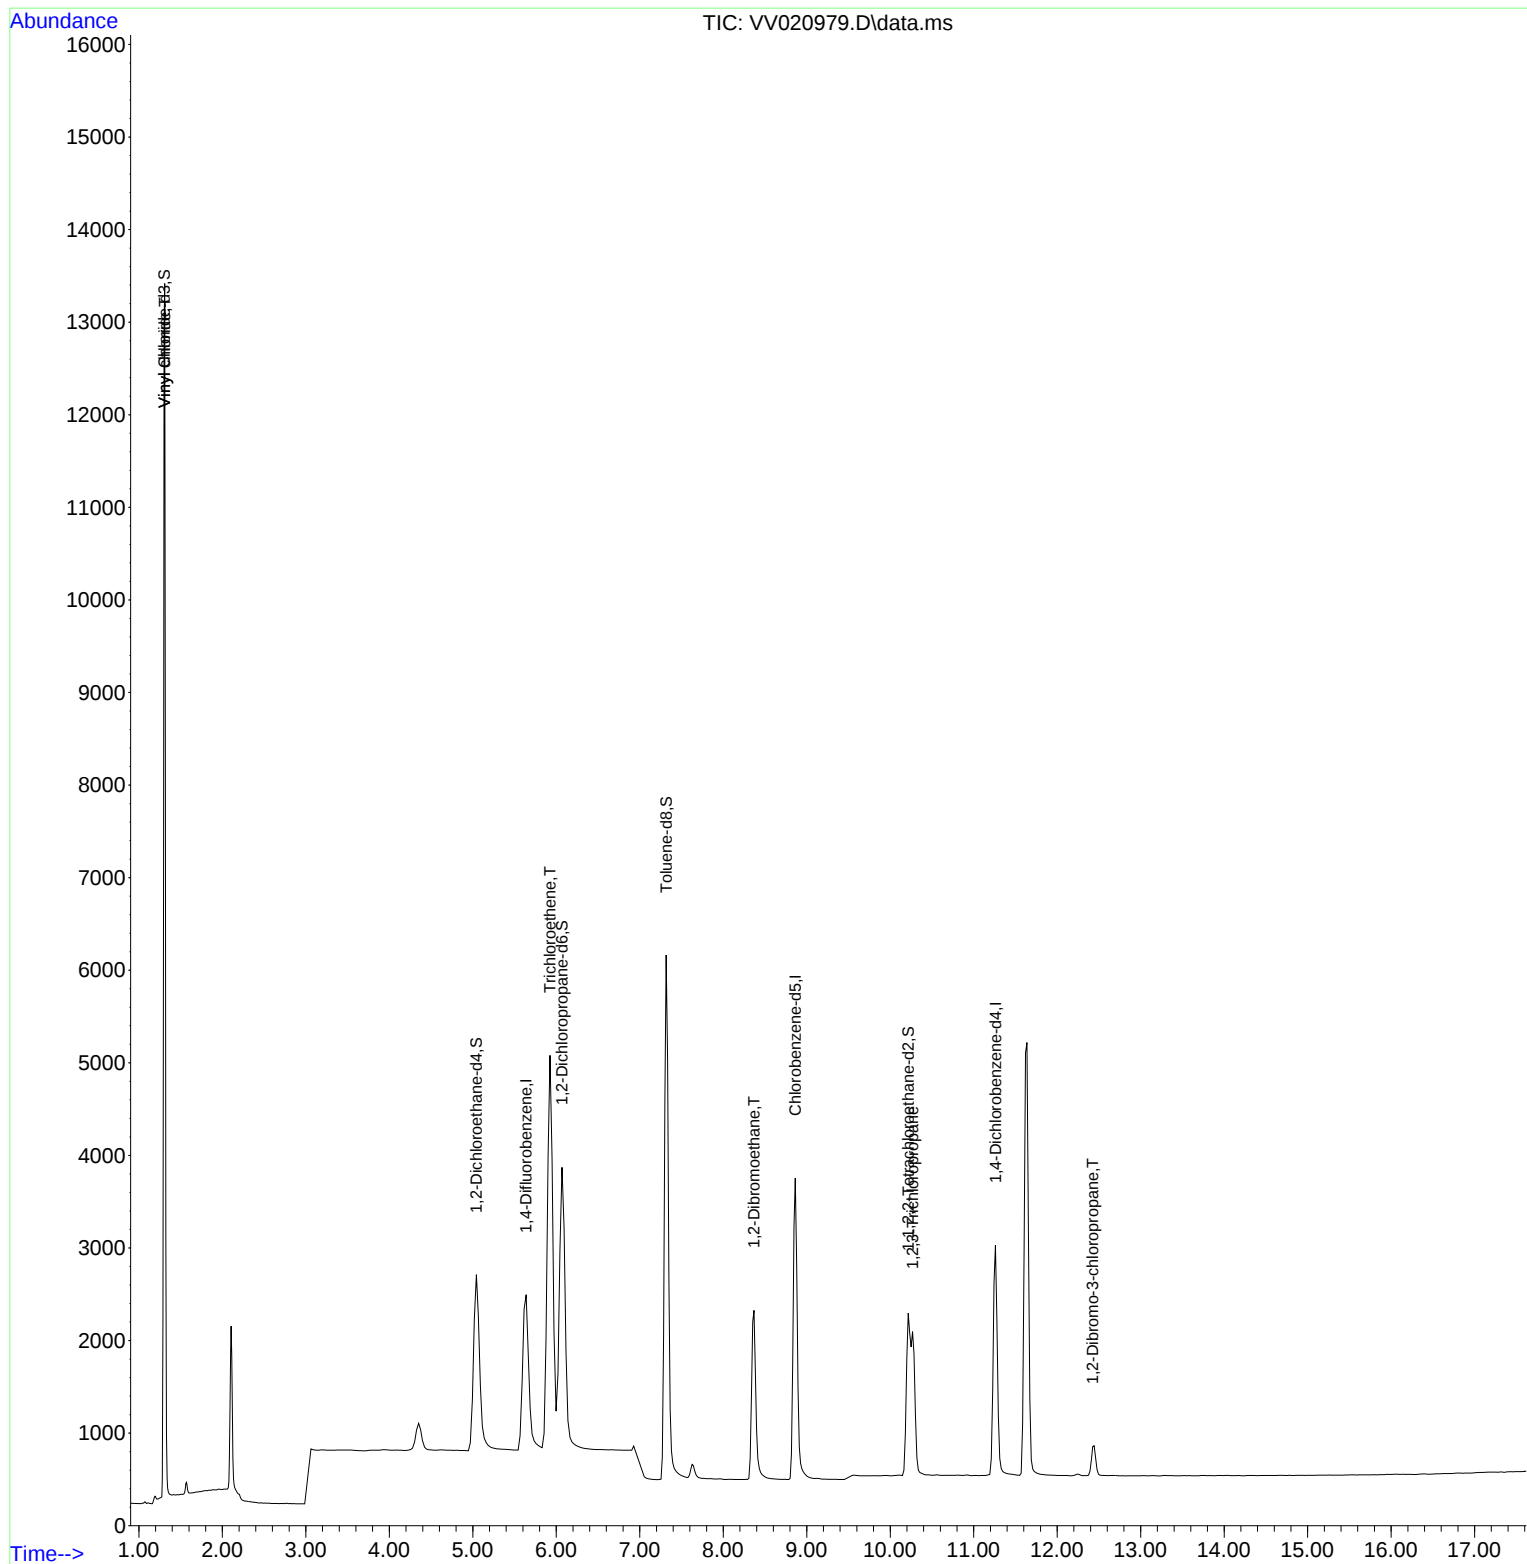


Abundance Scan 59 (1.310 min): VV020978.D\data.ms (-44)

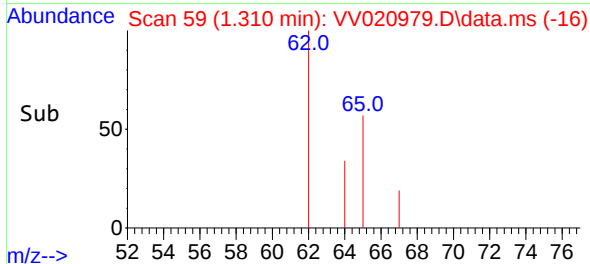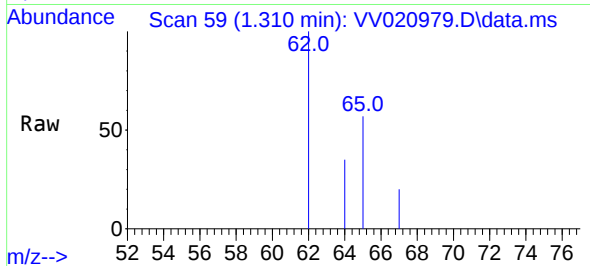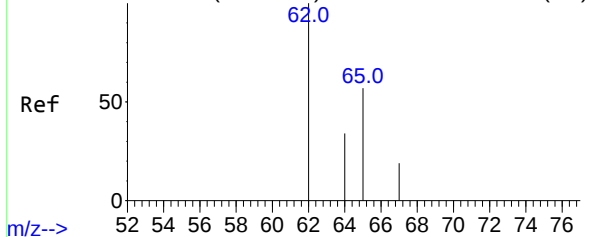


#3
Vinyl chloride
Concen: 1.34 ug/L
RT: 1.310 min Scan# 59
Delta R.T. -0.000 min
Lab File: VV020979.D
Acq: 08 Apr 2021 18:34


Tgt Ion: 62 Resp: 9515
Ion Ratio Lower Upper
62 100
64 35.0 24.3 45.1

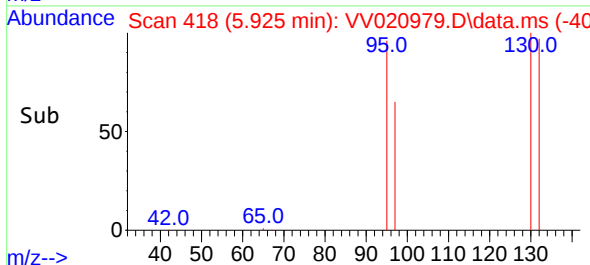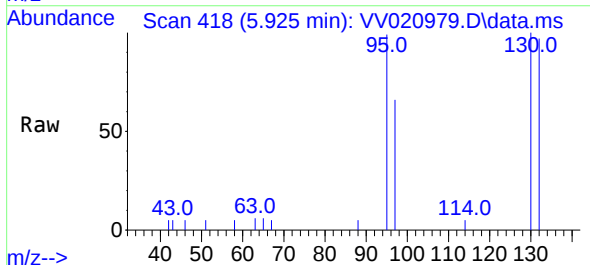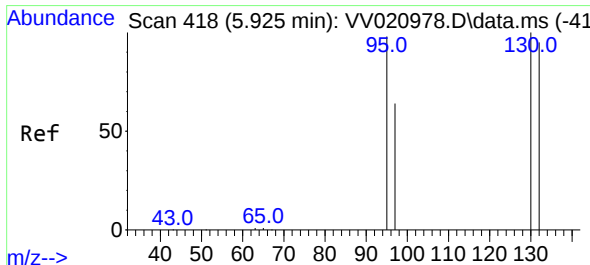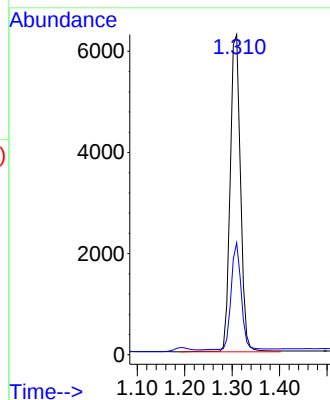

#6
Trichloroethene
Concen: 1.11 ug/L
RT: 5.925 min Scan# 418
Delta R.T. -0.000 min
Lab File: VV020979.D
Acq: 08 Apr 2021 18:34





Tgt Ion: 95 Resp: 5453
Ion Ratio Lower Upper
95 100
97 67.2 47.2 87.6
132 97.8 73.6 136.6
130 101.2 77.1 143.3

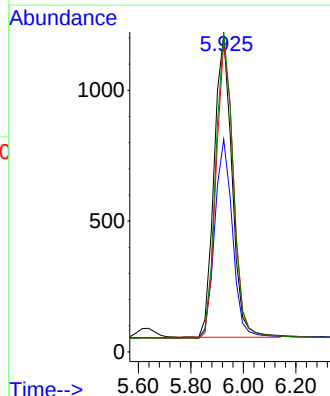

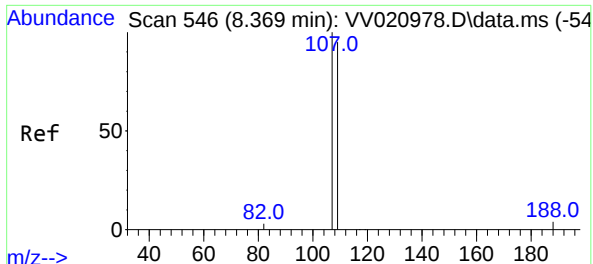




#9
1,2-Dibromoethane
Concen: 1.18 ug/L
RT: 8.368 min Scan# 546
Delta R.T. -0.000 min
Lab File: VV020979.D
Acq: 08 Apr 2021 18:34


Tgt Ion:	107	Resp:	3274
Ion	Ratio	Lower	Upper
107	100		
109	95.6	67.3	125.1
188	9.0	7.8	11.8

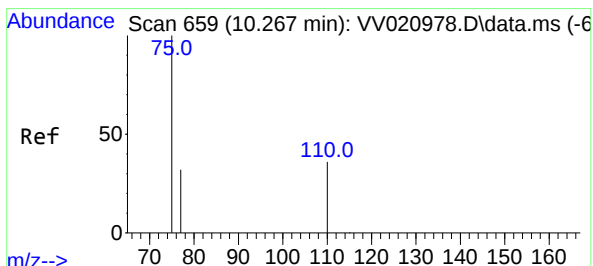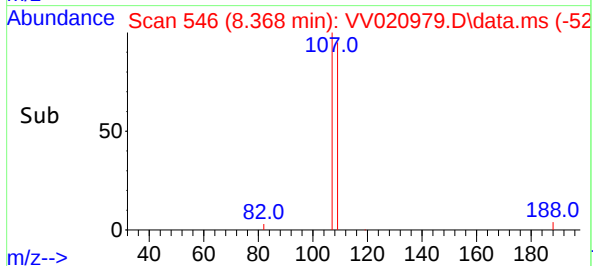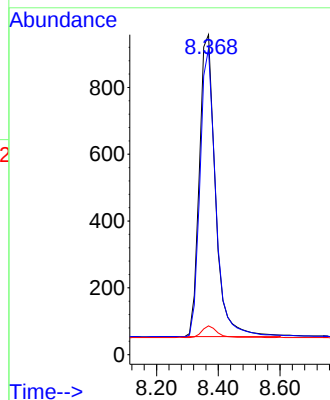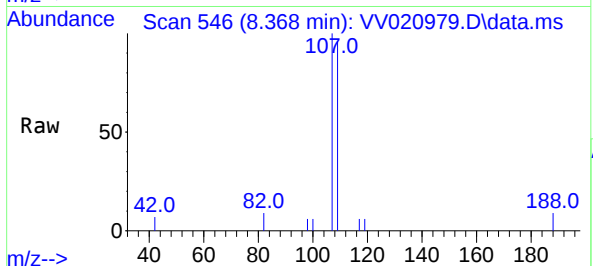

#12
1,2,3-Trichloropropane
Concen: 1.32 ug/L
RT: 10.267 min Scan# 659
Delta R.T. -0.000 min
Lab File: VV020979.D
Acq: 08 Apr 2021 18:34

Tgt Ion:	75	Resp:	2912
Ion	Ratio	Lower	Upper
75	100		
110	39.9	33.5	50.3
77	32.7	25.4	38.2

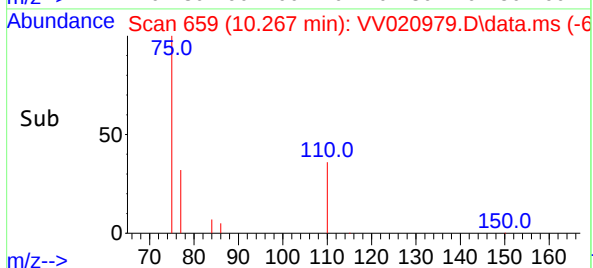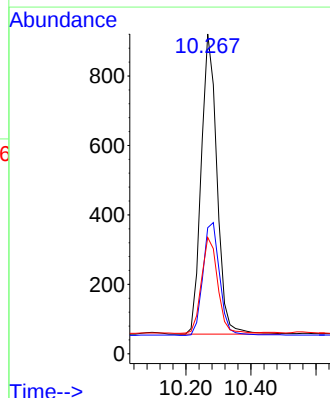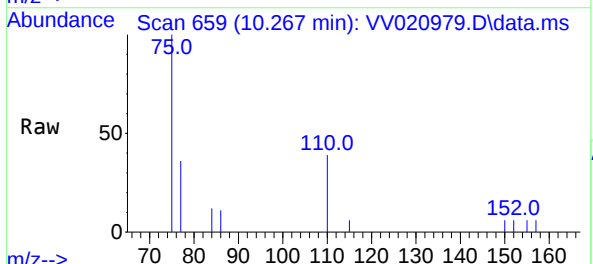

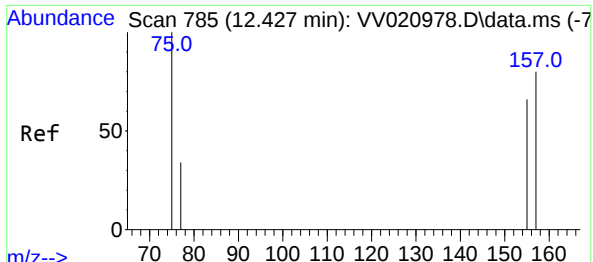

#13
 1,2-Dibromo-3-chloropropane
 Concen: 1.20 ug/L
 RT: 12.426 min Scan# 785
 Delta R.T. -0.000 min
 Lab File: VV020979.D
 Acq: 08 Apr 2021 18:34

Tgt Ion: 75	Resp:	365
Ion Ratio	Lower	Upper
75	100	
157	86.2	74.3 111.5
155	77.2	65.4 98.2

