

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
 Data File : VV020984.D
 Acq On : 09 Apr 2021 10:06
 Operator : SY/MD
 Sample : VV0409WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Apr 10 00:50:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 10 00:49:57 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	5440	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.864	117	5132	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	2239	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	2750	0.54	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	108.00%
4) 1,2-Dichloroethane-d4	5.042	65	1979	0.54	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.00%
7) 1,2-Dichloropropane-d6	6.068	67	2626	0.56	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	112.00%
8) Toluene-d8	7.317	98	4763	0.51	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.00%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	1610	0.54	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	108.00%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.409	75	6	0.02	ug/L	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
Data File : VV020984.D
Acq On : 09 Apr 2021 10:06
Operator : SY/MD
Sample : VV0409WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Apr 10 00:50:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Apr 10 00:49:57 2021
Response via : Initial Calibration

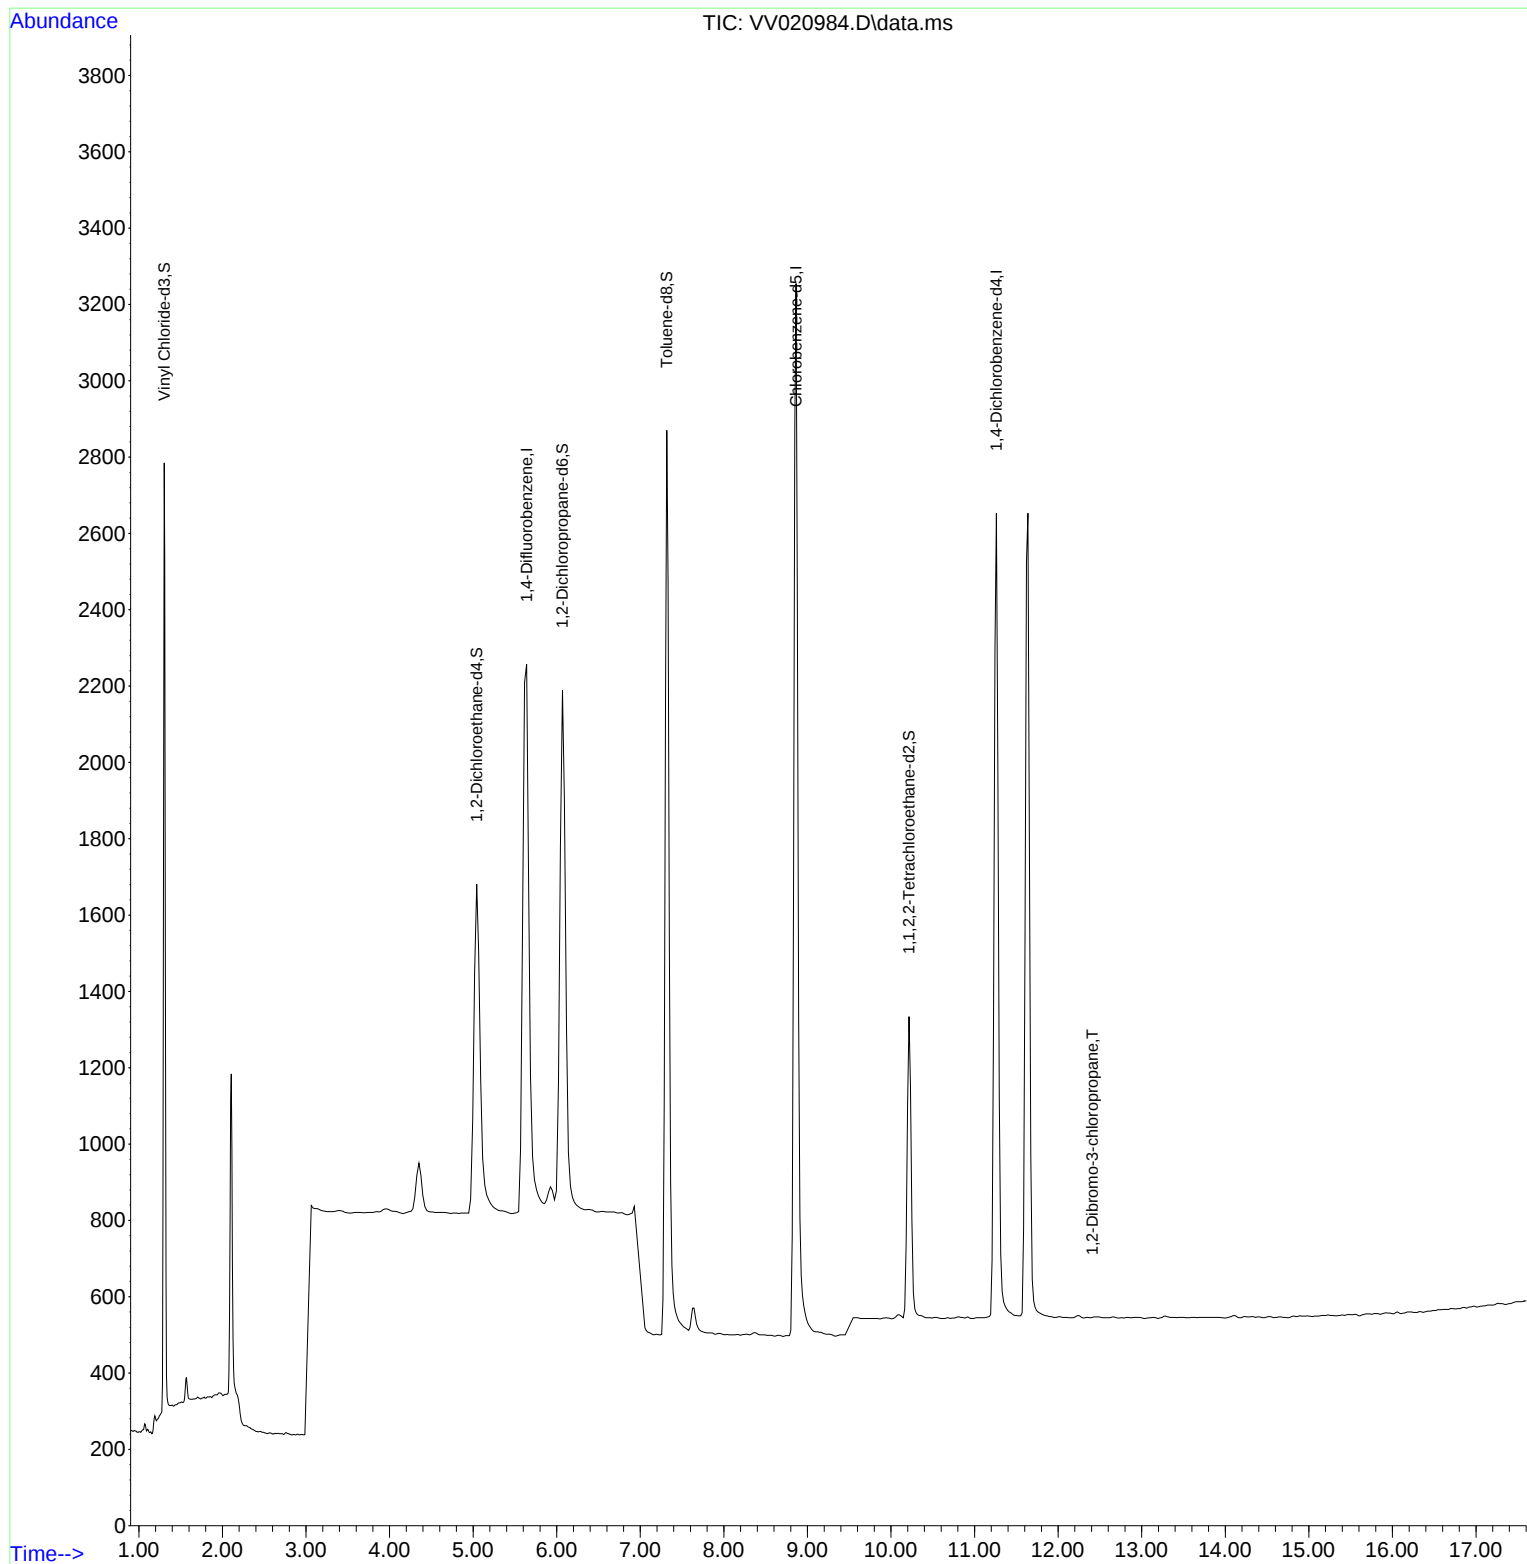

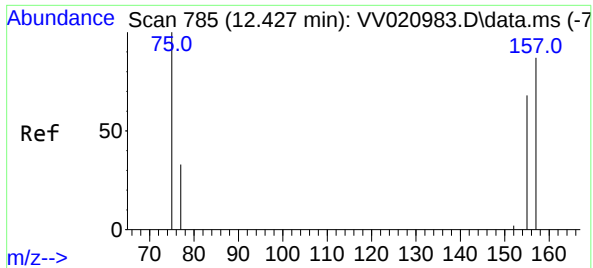

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.02 ug/L
 RT: 12.409 min Scan# 784
 Delta R.T. -0.017 min
 Lab File: VV020984.D
 Acq: 09 Apr 2021 10:06

Tgt Ion: 75	Resp: 6
Ratio	Lower Upper
75 100	
157 89.7	74.3 111.5
155 91.4	65.4 98.2

