
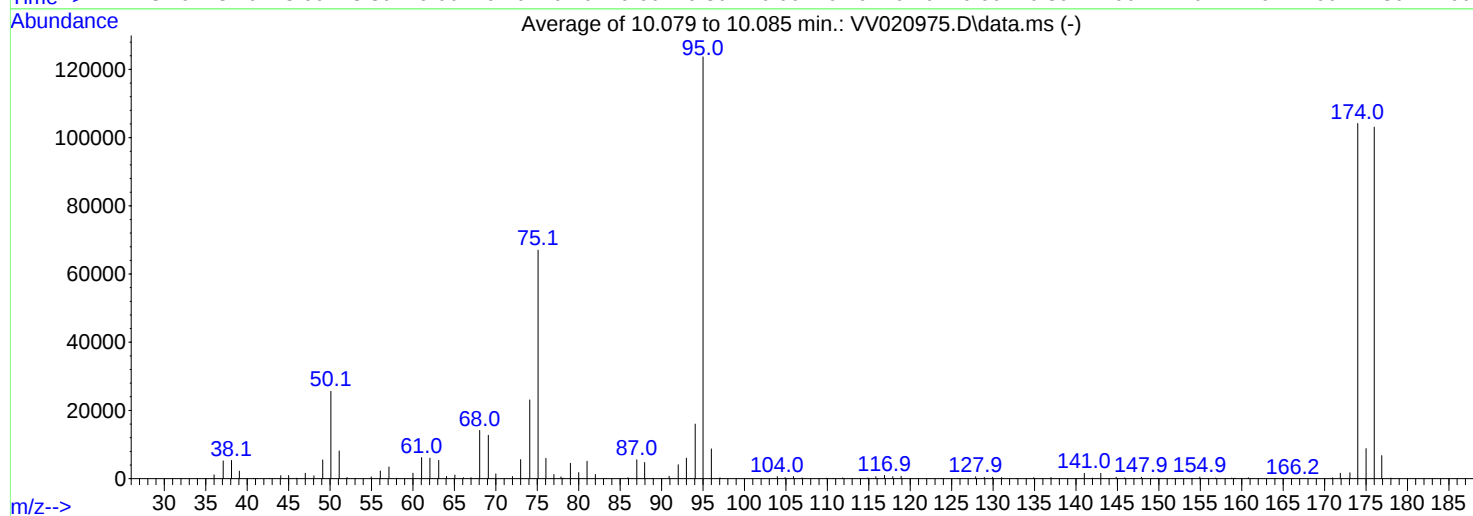


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
 Data File : VV020975.D
 Acq On : 08 Apr 2021 16:33
 Operator : SY/MD
 Sample : BFB35
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB308

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Apr 10 00:49:57 2021

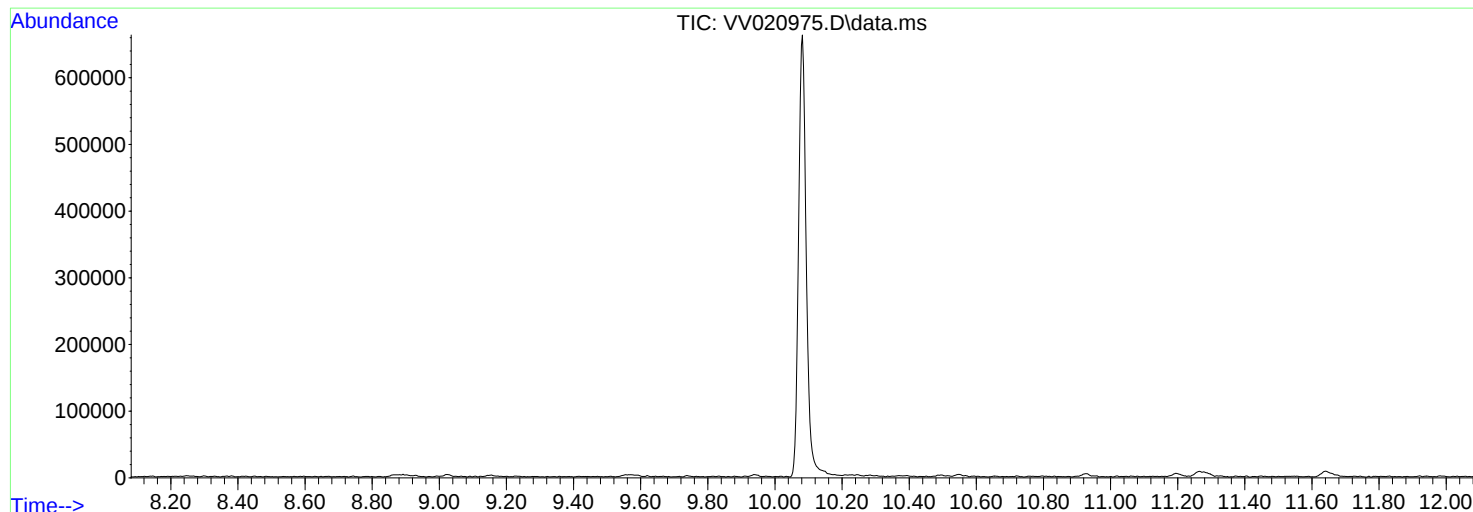

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	25611	PASS
75	95	30	80	54.2	66995	PASS
95	95	100	100	100.0	123685	PASS
96	95	5	9	7.0	8713	PASS
173	174	0.00	2	1.7	1722	PASS
174	95	50	120	84.2	104149	PASS
175	174	5	9	8.5	8808	PASS
176	174	95	101	99.0	103069	PASS
177	176	5	9	6.6	6777	PASS

m/z	Abundance
36.00	1213.0
37.10	4709.0
38.10	4934.0
39.00	2213.0
39.90	320.0
40.70	140.0
44.00	1460.0
45.00	773.0
45.90	162.0
47.00	1602.0
48.10	909.0
49.10	5357.0
50.10	23912.0
51.10	7883.0
52.10	289.0
53.00	120.0
55.00	454.0
56.00	2423.0
57.10	3239.0
58.10	160.0
60.00	1498.0
61.00	5717.0
62.10	5478.0
63.10	5040.0
64.10	544.0
65.00	1070.0
66.10	325.0
67.00	329.0
68.10	13586.0
69.10	12210.0
70.00	1375.0
72.00	600.0
73.00	5098.0
74.10	22032.0
75.10	63256.0
76.10	5758.0
77.00	1139.0
77.90	465.0
78.10	470.0
79.00	4550.0
80.00	1876.0
81.00	4812.0
82.00	1035.0
85.90	243.0
87.00	5214.0
88.00	4438.0
88.90	117.0
90.90	542.0
92.00	4104.0
93.00	5751.0
94.10	14713.0
95.00	117368.0
96.00	8052.0
97.10	225.0
103.80	594.0
105.00	370.0
105.90	608.0
106.90	268.0
109.90	154.0
110.70	155.0
111.80	234.0
113.00	131.0
114.90	161.0
115.90	490.0
116.90	826.0
117.90	443.0
118.90	760.0
124.00	117.0
127.90	502.0
128.90	391.0
130.00	348.0
131.00	305.0
134.90	288.0
137.00	402.0
141.00	1420.0
142.00	149.0
143.00	1574.0
144.80	372.0
145.90	187.0
147.90	437.0
149.10	114.0
150.10	173.0
151.70	108.0
155.00	536.0
156.80	233.0
158.10	163.0
158.80	152.0
160.80	203.0
170.90	182.0
171.90	1576.0
173.10	1753.0
174.00	102368.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

175.00	8605.0
176.00	99984.0
176.90	6574.0
178.00	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

m/z	Abundance
38.20	157.0
40.10	399.0
41.70	151.0
44.10	492.0
51.20	160.0
52.50	132.0
81.30	108.0
188.30	120.0
192.90	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

m/z	Abundance
36.00	1009.0
37.10	5632.0
38.10	5902.0
39.10	2224.0
40.00	310.0
41.90	139.0
42.70	137.0
44.10	1251.0
45.00	1087.0
46.00	124.0
47.00	1599.0
48.00	822.0
49.10	5606.0
50.10	26280.0
51.10	8289.0
52.00	398.0
53.10	107.0
54.90	536.0
56.10	1989.0
57.10	3501.0
58.00	150.0
60.00	1630.0
61.00	6401.0
62.00	6258.0
63.10	5456.0
64.00	820.0
65.10	1046.0
66.10	267.0
67.00	287.0
68.00	14111.0
69.10	12999.0
70.00	1335.0
72.00	619.0
73.00	5982.0
74.10	23584.0
75.10	68536.0
76.00	6013.0
77.00	1217.0
77.80	595.0
79.00	4437.0
80.00	1595.0
81.00	5201.0
82.00	1424.0
83.30	178.0
86.00	309.0
87.00	5580.0
87.90	4796.0
90.90	871.0
92.00	4021.0
93.00	6088.0
94.00	16656.0
95.00	126088.0
96.00	9082.0
97.00	286.0
104.00	663.0
104.80	324.0
105.90	551.0
107.00	162.0
109.90	153.0
111.90	201.0
114.90	269.0
115.80	654.0
116.90	1030.0
117.90	643.0
118.90	667.0
125.70	106.0
127.90	557.0
129.00	356.0
129.90	477.0
131.10	325.0
132.80	117.0
134.90	235.0
137.00	240.0
139.90	110.0
141.00	1661.0
142.00	222.0
143.00	1571.0
144.90	490.0
145.90	251.0
147.90	376.0
149.80	180.0
154.00	130.0
154.90	370.0
155.90	116.0
156.90	161.0
158.80	199.0
159.20	216.0
160.80	306.0
171.00	234.0
171.90	1587.0
173.00	1681.0
174.00	102432.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

175.00	8785.0
176.00	102000.0
176.90	6655.0
178.00	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

m/z	Abundance
36.00	1155.0
37.10	5321.0
38.10	5643.0
39.10	2220.0
39.90	279.0
40.80	114.0
41.20	107.0
42.70	115.0
44.00	1410.0
45.00	957.0
46.00	152.0
47.00	1633.0
48.10	844.0
49.10	5577.0
50.10	26640.0
51.10	8597.0
52.00	333.0
53.10	126.0
55.00	507.0
56.00	2317.0
57.10	3610.0
58.10	147.0
60.00	1620.0
61.10	6439.0
62.00	6273.0
63.10	5496.0
64.00	672.0
65.10	1103.0
66.10	314.0
67.00	299.0
68.10	14667.0
69.10	12881.0
70.00	1481.0
72.00	607.0
73.00	5729.0
74.10	23712.0
75.10	69192.0
76.00	6129.0
77.00	1349.0
77.80	546.0
79.00	4578.0
80.00	1820.0
81.00	5290.0
82.00	1217.0
83.30	102.0
85.90	287.0
87.00	5773.0
87.90	4942.0
90.90	693.0
92.00	4184.0
93.00	6244.0
94.00	16600.0
95.00	127600.0
96.00	9004.0
97.10	227.0
104.00	634.0
104.90	338.0
105.90	629.0
106.90	218.0
109.90	172.0
110.70	112.0
111.90	261.0
113.00	111.0
114.90	239.0
115.90	563.0
116.90	952.0
117.90	589.0
118.90	710.0
123.80	108.0
127.90	595.0
129.00	410.0
129.90	454.0
131.10	327.0
134.90	293.0
137.00	306.0
141.00	1610.0
142.00	181.0
143.00	1535.0
144.90	445.0
145.90	245.0
147.90	407.0
149.90	174.0
154.00	115.0
155.00	528.0
156.00	110.0
156.80	177.0
158.10	146.0
158.80	171.0
159.20	146.0
160.80	279.0
166.20	125.0
170.90	239.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308

171.90	1627.0
173.10	1733.0
174.00	107648.0
175.00	9034.0
176.00	107224.0
176.90	7101.0
178.00	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB308