
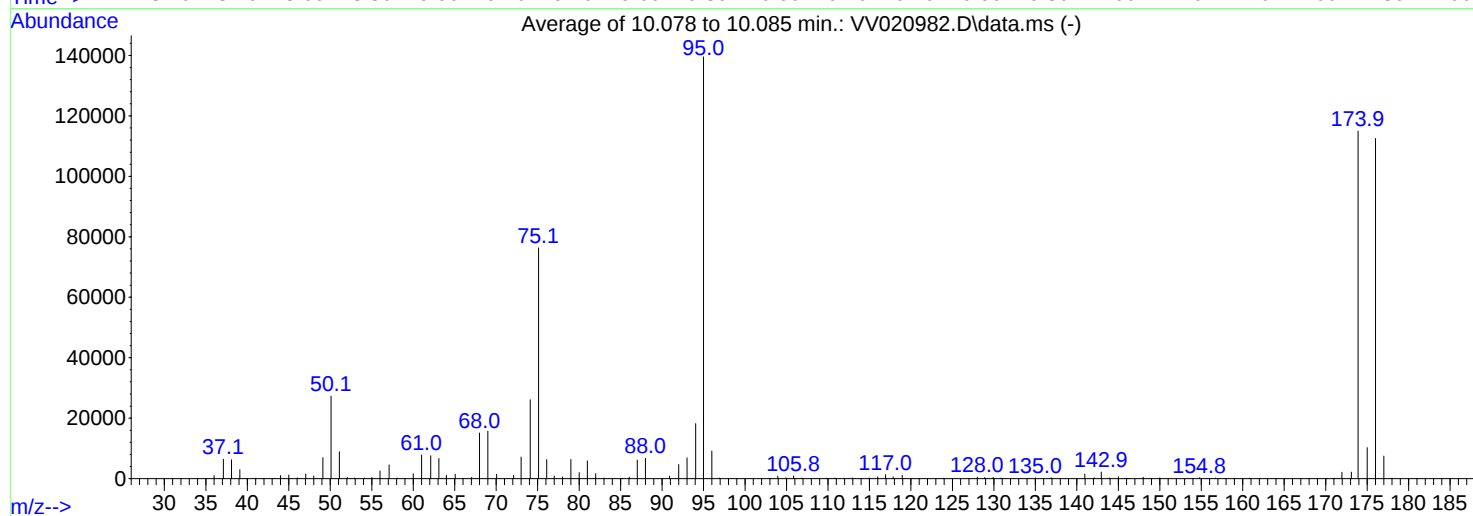


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040921\
 Data File : VV020982.D
 Acq On : 09 Apr 2021 09:00
 Operator : SY/MD
 Sample : BFB36
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB309

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM040921.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Apr 10 00:49:57 2021

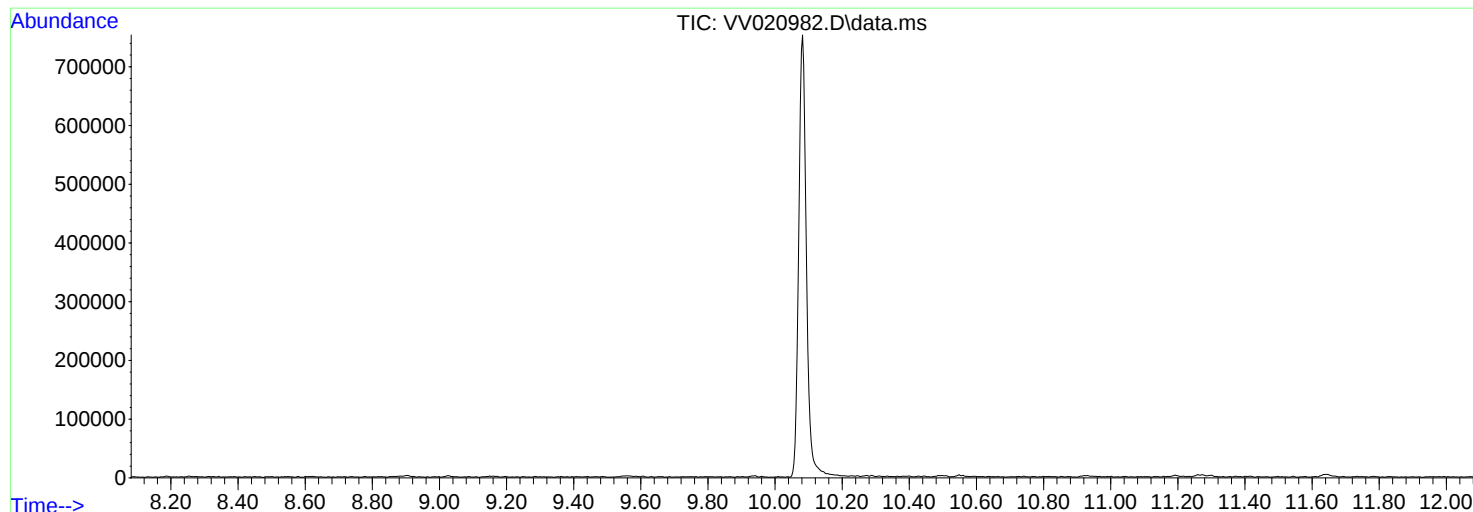

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	27301	PASS
75	95	30	80	54.7	76320	PASS
95	95	100	100	100.0	139541	PASS
96	95	5	9	6.6	9176	PASS
173	174	0.00	2	1.9	2165	PASS
174	95	50	120	82.4	114992	PASS
175	174	5	9	8.9	10260	PASS
176	174	95	101	97.9	112528	PASS
177	176	5	9	6.7	7490	PASS

m/z	Abundance
35.40	257.0
36.20	198.0
39.10	100.0
39.80	205.0
42.00	118.0
43.90	501.0
64.70	134.0
66.10	107.0
71.70	156.0
100.40	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	976.0
37.10	5653.0
38.10	6026.0
39.10	2723.0
40.00	306.0
40.90	226.0
41.80	238.0
44.00	1446.0
45.00	1256.0
45.90	295.0
47.10	1360.0
48.00	901.0
49.10	6423.0
50.10	25144.0
51.10	8291.0
52.10	362.0
52.90	161.0
54.10	205.0
54.90	386.0
56.00	2452.0
57.10	4302.0
58.10	210.0
60.00	1642.0
61.00	7141.0
62.10	6785.0
63.10	6152.0
64.00	989.0
65.10	1321.0
66.00	248.0
67.10	455.0
68.00	14313.0
69.00	15017.0
70.10	1505.0
72.10	1110.0
73.00	6777.0
74.10	24032.0
75.10	74336.0
76.10	5592.0
77.00	827.0
78.00	583.0
79.00	5990.0
80.00	1853.0
81.00	5727.0
82.00	1641.0
83.00	185.0
86.10	497.0
87.00	6080.0
88.00	6706.0
90.90	770.0
92.00	4210.0
93.00	6666.0
94.10	17928.0
95.00	136576.0
96.00	9058.0
96.90	251.0
103.90	737.0
104.90	326.0
105.80	831.0
106.90	208.0
108.40	108.0
109.90	108.0
110.80	213.0
111.90	201.0
112.80	219.0
114.90	200.0
116.00	682.0
116.90	1330.0
117.80	690.0
118.90	1040.0
123.80	141.0
128.00	446.0
128.90	402.0
130.00	459.0
130.90	165.0
135.10	199.0
136.90	286.0
138.60	117.0
140.10	157.0
141.00	1685.0
142.00	241.0
142.90	2158.0
143.90	223.0
145.00	537.0
145.70	106.0
146.30	148.0
148.00	433.0
150.00	201.0
154.80	272.0
156.00	107.0
156.70	163.0
159.00	171.0
160.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

170.20	113.0
170.80	193.0
172.00	2040.0
173.10	2310.0
173.90	111704.0
175.00	9956.0
176.00	111048.0
177.00	7400.0
177.80	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
35.40	282.0
36.30	144.0
39.10	142.0
39.80	210.0
42.00	113.0
43.90	466.0
45.30	112.0
64.70	182.0
71.70	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
38.20	157.0
40.10	399.0
41.70	151.0
44.10	492.0
51.20	160.0
52.50	132.0
81.30	108.0
188.30	120.0
192.90	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	1353.0
37.10	6967.0
38.10	6373.0
39.10	3230.0
40.00	319.0
41.00	187.0
43.20	212.0
44.10	1498.0
45.00	1163.0
46.10	288.0
47.00	1637.0
48.00	883.0
49.10	7098.0
50.10	28576.0
51.10	9081.0
52.00	400.0
53.00	266.0
54.20	174.0
55.10	428.0
56.00	2552.0
57.10	4653.0
58.00	185.0
60.00	1462.0
61.00	8318.0
62.10	8134.0
63.10	6825.0
64.00	1188.0
65.00	1652.0
65.90	121.0
67.00	359.0
68.00	15330.0
69.00	15868.0
70.00	1291.0
72.10	993.0
73.00	7293.0
74.10	27128.0
75.10	75544.0
76.10	6797.0
77.00	954.0
78.00	619.0
79.00	6486.0
80.00	2173.0
81.00	5902.0
82.00	1565.0
83.00	244.0
85.20	142.0
86.00	530.0
87.00	5998.0
88.00	6378.0
90.90	837.0
92.00	4902.0
93.00	6889.0
94.00	17856.0
95.00	137984.0
96.00	8936.0
96.90	154.0
104.00	954.0
105.00	237.0
105.80	934.0
106.80	210.0
107.90	183.0
109.90	225.0
110.90	255.0
112.00	152.0
113.00	243.0
114.90	193.0
116.00	535.0
117.00	1256.0
117.90	539.0
119.00	1112.0
124.00	147.0
128.00	516.0
128.90	286.0
129.80	407.0
130.80	264.0
131.10	276.0
134.00	122.0
134.90	337.0
136.90	301.0
140.90	1384.0
142.20	253.0
143.00	2169.0
144.00	176.0
145.00	664.0
145.80	149.0
146.10	115.0
148.00	522.0
150.00	258.0
154.00	204.0
154.80	472.0
156.70	291.0
157.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

158.90	187.0
160.70	200.0
170.00	155.0
171.00	252.0
171.90	2113.0
173.10	1978.0
173.90	114552.0
175.00	10082.0
176.00	109904.0
177.00	7227.0
177.90	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	1218.0
37.10	6605.0
38.10	6344.0
39.10	3202.0
40.00	302.0
40.90	161.0
41.80	185.0
43.20	156.0
44.00	1541.0
45.00	1269.0
46.10	271.0
47.10	1631.0
48.00	927.0
49.10	7215.0
50.10	28184.0
51.10	9254.0
52.10	400.0
52.90	214.0
54.20	212.0
55.00	423.0
56.00	2665.0
57.10	4740.0
58.10	195.0
60.00	1753.0
61.00	8043.0
62.10	7874.0
63.10	7005.0
64.00	1136.0
65.00	1511.0
65.90	183.0
67.10	399.0
68.00	15572.0
69.00	16281.0
70.00	1469.0
72.10	1130.0
73.00	7437.0
74.10	27056.0
75.10	79080.0
76.10	6468.0
77.00	994.0
78.00	641.0
79.00	6552.0
80.00	2080.0
81.00	6023.0
82.00	1673.0
83.00	232.0
85.20	131.0
86.00	515.0
87.00	6370.0
88.00	7138.0
90.90	884.0
92.00	4899.0
93.00	7122.0
94.10	18848.0
95.00	144064.0
96.00	9533.0
96.90	208.0
103.20	108.0
104.00	931.0
104.90	285.0
105.90	976.0
106.90	207.0
107.90	158.0
109.80	162.0
110.90	243.0
112.00	166.0
113.00	236.0
115.00	222.0
116.00	625.0
116.90	1402.0
117.90	607.0
119.00	1150.0
124.00	141.0
128.00	508.0
128.90	408.0
129.90	428.0
130.90	228.0
135.00	281.0
136.90	309.0
138.60	118.0
140.10	114.0
140.90	1555.0
142.10	267.0
142.90	2219.0
143.90	236.0
145.00	651.0
145.70	124.0
146.30	124.0
148.00	527.0
148.90	113.0
150.00	266.0
154.00	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

154.80	398.0
155.70	119.0
156.70	241.0
157.80	113.0
158.90	207.0
160.80	202.0
170.00	154.0
171.10	251.0
171.90	2220.0
173.10	2207.0
173.90	118720.0
175.00	10742.0
176.00	116632.0
177.00	7843.0
177.90	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309