

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035091.D
 Acq On : 09 Apr 2024 18:39
 Operator : SY/MD
 Sample : PB160098TB 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 10 04:59:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:53:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	335433	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	327800	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	133646	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	124437	38.413	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.820%		
7) Chloroethane-d5	1.526	69	116129	41.273	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.540%		
11) 1,1-Dichloroethene-d2	2.056	65	57428	40.442	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.880%		
21) 2-Butanone-d5	3.786	46	189289	98.524	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.520%		
24) Chloroform-d	4.246	84	253165	46.482	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.960%		
26) 1,2-Dichloroethane-d4	4.941	65	167711	48.499	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.000%		
32) Benzene-d6	4.957	84	493406	44.811	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.620%		
36) 1,2-Dichloropropane-d6	5.989	67	166094	47.503	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.000%		
41) Toluene-d8	7.243	98	414678	41.818	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.640%		
43) trans-1,3-Dichloroprop...	7.555	79	68631	40.376	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.760%		
47) 2-Hexanone-d5	8.024	63	116997	88.502	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.500%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	226975	47.139	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.280%		
66) 1,2-Dichlorobenzene-d4	11.561	152	147048	49.005	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.020%		
Target Compounds						Qvalue
13) Acetone	2.118	43	9180	5.204	ug/L	95
61) 1,2,3-Trichloropropane	11.185	75	17387	6.004	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035091.D
Acq On : 09 Apr 2024 18:39
Operator : SY/MD
Sample : PB160098TB 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 10 04:59:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

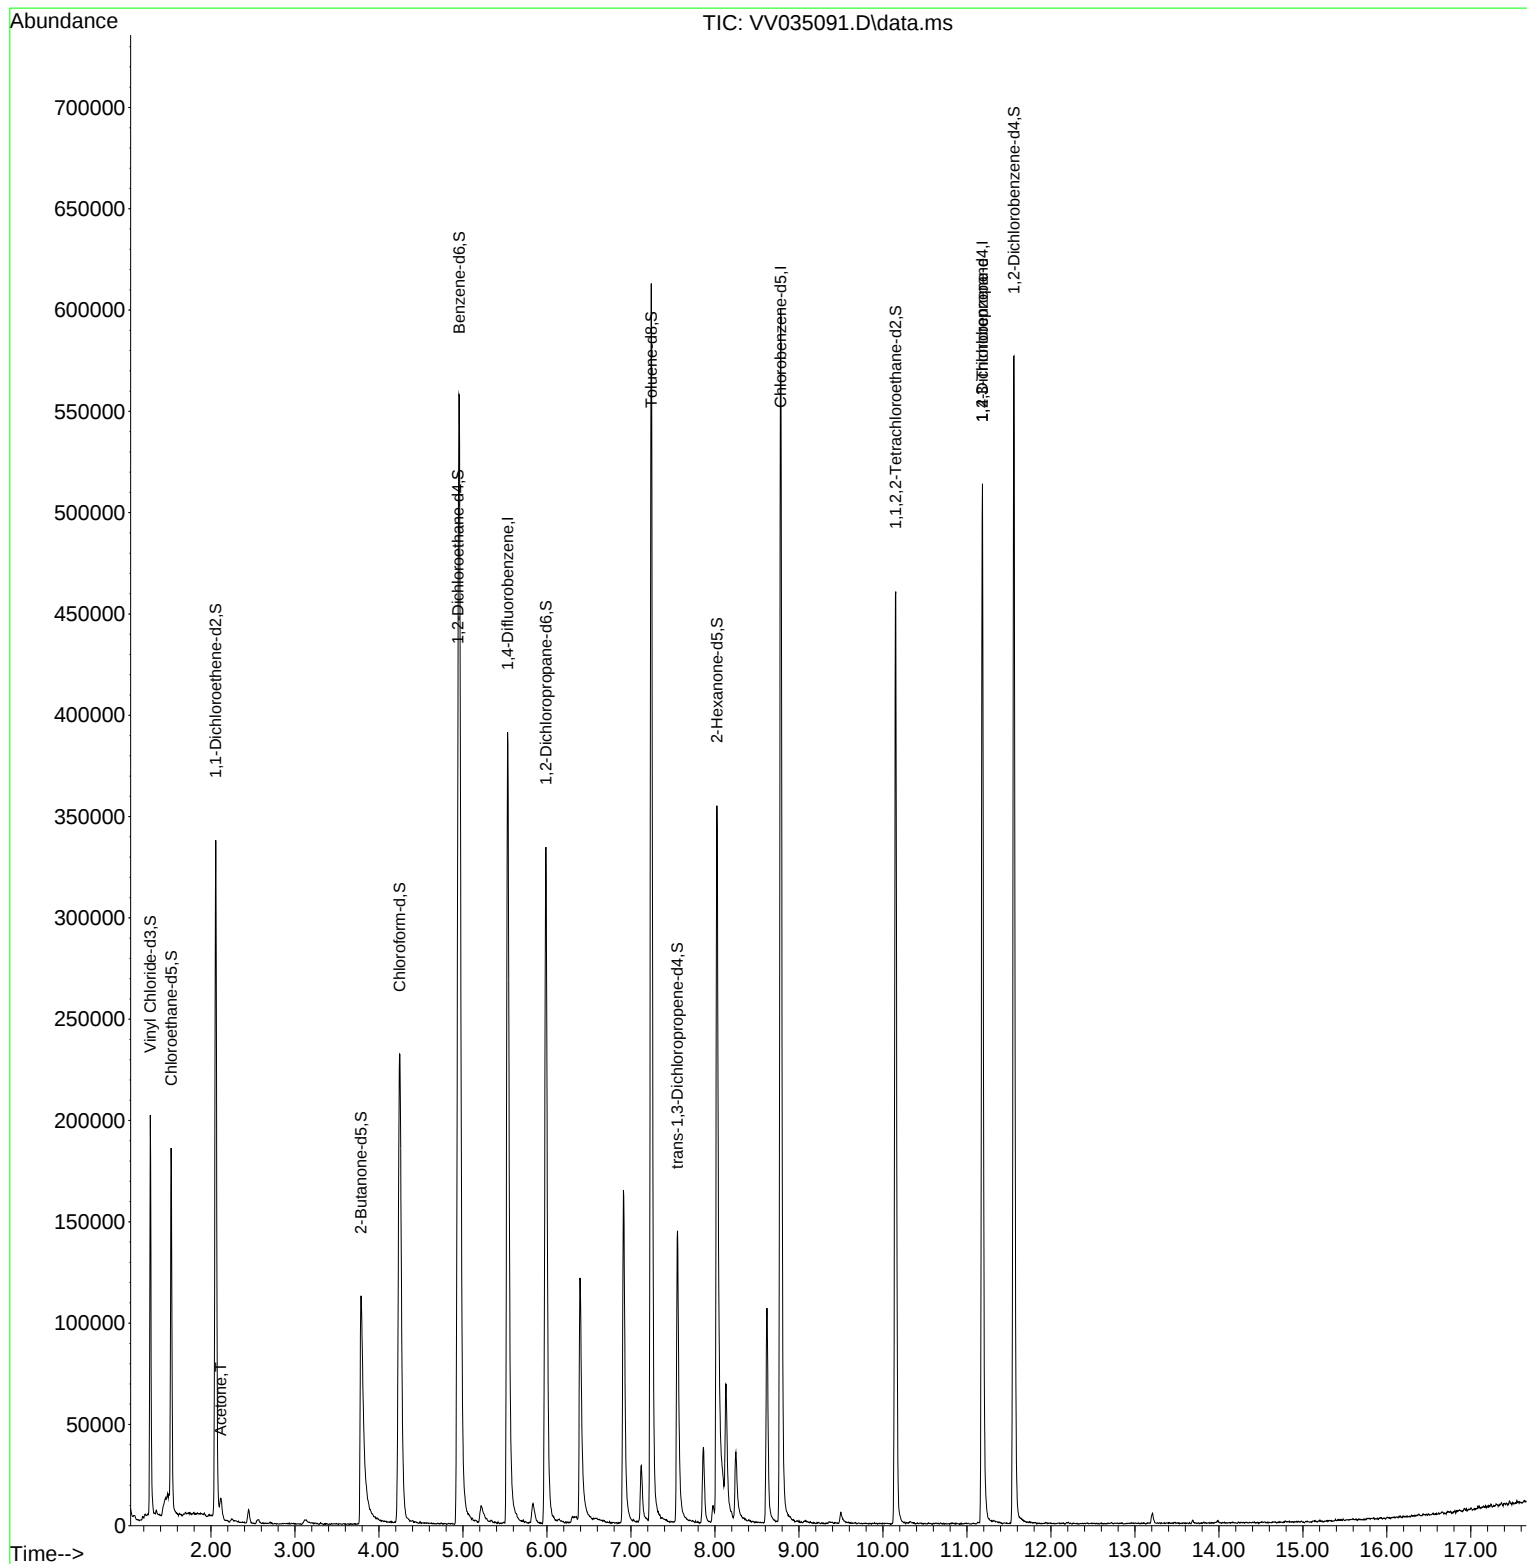

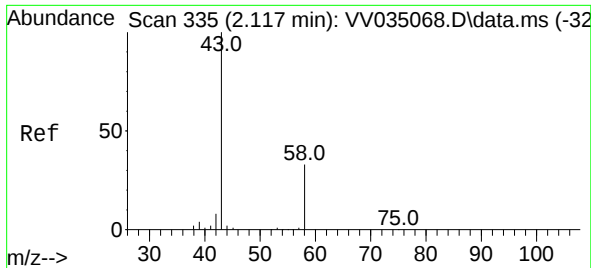

#13

Acetone

Concen: 5.204 ug/L

RT: 2.118 min Scan# 3155

Delta R.T. 0.000 min

Lab File: VV035091.D

Acq: 09 Apr 2024 18:39

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 9180

Ion Ratio Lower Upper

43 100

58 35.6 0.0 66.0

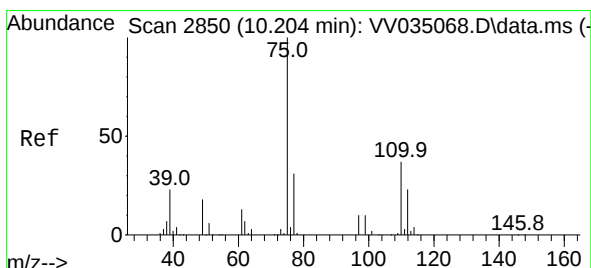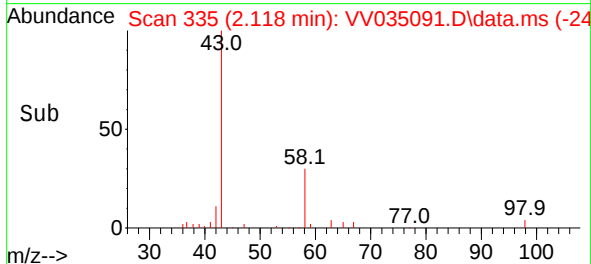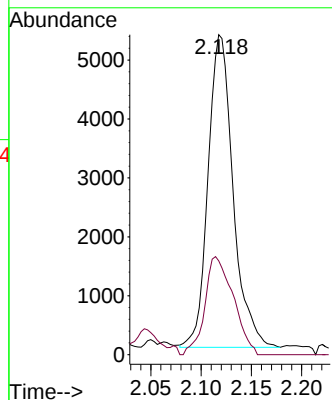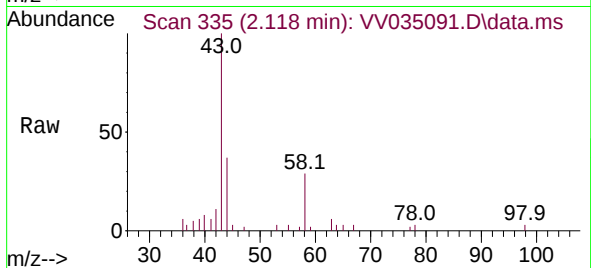

#61

1,2,3-Trichloropropane

Concen: 6.004 ug/L

RT: 11.185 min Scan# 3155

Delta R.T. 0.981 min

Lab File: VV035091.D

Acq: 09 Apr 2024 18:39

Tgt Ion: 75 Resp: 17387

Ion Ratio Lower Upper

75 100

77 31.7 26.0 39.0

110 2.4 30.5 45.7#

