

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035069.D
 Acq On : 09 Apr 2024 09:51
 Operator : SY/MD
 Sample : VV0409MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	240109	250612	15.38%	2.172%
2	1.529	145	152	170	rVB	207413	245572	15.07%	2.129%
3	2.056	307	316	336	rVB	396364	574727	35.27%	4.982%
4	2.449	431	438	449	rVB6	2041	3534	0.22%	0.031%
5	2.507	454	456	459	rBV2	635	358	0.02%	0.003%
6	2.529	461	463	467	rBV3	365	203	0.01%	0.002%
7	2.728	523	525	530	rBV2	401	313	0.02%	0.003%
8	2.841	557	560	563	rBV4	291	227	0.01%	0.002%
9	2.870	566	569	570	rBV	323	205	0.01%	0.002%
10	2.915	581	583	589	rVB2	405	199	0.01%	0.002%
11	2.950	592	594	597	rVV3	273	154	0.01%	0.001%
12	3.140	649	653	658	rVB	329	285	0.02%	0.002%
13	3.269	688	693	694	rBV2	358	233	0.01%	0.002%
14	3.301	699	703	704	rBV	280	185	0.01%	0.002%
15	3.317	706	708	710	rBV	352	202	0.01%	0.002%
16	3.365	720	723	728	rBV2	208	172	0.01%	0.001%
17	3.407	732	736	741	rBV4	330	348	0.02%	0.003%
18	3.478	756	758	760	rBV	310	156	0.01%	0.001%
19	3.497	760	764	769	rVV3	452	408	0.03%	0.004%
20	3.548	776	780	781	rBV	296	176	0.01%	0.002%
21	3.574	785	788	791	rVV2	325	216	0.01%	0.002%
22	3.625	799	804	807	rBV3	397	246	0.02%	0.002%
23	3.645	807	810	814	rVB2	257	194	0.01%	0.002%
24	3.786	845	854	893	rBV	118833	343377	21.07%	2.977%
25	4.246	982	997	1034	rBV	253603	645960	39.64%	5.600%
26	4.616	1110	1112	1117	rBV3	327	279	0.02%	0.002%
27	4.815	1167	1174	1179	rBV4	490	720	0.04%	0.006%
28	4.953	1199	1217	1263	rBV2	610045	1629561	100.00%	14.126%
29	5.326	1329	1333	1336	rBV2	826	693	0.04%	0.006%
30	5.423	1360	1363	1366	rBV3	473	302	0.02%	0.003%
31	5.532	1386	1397	1429	rBV	394164	831433	51.02%	7.207%
32	5.831	1480	1490	1508	rBV4	11295	26762	1.64%	0.232%
33	5.985	1525	1538	1568	rBV	356662	746460	45.81%	6.471%
34	6.294	1631	1634	1639	rVB6	745	632	0.04%	0.005%
35	6.387	1659	1663	1668	rVB3	559	562	0.03%	0.005%
36	6.410	1668	1670	1672	rBV	397	213	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035069.D
 Acq On : 09 Apr 2024 09:51
 Operator : SY/MD
 Sample : VV0409MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.439	1677	1679	1683	rVB2	738	340	0.02%	0.003%
38	6.510	1699	1701	1704	rVB	372	171	0.01%	0.001%
39	6.542	1707	1711	1712	rBV3	413	297	0.02%	0.003%
40	6.555	1713	1715	1720	rVB2	324	190	0.01%	0.002%
41	6.690	1755	1757	1759	rBV	324	187	0.01%	0.002%
42	6.712	1762	1764	1767	rBV	618	313	0.02%	0.003%
43	6.738	1767	1772	1776	rBV4	515	474	0.03%	0.004%
44	6.809	1789	1794	1795	rBV2	307	149	0.01%	0.001%
45	6.821	1795	1798	1801	rVB2	515	294	0.02%	0.003%
46	6.857	1806	1809	1815	rBV4	633	549	0.03%	0.005%
47	6.911	1816	1826	1855	rBV	171936	336645	20.66%	2.918%
48	7.239	1918	1928	1971	rBV	674907	1200604	73.68%	10.408%
49	7.551	2016	2025	2056	rBV	116438	222961	13.68%	1.933%
50	8.024	2163	2172	2211	rBV2	330441	731805	44.91%	6.344%
51	8.551	2334	2336	2338	rBV2	663	351	0.02%	0.003%
52	8.645	2363	2365	2368	rBV3	443	278	0.02%	0.002%
53	8.677	2374	2375	2376	rBV3	483	180	0.01%	0.002%
54	8.709	2383	2385	2388	rBV	407	147	0.01%	0.001%
55	8.783	2397	2408	2441	rBV	599831	1012092	62.11%	8.773%
56	9.056	2488	2493	2499	rVB6	901	1339	0.08%	0.012%
57	9.082	2499	2501	2505	rBV	724	409	0.03%	0.004%
58	9.101	2505	2507	2509	rBV3	689	418	0.03%	0.004%
59	9.194	2534	2536	2539	rBV3	269	148	0.01%	0.001%
60	9.210	2539	2541	2543	rVB2	352	146	0.01%	0.001%
61	9.230	2543	2547	2550	rBV2	542	476	0.03%	0.004%
62	9.262	2555	2557	2559	rBV	381	232	0.01%	0.002%
63	9.307	2567	2571	2573	rBV3	360	282	0.02%	0.002%
64	9.336	2578	2580	2581	rBV	350	150	0.01%	0.001%
65	9.368	2587	2590	2593	rBV2	425	292	0.02%	0.003%
66	9.419	2602	2606	2607	rBV3	252	140	0.01%	0.001%
67	9.481	2623	2625	2626	rBV	361	162	0.01%	0.001%
68	9.497	2627	2630	2633	rVV3	711	401	0.02%	0.003%
69	9.619	2666	2668	2670	rBV	322	150	0.01%	0.001%
70	9.693	2687	2691	2693	rBV3	349	311	0.02%	0.003%
71	9.744	2704	2707	2709	rVB2	280	162	0.01%	0.001%
72	9.808	2722	2727	2731	rBV3	273	278	0.02%	0.002%
73	9.837	2731	2736	2741	rVV2	471	366	0.02%	0.003%
74	9.870	2744	2746	2750	rVV2	500	509	0.03%	0.004%
75	9.905	2754	2757	2759	rVV2	332	178	0.01%	0.002%
76	9.966	2774	2776	2779	rVB2	303	148	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035069.D
 Acq On : 09 Apr 2024 09:51
 Operator : SY/MD
 Sample : VV0409MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.014	2787	2791	2793	rBV	335	244	0.01%	0.002%
78	10.034	2793	2797	2800	rBV3	371	215	0.01%	0.002%
79	10.050	2800	2802	2805	rBV	258	145	0.01%	0.001%
80	10.149	2821	2833	2859	rBV	484685	773874	47.49%	6.708%
81	10.342	2891	2893	2895	rVB2	518	186	0.01%	0.002%
82	10.394	2907	2909	2915	rVB2	484	295	0.02%	0.003%
83	10.423	2915	2918	2920	rVB2	371	206	0.01%	0.002%
84	10.471	2932	2933	2935	rVB2	298	141	0.01%	0.001%
85	10.590	2967	2970	2973	rBV2	266	202	0.01%	0.002%
86	10.731	3007	3014	3017	rBV4	585	749	0.05%	0.006%
87	10.780	3026	3029	3032	rBV2	414	305	0.02%	0.003%
88	11.133	3132	3139	3144	rBV6	1732	2393	0.15%	0.021%
89	11.185	3144	3155	3185	rVV	543340	865633	53.12%	7.504%
90	11.426	3228	3230	3232	rBV	393	206	0.01%	0.002%
91	11.558	3258	3271	3297	rBV	638145	1022127	62.72%	8.860%
92	12.046	3420	3423	3424	rBV	336	195	0.01%	0.002%
93	12.458	3547	3551	3557	rBV3	552	595	0.04%	0.005%
94	12.509	3565	3567	3571	rVB2	473	204	0.01%	0.002%
95	12.590	3587	3592	3594	rBV4	1436	1372	0.08%	0.012%
96	12.683	3619	3621	3625	rBV4	363	281	0.02%	0.002%
97	13.204	3775	3783	3793	rBV5	5814	9981	0.61%	0.087%
98	13.445	3850	3858	3874	rVB	17087	28265	1.73%	0.245%
99	13.683	3926	3932	3941	rVB3	5097	6878	0.42%	0.060%
100	14.522	4191	4193	4198	rBV3	616	540	0.03%	0.005%

Sum of corrected areas: 11535835




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035069.D
Acq On : 09 Apr 2024 09:51
Operator : SY/MD
Sample : VV0409MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

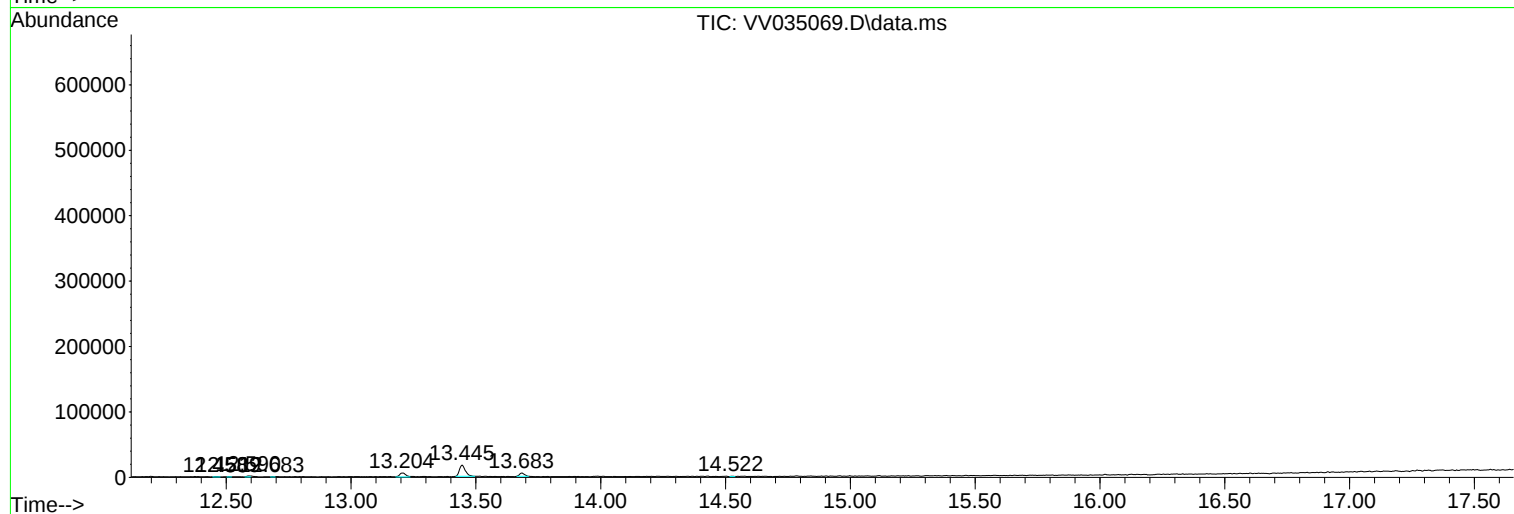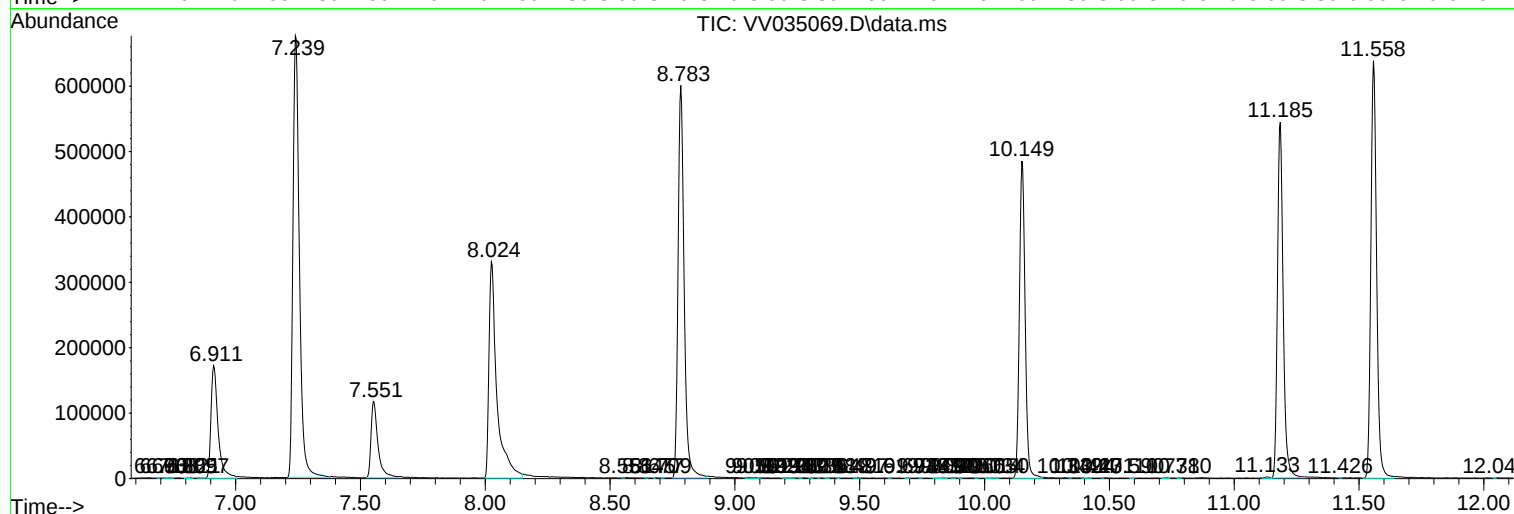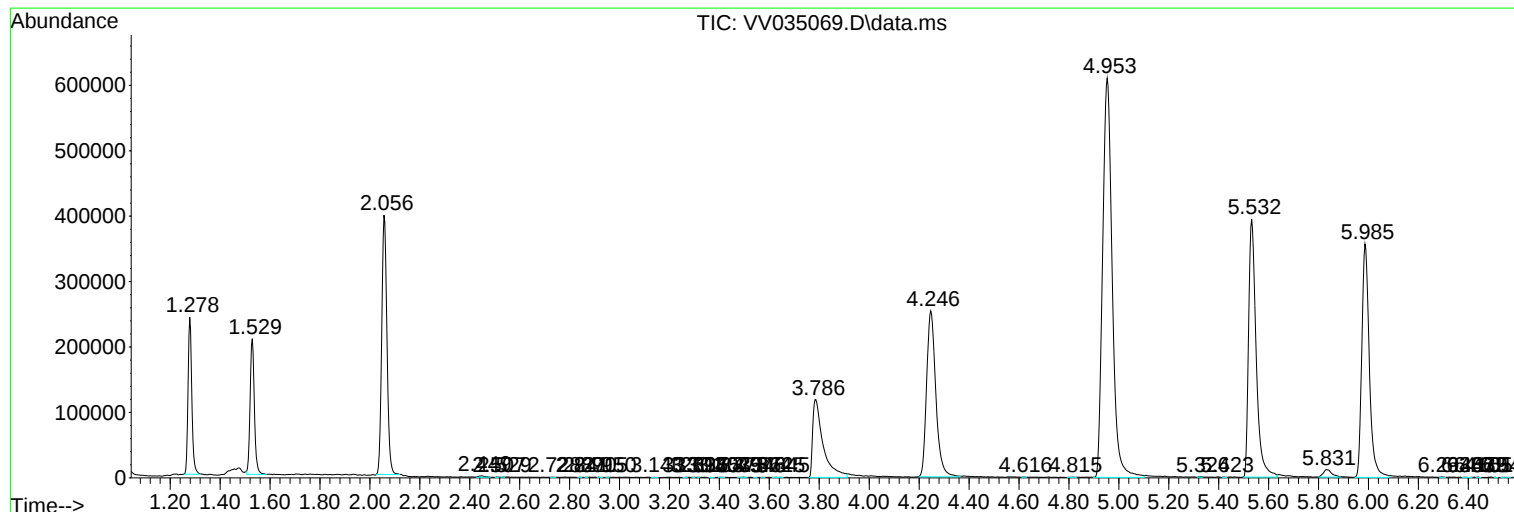

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035069.D
Acq On : 09 Apr 2024 09:51
Operator : SY/MD
Sample : VV0409MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035069.D
Acq On : 09 Apr 2024 09:51
Operator : SY/MD
Sample : VV0409MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc