

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035070.D
 Acq On : 09 Apr 2024 10:15
 Operator : SY/MD
 Sample : VV0409WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	233074	247709	15.56%	2.182%
2	1.529	145	152	169	rVB	201090	236890	14.88%	2.087%
3	2.056	307	316	332	rBV	387268	559300	35.14%	4.927%
4	2.423	427	430	431	rBV2	676	345	0.02%	0.003%
5	2.503	452	455	459	rBV	683	525	0.03%	0.005%
6	2.568	472	475	478	rBV2	366	221	0.01%	0.002%
7	2.584	478	480	487	rVB3	440	419	0.03%	0.004%
8	2.619	489	491	498	rVV4	441	487	0.03%	0.004%
9	2.677	505	509	510	rBV	374	267	0.02%	0.002%
10	2.706	515	518	519	rBV	394	245	0.02%	0.002%
11	2.783	540	542	546	rBV2	329	253	0.02%	0.002%
12	2.873	567	570	572	rBV2	455	323	0.02%	0.003%
13	2.902	577	579	582	rBV2	299	189	0.01%	0.002%
14	2.944	590	592	597	rBV3	295	205	0.01%	0.002%
15	3.024	613	617	622	rBV3	414	458	0.03%	0.004%
16	3.105	640	642	646	rBV3	333	299	0.02%	0.003%
17	3.121	646	647	650	rVB	437	188	0.01%	0.002%
18	3.159	656	659	664	rVB2	382	286	0.02%	0.003%
19	3.204	667	673	677	rBV2	430	391	0.02%	0.003%
20	3.320	705	709	713	rBV2	395	300	0.02%	0.003%
21	3.384	727	729	732	rBV2	238	152	0.01%	0.001%
22	3.407	732	736	738	rVV3	262	184	0.01%	0.002%
23	3.420	738	740	744	rVB	298	160	0.01%	0.001%
24	3.523	768	772	777	rBV2	315	243	0.02%	0.002%
25	3.558	781	783	787	rVB	260	161	0.01%	0.001%
26	3.609	796	799	803	rBV	333	276	0.02%	0.002%
27	3.680	815	821	823	rBV2	339	343	0.02%	0.003%
28	3.744	838	841	845	rVB2	331	306	0.02%	0.003%
29	3.786	845	854	894	rBV	118790	349289	21.94%	3.077%
30	4.246	983	997	1025	rBV	244161	624471	39.23%	5.501%
31	4.812	1171	1173	1177	rBV2	375	278	0.02%	0.002%
32	4.854	1184	1186	1188	rBV2	398	169	0.01%	0.001%
33	4.953	1201	1217	1254	rBV2	591091	1591660	100.00%	14.021%
34	5.249	1306	1309	1312	rBV2	612	476	0.03%	0.004%
35	5.291	1320	1322	1325	rBV2	640	341	0.02%	0.003%
36	5.407	1356	1358	1360	rBV	338	201	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035070.D
 Acq On : 09 Apr 2024 10:15
 Operator : SY/MD
 Sample : VV0409WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1433	rBV	392841	822096	51.65%	7.242%
38	5.834	1477	1491	1507	rBV3	12336	29838	1.87%	0.263%
39	5.985	1522	1538	1573	rBV2	349360	740128	46.50%	6.520%
40	6.307	1636	1638	1642	rVB	725	394	0.02%	0.003%
41	6.326	1642	1644	1646	rBV2	344	174	0.01%	0.002%
42	6.391	1662	1664	1669	rVB2	355	253	0.02%	0.002%
43	6.420	1669	1673	1676	rBV2	515	373	0.02%	0.003%
44	6.458	1683	1685	1691	rVB3	648	376	0.02%	0.003%
45	6.532	1707	1708	1715	rVB2	364	273	0.02%	0.002%
46	6.567	1715	1719	1720	rBV2	322	237	0.01%	0.002%
47	6.674	1749	1752	1753	rBV2	239	145	0.01%	0.001%
48	6.712	1762	1764	1767	rBV2	522	324	0.02%	0.003%
49	6.748	1771	1775	1779	rVB3	666	510	0.03%	0.004%
50	6.776	1782	1784	1785	rBV	334	155	0.01%	0.001%
51	6.857	1807	1809	1814	rVB2	296	194	0.01%	0.002%
52	6.912	1814	1826	1857	rBV	170764	332403	20.88%	2.928%
53	7.243	1918	1929	1960	rBV	663459	1184056	74.39%	10.430%
54	7.555	2016	2026	2053	rBV	114688	219242	13.77%	1.931%
55	7.860	2117	2121	2125	rBV3	557	455	0.03%	0.004%
56	7.934	2140	2144	2146	rBV3	485	357	0.02%	0.003%
57	7.956	2149	2151	2154	rBV3	307	151	0.01%	0.001%
58	7.985	2157	2160	2163	rBV4	596	365	0.02%	0.003%
59	8.024	2163	2172	2211	rBV2	330472	736433	46.27%	6.487%
60	8.455	2304	2306	2311	rBV3	644	522	0.03%	0.005%
61	8.783	2397	2408	2442	rBV	604759	1006119	63.21%	8.863%
62	9.024	2481	2483	2487	rVB3	730	360	0.02%	0.003%
63	9.088	2499	2503	2505	rBV2	758	568	0.04%	0.005%
64	9.130	2514	2516	2518	rVB2	453	189	0.01%	0.002%
65	9.165	2525	2527	2531	rVB2	653	442	0.03%	0.004%
66	9.191	2532	2535	2539	rBV	340	203	0.01%	0.002%
67	9.217	2539	2543	2544	rBV2	747	415	0.03%	0.004%
68	9.239	2548	2550	2552	rVV2	299	143	0.01%	0.001%
69	9.265	2556	2558	2560	rBV	466	229	0.01%	0.002%
70	9.329	2576	2578	2580	rVB2	383	160	0.01%	0.001%
71	9.349	2580	2584	2588	rBV	424	437	0.03%	0.004%
72	9.506	2625	2633	2636	rBV2	608	652	0.04%	0.006%
73	9.529	2638	2640	2642	rVB	334	144	0.01%	0.001%
74	9.580	2651	2656	2658	rVB3	436	358	0.02%	0.003%
75	9.603	2658	2663	2665	rBV	452	323	0.02%	0.003%
76	9.760	2710	2712	2715	rBV2	536	339	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035070.D
 Acq On : 09 Apr 2024 10:15
 Operator : SY/MD
 Sample : VV0409WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.799	2721	2724	2726	rVB2	368	163	0.01%	0.001%
78	9.918	2758	2761	2763	rBV2	358	234	0.01%	0.002%
79	9.950	2768	2771	2775	rBV2	185	165	0.01%	0.001%
80	10.027	2789	2795	2799	rBV	395	545	0.03%	0.005%
81	10.091	2812	2815	2818	rBV2	237	178	0.01%	0.002%
82	10.149	2822	2833	2857	rVV	486360	762286	47.89%	6.715%
83	10.519	2947	2948	2953	rVB	497	275	0.02%	0.002%
84	10.593	2969	2971	2972	rBV	413	173	0.01%	0.002%
85	10.783	3027	3030	3031	rBV2	326	208	0.01%	0.002%
86	10.960	3081	3085	3090	rBV3	452	530	0.03%	0.005%
87	10.998	3095	3097	3099	rBV2	410	168	0.01%	0.001%
88	11.114	3129	3133	3134	rBV	509	306	0.02%	0.003%
89	11.185	3143	3155	3178	rBV	533907	854613	53.69%	7.528%
90	11.497	3250	3252	3255	rBV3	306	147	0.01%	0.001%
91	11.558	3259	3271	3292	rBV	640144	1012030	63.58%	8.915%
92	12.001	3404	3409	3412	rBV4	602	679	0.04%	0.006%
93	12.040	3419	3421	3423	rBV	376	191	0.01%	0.002%
94	12.152	3453	3456	3459	rBV2	530	497	0.03%	0.004%
95	12.503	3563	3565	3570	rBV2	311	236	0.01%	0.002%
96	12.596	3592	3594	3595	rBV2	607	251	0.02%	0.002%
97	12.689	3619	3623	3625	rBV	362	294	0.02%	0.003%
98	13.204	3778	3783	3799	rVB6	3796	6579	0.41%	0.058%
99	13.451	3854	3860	3872	rVB3	5704	9058	0.57%	0.080%
100	13.689	3926	3934	3942	rBV6	2855	3985	0.25%	0.035%




Sum of corrected areas: 11352336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035070.D
Acq On : 09 Apr 2024 10:15
Operator : SY/MD
Sample : VV0409WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

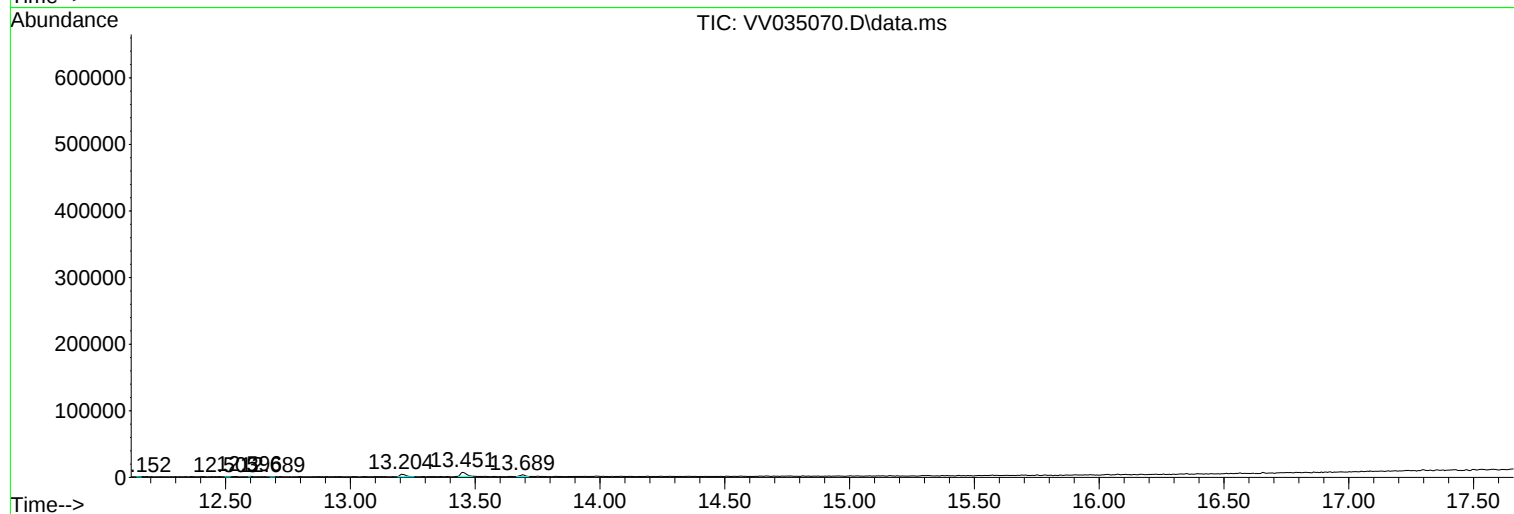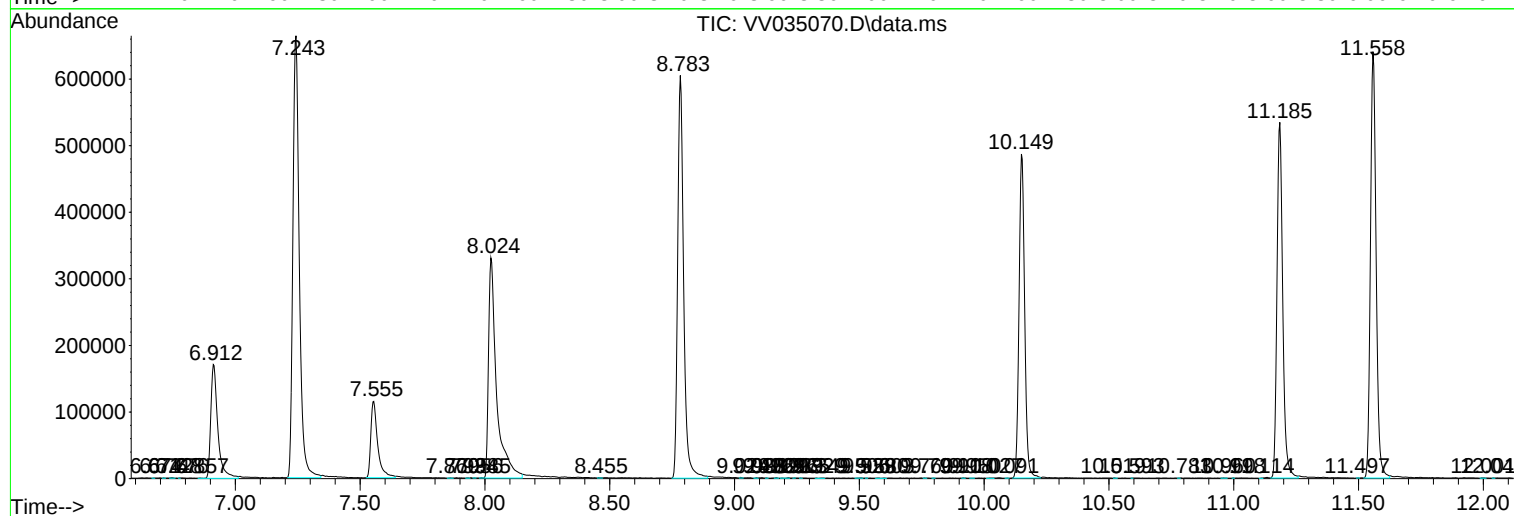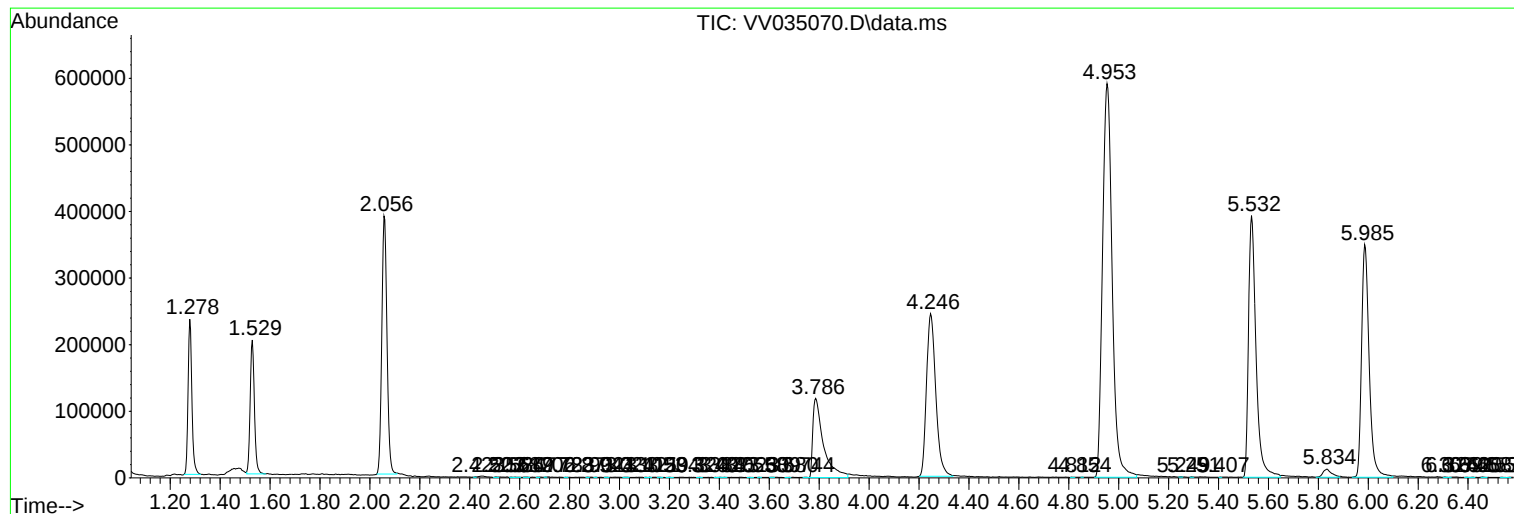

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035070.D
Acq On : 09 Apr 2024 10:15
Operator : SY/MD
Sample : VV0409WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035070.D
Acq On : 09 Apr 2024 10:15
Operator : SY/MD
Sample : VV0409WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
