

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035071.D
 Acq On : 09 Apr 2024 10:39
 Operator : SY/MD
 Sample : PB160061TB
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VLEB061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	231410	245160	15.31%	2.149%
2	1.529	145	152	169	rVB	204764	244925	15.29%	2.147%
3	2.056	307	316	333	rBV	385454	562983	35.15%	4.935%
4	2.449	428	438	451	rBV2	18761	31095	1.94%	0.273%
5	2.522	459	461	463	rBV2	585	296	0.02%	0.003%
6	2.699	508	516	517	rBV4	542	670	0.04%	0.006%
7	2.751	528	532	533	rBV	501	300	0.02%	0.003%
8	2.940	587	591	595	rVB	291	216	0.01%	0.002%
9	2.960	595	597	599	rBV2	635	272	0.02%	0.002%
10	3.182	664	666	668	rBV	278	121	0.01%	0.001%
11	3.243	683	685	690	rVB2	246	121	0.01%	0.001%
12	3.275	690	695	697	rBV2	398	360	0.02%	0.003%
13	3.355	715	720	724	rBV2	517	497	0.03%	0.004%
14	3.481	757	759	761	rBV2	342	164	0.01%	0.001%
15	3.516	768	770	771	rBV2	145	68	0.00%	0.001%
16	3.551	779	781	783	rBV	165	91	0.01%	0.001%
17	3.561	783	784	787	rVB3	282	130	0.01%	0.001%
18	3.616	797	801	802	rBV2	626	339	0.02%	0.003%
19	3.645	808	810	816	rVB2	416	265	0.02%	0.002%
20	3.690	822	824	827	rBV2	222	139	0.01%	0.001%
21	3.709	828	830	833	rVB2	284	114	0.01%	0.001%
22	3.747	839	842	845	rBV2	344	279	0.02%	0.002%
23	3.786	846	854	894	rBV	120765	353695	22.08%	3.101%
24	4.246	982	997	1028	rBV	245614	635951	39.71%	5.575%
25	4.680	1128	1132	1135	rBV2	626	422	0.03%	0.004%
26	4.780	1160	1163	1164	rBV2	280	161	0.01%	0.001%
27	4.825	1175	1177	1182	rBV5	516	296	0.02%	0.003%
28	4.953	1200	1217	1260	rBV2	606220	1601524	100.00%	14.040%
29	5.329	1331	1334	1335	rBV3	509	285	0.02%	0.002%
30	5.426	1359	1364	1365	rBV2	614	425	0.03%	0.004%
31	5.484	1379	1382	1384	rBV	527	318	0.02%	0.003%
32	5.532	1387	1397	1442	rVV	390296	822465	51.36%	7.210%
33	5.831	1482	1490	1509	rVB4	14250	30940	1.93%	0.271%
34	5.985	1525	1538	1573	rBV	349630	740505	46.24%	6.492%
35	6.362	1653	1655	1657	rBV2	539	262	0.02%	0.002%
36	6.407	1666	1669	1672	rBV	617	425	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035071.D
 Acq On : 09 Apr 2024 10:39
 Operator : SY/MD
 Sample : PB160061TB
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VLEB061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.455	1682	1684	1689	rVB4	398	279	0.02%	0.002%
38	6.509	1700	1701	1702	rBV2	121	43	0.00%	0.000%
39	6.554	1713	1715	1718	rBV	270	193	0.01%	0.002%
40	6.587	1723	1725	1728	rBV	307	215	0.01%	0.002%
41	6.612	1729	1733	1735	rBV3	486	324	0.02%	0.003%
42	6.702	1760	1761	1764	rBV3	466	200	0.01%	0.002%
43	6.722	1764	1767	1769	rVB3	734	324	0.02%	0.003%
44	6.870	1810	1813	1816	rVB	316	219	0.01%	0.002%
45	6.911	1816	1826	1855	rBV	168449	334006	20.86%	2.928%
46	7.243	1918	1929	1958	rBV	667504	1180204	73.69%	10.346%
47	7.551	2017	2025	2057	rBV	116225	222670	13.90%	1.952%
48	7.908	2133	2136	2137	rBV2	351	178	0.01%	0.002%
49	7.940	2144	2146	2148	rBV2	291	180	0.01%	0.002%
50	8.024	2163	2172	2220	rBV2	330305	736690	46.00%	6.458%
51	8.506	2320	2322	2327	rVB2	1022	650	0.04%	0.006%
52	8.619	2354	2357	2361	rVB4	468	309	0.02%	0.003%
53	8.638	2361	2363	2366	rBV2	428	200	0.01%	0.002%
54	8.783	2397	2408	2444	rBV	591465	1005221	62.77%	8.812%
55	9.252	2551	2554	2558	rVB4	745	596	0.04%	0.005%
56	9.271	2558	2560	2561	rBV4	167	80	0.00%	0.001%
57	9.316	2571	2574	2576	rBV3	511	267	0.02%	0.002%
58	9.355	2583	2586	2592	rVB3	663	525	0.03%	0.005%
59	9.387	2592	2596	2602	rBV4	390	408	0.03%	0.004%
60	9.477	2622	2624	2626	rBV	301	151	0.01%	0.001%
61	9.493	2627	2629	2630	rBV	373	133	0.01%	0.001%
62	9.612	2664	2666	2670	rBV3	297	207	0.01%	0.002%
63	9.641	2673	2675	2676	rBV2	141	39	0.00%	0.000%
64	9.670	2680	2684	2686	rBV3	561	445	0.03%	0.004%
65	9.696	2690	2692	2695	rBV2	306	180	0.01%	0.002%
66	9.728	2699	2702	2706	rBV3	473	344	0.02%	0.003%
67	9.895	2753	2754	2755	rBV3	234	77	0.00%	0.001%
68	9.950	2768	2771	2774	rBV2	287	203	0.01%	0.002%
69	9.972	2776	2778	2780	rBV	151	75	0.00%	0.001%
70	9.985	2780	2782	2783	rBV	242	98	0.01%	0.001%
71	10.030	2794	2796	2799	rBV2	267	142	0.01%	0.001%
72	10.053	2799	2803	2804	rBV	361	243	0.02%	0.002%
73	10.149	2822	2833	2857	rBV	471586	750661	46.87%	6.581%
74	10.564	2961	2962	2966	rBV	342	155	0.01%	0.001%
75	10.628	2979	2982	2984	rBV2	286	144	0.01%	0.001%
76	10.792	3031	3033	3035	rBV2	741	266	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035071.D
 Acq On : 09 Apr 2024 10:39
 Operator : SY/MD
 Sample : PB160061TB
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VLEB061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.840	3046	3048	3052	rBV2	331	254	0.02%	0.002%
78	10.950	3080	3082	3087	rBV2	569	512	0.03%	0.004%
79	11.114	3128	3133	3134	rBV	548	363	0.02%	0.003%
80	11.130	3135	3138	3144	rVB5	775	579	0.04%	0.005%
81	11.184	3144	3155	3180	rBV	541287	861023	53.76%	7.548%
82	11.557	3258	3271	3297	rBV	632461	1019790	63.68%	8.940%
83	11.882	3368	3372	3376	rBV3	857	711	0.04%	0.006%
84	12.596	3592	3594	3595	rBV3	490	180	0.01%	0.002%
85	12.715	3628	3631	3632	rBV	432	220	0.01%	0.002%
86	12.847	3670	3672	3678	rVB4	543	404	0.03%	0.004%
87	12.953	3704	3705	3706	rBV4	353	123	0.01%	0.001%
88	13.056	3735	3737	3739	rBV2	477	260	0.02%	0.002%
89	13.210	3778	3785	3799	rVB6	2733	4732	0.30%	0.041%
90	13.455	3855	3861	3869	rBV2	2809	3993	0.25%	0.035%




Sum of corrected areas: 11406967

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035071.D
Acq On : 09 Apr 2024 10:39
Operator : SY/MD
Sample : PB160061TB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VLEB061

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

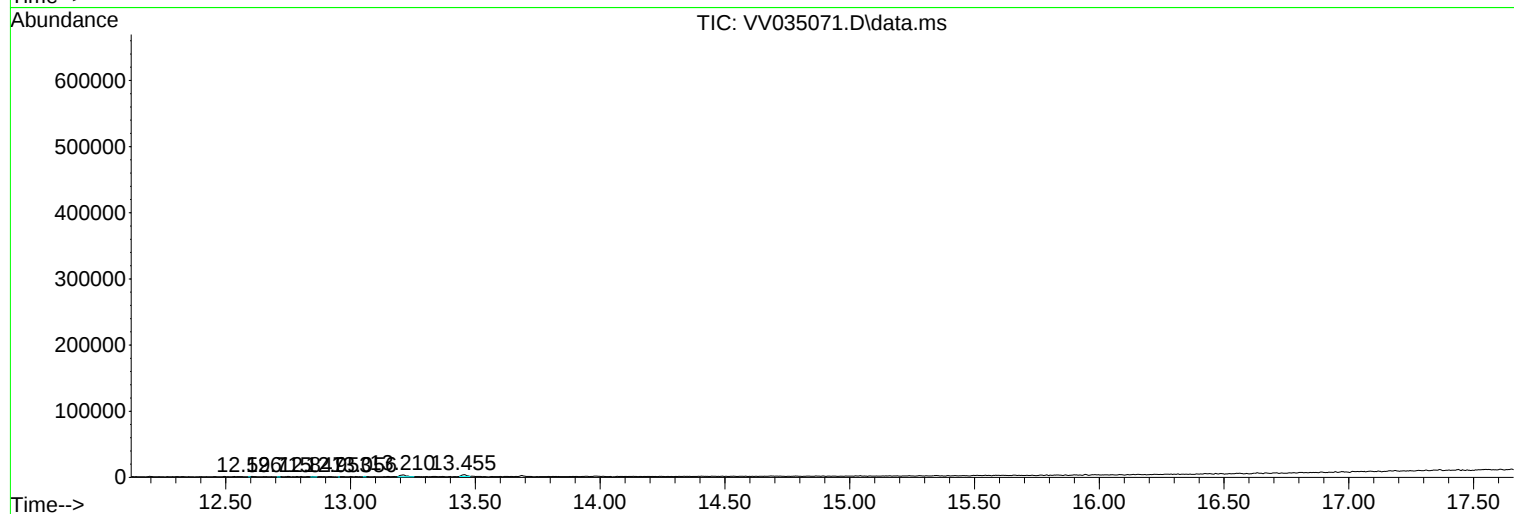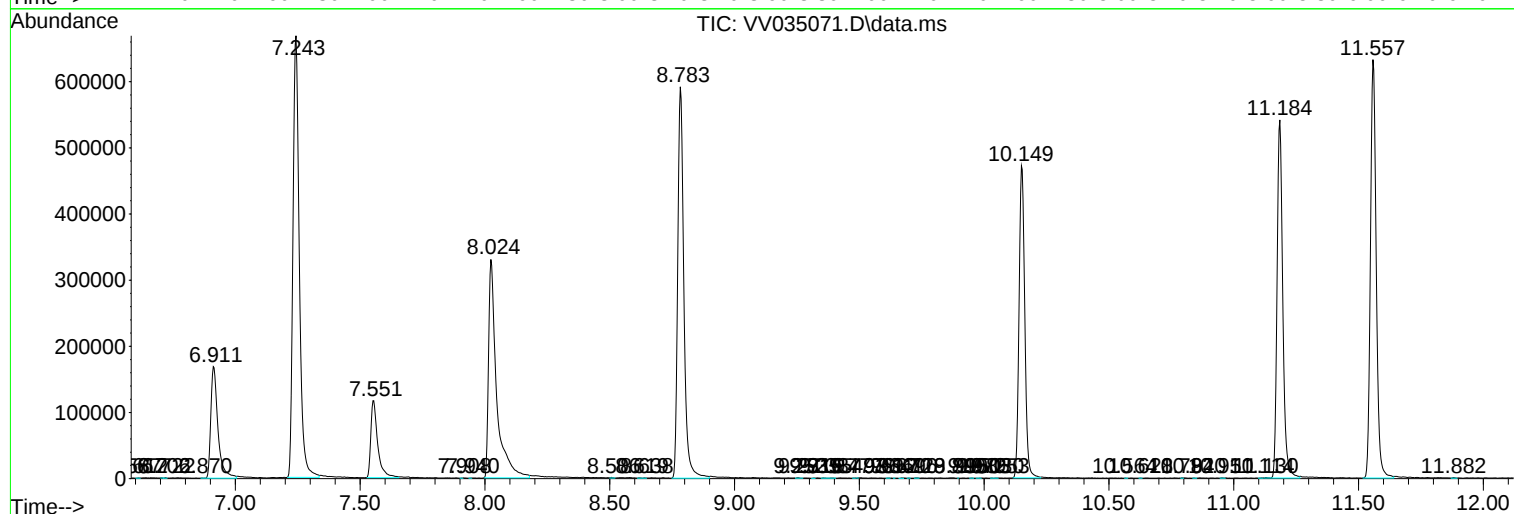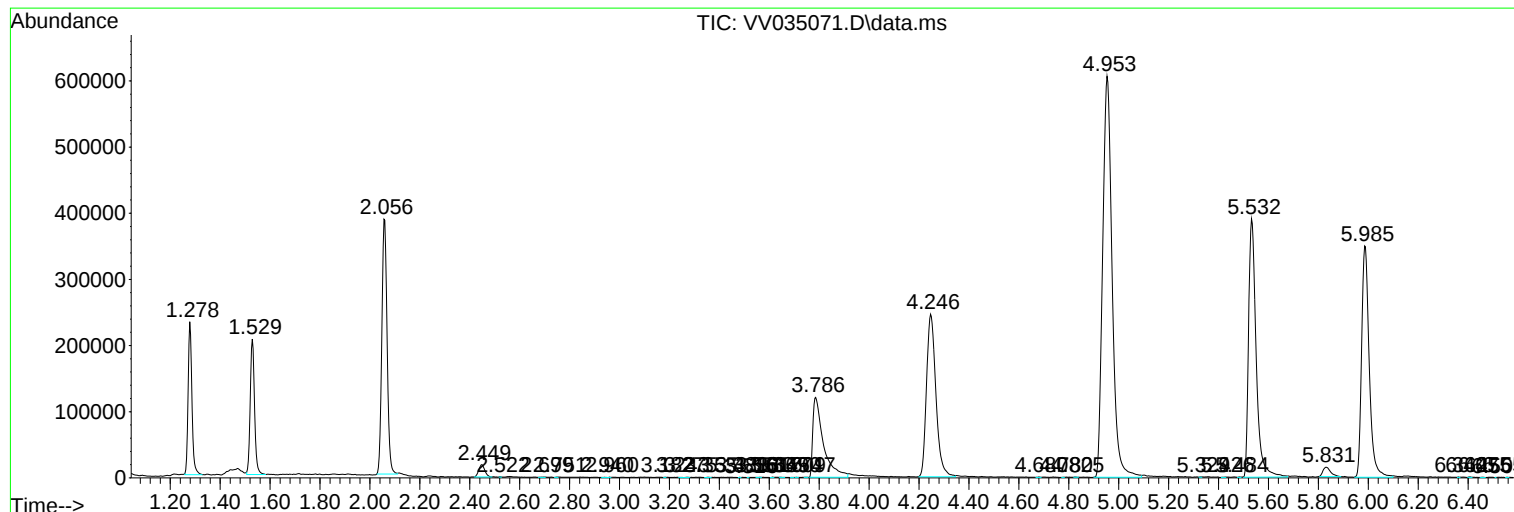

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035071.D
Acq On : 09 Apr 2024 10:39
Operator : SY/MD
Sample : PB160061TB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VLEB061

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035071.D
Acq On : 09 Apr 2024 10:39
Operator : SY/MD
Sample : PB160061TB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VLEB061

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc