

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035074.D
 Acq On : 09 Apr 2024 11:51
 Operator : SY/MD
 Sample : P2009-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	190762	202130	13.85%	1.956%
2	1.529	146	152	177	rVB	199033	239742	16.43%	2.320%
3	2.056	307	316	330	rBV	319012	464589	31.83%	4.495%
4	2.481	446	448	451	rVB2	437	213	0.01%	0.002%
5	2.516	457	459	463	rBV3	623	318	0.02%	0.003%
6	2.796	545	546	548	rBV	295	129	0.01%	0.001%
7	2.876	568	571	576	rVB2	401	322	0.02%	0.003%
8	2.899	576	578	579	rBV2	228	115	0.01%	0.001%
9	2.970	598	600	605	rBV2	513	421	0.03%	0.004%
10	2.989	605	606	609	rVV	300	117	0.01%	0.001%
11	3.117	642	646	647	rBV2	190	137	0.01%	0.001%
12	3.195	668	670	673	rBV2	237	145	0.01%	0.001%
13	3.214	673	676	678	rVV	219	136	0.01%	0.001%
14	3.230	679	681	684	rVB2	430	204	0.01%	0.002%
15	3.256	684	689	697	rBV3	672	750	0.05%	0.007%
16	3.310	703	706	708	rBV2	340	204	0.01%	0.002%
17	3.375	723	726	730	rVB	372	243	0.02%	0.002%
18	3.461	749	753	755	rBV2	305	256	0.02%	0.002%
19	3.580	786	790	792	rVB	287	154	0.01%	0.001%
20	3.645	807	810	812	rBV2	360	229	0.02%	0.002%
21	3.687	821	823	826	rBV	210	131	0.01%	0.001%
22	3.789	846	855	895	rBV	120723	367227	25.16%	3.553%
23	4.246	982	997	1033	rBV	225379	581832	39.86%	5.630%
24	4.571	1097	1098	1101	rBV	391	191	0.01%	0.002%
25	4.635	1115	1118	1121	rBV3	651	426	0.03%	0.004%
26	4.693	1132	1136	1138	rBV2	315	216	0.01%	0.002%
27	4.767	1157	1159	1160	rBV2	284	145	0.01%	0.001%
28	4.953	1200	1217	1255	rBV2	550031	1459548	100.00%	14.122%
29	5.304	1323	1326	1330	rBV5	553	547	0.04%	0.005%
30	5.359	1340	1343	1346	rVB4	606	439	0.03%	0.004%
31	5.429	1363	1365	1366	rBV2	338	133	0.01%	0.001%
32	5.532	1386	1397	1432	rBV	339253	718972	49.26%	6.957%
33	5.838	1482	1492	1509	rVB3	10958	25243	1.73%	0.244%
34	5.985	1525	1538	1566	rBV	323673	683501	46.83%	6.613%
35	6.285	1628	1631	1635	rVB5	346	239	0.02%	0.002%
36	6.413	1667	1671	1675	rBV3	448	432	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035074.D
 Acq On : 09 Apr 2024 11:51
 Operator : SY/MD
 Sample : P2009-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.432	1675	1677	1679	rBV	309	151	0.01%	0.001%
38	6.458	1684	1685	1687	rBV	524	218	0.01%	0.002%
39	6.494	1692	1696	1697	rBV2	423	273	0.02%	0.003%
40	6.522	1701	1705	1707	rBV2	238	216	0.01%	0.002%
41	6.551	1711	1714	1716	rBV2	333	207	0.01%	0.002%
42	6.629	1736	1738	1746	rVB7	787	855	0.06%	0.008%
43	6.690	1755	1757	1759	rBV2	430	154	0.01%	0.001%
44	6.728	1766	1769	1770	rBV2	252	146	0.01%	0.001%
45	6.741	1770	1773	1776	rVV3	665	488	0.03%	0.005%
46	6.847	1803	1806	1809	rVB	370	151	0.01%	0.001%
47	6.873	1809	1814	1816	rBV3	429	378	0.03%	0.004%
48	6.915	1816	1827	1861	rBV	155005	309457	21.20%	2.994%
49	7.243	1918	1929	1955	rBV	571610	1028198	70.45%	9.949%
50	7.555	2017	2026	2054	rBV	108881	207341	14.21%	2.006%
51	7.857	2118	2120	2123	rBV2	292	208	0.01%	0.002%
52	7.876	2123	2126	2127	rBV2	423	279	0.02%	0.003%
53	7.960	2150	2152	2158	rVB3	409	350	0.02%	0.003%
54	7.982	2158	2159	2163	rBV2	501	291	0.02%	0.003%
55	8.027	2163	2173	2219	rBV2	331047	750437	51.42%	7.261%
56	8.596	2348	2350	2352	rBV3	400	195	0.01%	0.002%
57	8.709	2383	2385	2388	rBV3	370	247	0.02%	0.002%
58	8.783	2397	2408	2438	rBV	531147	887258	60.79%	8.585%
59	9.175	2526	2530	2531	rBV3	528	341	0.02%	0.003%
60	9.288	2563	2565	2567	rBV2	242	150	0.01%	0.001%
61	9.313	2569	2573	2578	rVB3	391	416	0.03%	0.004%
62	9.358	2584	2587	2589	rVB2	441	247	0.02%	0.002%
63	9.378	2591	2593	2594	rBV	445	175	0.01%	0.002%
64	9.442	2611	2613	2614	rBV	447	158	0.01%	0.002%
65	9.493	2627	2629	2631	rBV2	329	171	0.01%	0.002%
66	9.542	2641	2644	2646	rBV	313	201	0.01%	0.002%
67	9.709	2694	2696	2700	rVB2	206	142	0.01%	0.001%
68	9.735	2700	2704	2706	rBV2	272	163	0.01%	0.002%
69	9.744	2706	2707	2710	rVV	221	145	0.01%	0.001%
70	9.760	2710	2712	2715	rVV2	366	189	0.01%	0.002%
71	9.786	2717	2720	2727	rVB3	509	398	0.03%	0.004%
72	9.828	2732	2733	2736	rBV	213	112	0.01%	0.001%
73	10.030	2792	2796	2798	rBV2	280	181	0.01%	0.002%
74	10.046	2798	2801	2804	rBV2	175	129	0.01%	0.001%
75	10.062	2804	2806	2809	rBV2	296	163	0.01%	0.002%
76	10.104	2817	2819	2821	rBV	277	125	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035074.D
 Acq On : 09 Apr 2024 11:51
 Operator : SY/MD
 Sample : P2009-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.149	2822	2833	2868	rBV	462105	745043	51.05%	7.209%
78	10.365	2898	2900	2902	rBV	264	127	0.01%	0.001%
79	10.554	2956	2959	2963	rBV	465	328	0.02%	0.003%
80	10.587	2967	2969	2970	rBV	335	143	0.01%	0.001%
81	10.651	2986	2989	2990	rBV	234	123	0.01%	0.001%
82	10.689	2999	3001	3003	rVB2	373	151	0.01%	0.001%
83	10.757	3019	3022	3027	rBV3	535	338	0.02%	0.003%
84	10.805	3034	3037	3041	rBV3	312	324	0.02%	0.003%
85	11.043	3108	3111	3113	rBV2	438	273	0.02%	0.003%
86	11.101	3127	3129	3133	rBV2	428	266	0.02%	0.003%
87	11.120	3133	3135	3138	rBV2	324	186	0.01%	0.002%
88	11.185	3144	3155	3184	rBV	464843	747115	51.19%	7.229%
89	11.558	3260	3271	3291	rBV	563059	893650	61.23%	8.647%
90	11.847	3359	3361	3363	rBV3	427	179	0.01%	0.002%
91	11.915	3380	3382	3384	rBV	418	162	0.01%	0.002%
92	11.943	3389	3391	3394	rBV	580	321	0.02%	0.003%
93	12.300	3500	3502	3503	rVB	419	121	0.01%	0.001%
94	12.355	3517	3519	3522	rBV2	373	185	0.01%	0.002%
95	12.445	3544	3547	3549	rBV	439	231	0.02%	0.002%
96	12.619	3599	3601	3604	rVB2	463	192	0.01%	0.002%
97	13.159	3767	3769	3771	rBV2	539	302	0.02%	0.003%
98	13.210	3779	3785	3795	rBV8	2230	3897	0.27%	0.038%
99	13.345	3824	3827	3830	rBV2	535	363	0.02%	0.004%
100	13.394	3840	3842	3843	rBV	410	128	0.01%	0.001%




Sum of corrected areas: 10335028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035074.D
Acq On : 09 Apr 2024 11:51
Operator : SY/MD
Sample : P2009-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

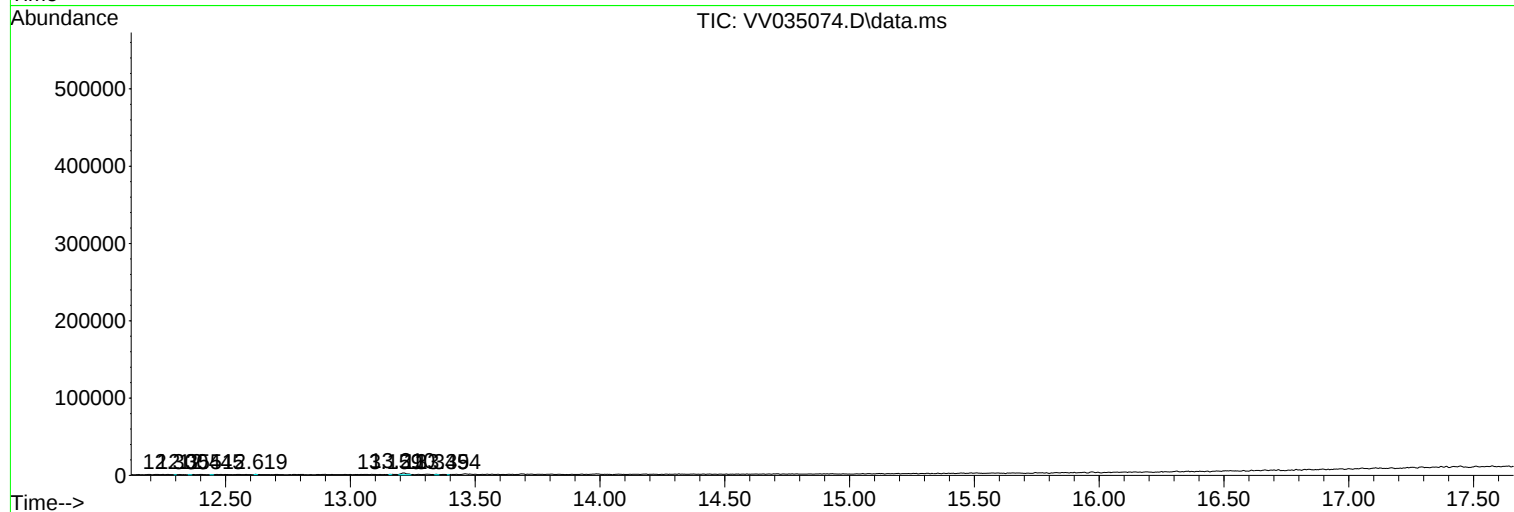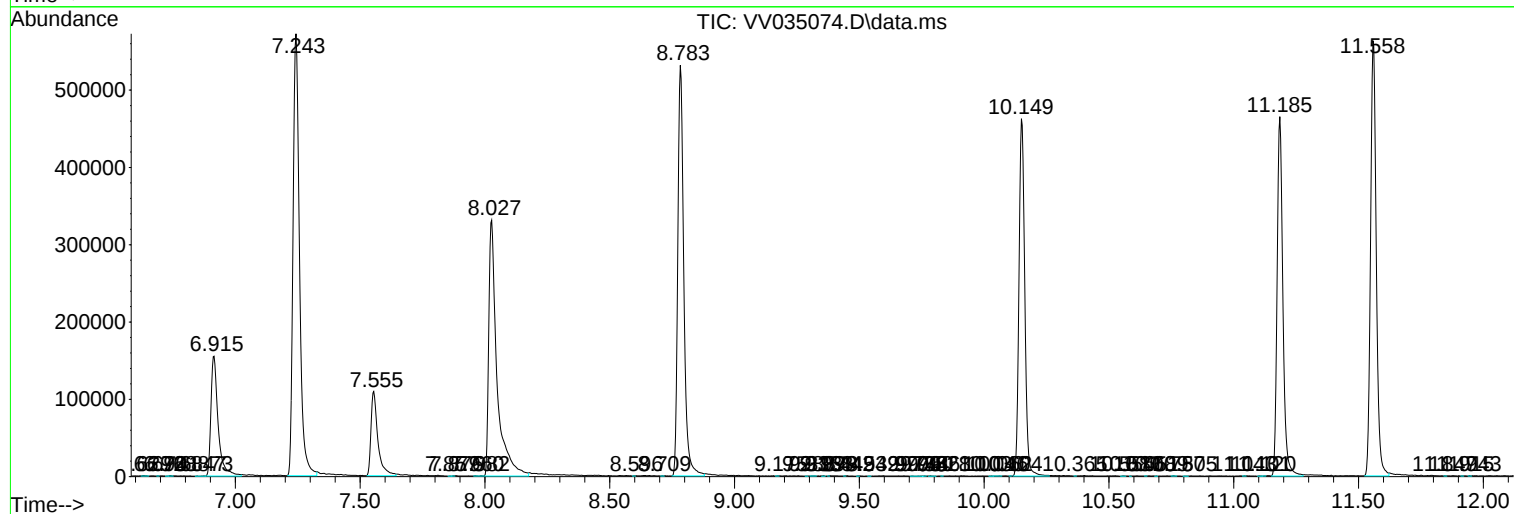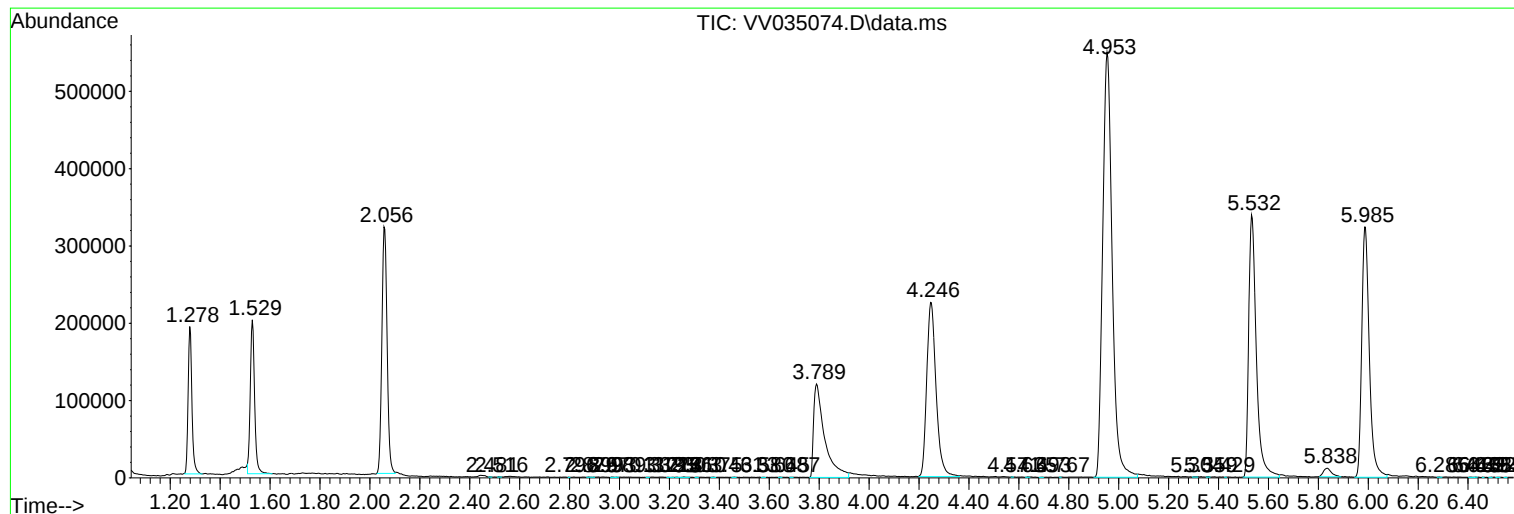

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035074.D
Acq On : 09 Apr 2024 11:51
Operator : SY/MD
Sample : P2009-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035074.D
Acq On : 09 Apr 2024 11:51
Operator : SY/MD
Sample : P2009-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------