

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035075.D
 Acq On : 09 Apr 2024 12:15
 Operator : SY/MD
 Sample : P2017-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rBV	212217	223121	14.27%	1.982%
2	1.532	146	153	168	rBV	209666	242950	15.54%	2.158%
3	2.060	307	317	331	rBV	361923	527593	33.75%	4.686%
4	2.349	405	407	409	rBV	768	456	0.03%	0.004%
5	2.449	429	438	456	rVB	35553	61369	3.93%	0.545%
6	2.532	462	464	468	rVB4	624	310	0.02%	0.003%
7	2.610	484	488	494	rBV5	704	638	0.04%	0.006%
8	2.635	494	496	500	rVB2	452	366	0.02%	0.003%
9	2.754	530	533	535	rBV2	365	177	0.01%	0.002%
10	3.028	615	618	620	rBV2	421	175	0.01%	0.002%
11	3.085	632	636	638	rBV	297	245	0.02%	0.002%
12	3.137	650	652	655	rBV2	273	157	0.01%	0.001%
13	3.169	660	662	664	rBV	248	166	0.01%	0.001%
14	3.233	679	682	684	rBV	330	247	0.02%	0.002%
15	3.294	697	701	705	rVB3	529	408	0.03%	0.004%
16	3.320	705	709	710	rBV	462	187	0.01%	0.002%
17	3.346	716	717	720	rBV2	392	171	0.01%	0.002%
18	3.397	729	733	735	rBV4	434	384	0.02%	0.003%
19	3.465	751	754	757	rVB3	345	223	0.01%	0.002%
20	3.622	801	803	804	rVV	270	126	0.01%	0.001%
21	3.796	848	857	891	rBV	102119	324828	20.78%	2.885%
22	4.188	977	979	980	rBV2	640	326	0.02%	0.003%
23	4.246	984	997	1036	rVB	242471	629744	40.28%	5.594%
24	4.706	1137	1140	1141	rBV2	335	167	0.01%	0.001%
25	4.738	1149	1150	1154	rBV2	565	212	0.01%	0.002%
26	4.825	1173	1177	1181	rBV2	422	476	0.03%	0.004%
27	4.953	1201	1217	1249	rBV2	589407	1563278	100.00%	13.886%
28	5.381	1348	1350	1351	rBV	765	349	0.02%	0.003%
29	5.532	1386	1397	1435	rBV	399401	838138	53.61%	7.445%
30	5.834	1481	1491	1507	rBV4	11401	27227	1.74%	0.242%
31	5.928	1518	1520	1525	rVB3	516	397	0.03%	0.004%
32	5.986	1525	1538	1576	rBV	348928	734695	47.00%	6.526%
33	6.249	1618	1620	1624	rBV3	688	429	0.03%	0.004%
34	6.310	1636	1639	1643	rBV3	437	369	0.02%	0.003%
35	6.333	1643	1646	1647	rBV2	676	275	0.02%	0.002%
36	6.381	1658	1661	1665	rBV3	636	560	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035075.D
 Acq On : 09 Apr 2024 12:15
 Operator : SY/MD
 Sample : P2017-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.484	1691	1693	1697	rBV2	658	445	0.03%	0.004%
38	6.510	1697	1701	1706	rVB3	525	496	0.03%	0.004%
39	6.539	1706	1710	1712	rBV2	208	152	0.01%	0.001%
40	6.561	1715	1717	1720	rBV2	541	169	0.01%	0.002%
41	6.609	1728	1732	1734	rBV3	503	371	0.02%	0.003%
42	6.728	1767	1769	1770	rBV	386	135	0.01%	0.001%
43	6.786	1786	1787	1791	rBV2	208	126	0.01%	0.001%
44	6.841	1801	1804	1806	rBV2	274	153	0.01%	0.001%
45	6.863	1809	1811	1815	rVB3	489	246	0.02%	0.002%
46	6.912	1815	1826	1853	rBV	167997	328174	20.99%	2.915%
47	7.243	1917	1929	1961	rBV	648302	1165564	74.56%	10.353%
48	7.551	2017	2025	2045	rBV	113928	212730	13.61%	1.890%
49	7.876	2122	2126	2132	rVB3	939	831	0.05%	0.007%
50	7.902	2132	2134	2137	rBV2	226	136	0.01%	0.001%
51	7.979	2156	2158	2161	rBV2	431	228	0.01%	0.002%
52	8.027	2164	2173	2210	rBV2	309500	712294	45.56%	6.327%
53	8.529	2326	2329	2331	rBV3	647	443	0.03%	0.004%
54	8.670	2372	2373	2376	rVB	593	205	0.01%	0.002%
55	8.686	2376	2378	2381	rBV2	566	413	0.03%	0.004%
56	8.719	2385	2388	2391	rVB3	512	346	0.02%	0.003%
57	8.783	2397	2408	2436	rBV	602233	1011752	64.72%	8.987%
58	9.063	2494	2495	2496	rBV	565	156	0.01%	0.001%
59	9.156	2519	2524	2525	rBV	656	370	0.02%	0.003%
60	9.185	2530	2533	2535	rBV2	590	301	0.02%	0.003%
61	9.227	2544	2546	2549	rVB	300	182	0.01%	0.002%
62	9.297	2565	2568	2571	rBV2	391	214	0.01%	0.002%
63	9.362	2586	2588	2591	rBV2	224	151	0.01%	0.001%
64	9.394	2595	2598	2601	rVB3	286	219	0.01%	0.002%
65	9.452	2613	2616	2619	rBV4	383	241	0.02%	0.002%
66	9.487	2623	2627	2629	rBV2	1076	866	0.06%	0.008%
67	9.535	2639	2642	2644	rVB3	372	226	0.01%	0.002%
68	9.619	2666	2668	2671	rBV3	323	228	0.01%	0.002%
69	9.648	2675	2677	2679	rVB	327	124	0.01%	0.001%
70	9.699	2690	2693	2696	rVB	310	136	0.01%	0.001%
71	9.738	2703	2705	2709	rVV2	277	165	0.01%	0.001%
72	9.834	2731	2735	2737	rBV3	341	217	0.01%	0.002%
73	9.886	2748	2751	2753	rVB3	363	200	0.01%	0.002%
74	9.985	2779	2782	2784	rBV2	246	147	0.01%	0.001%
75	10.063	2803	2806	2808	rBV2	443	203	0.01%	0.002%
76	10.149	2820	2833	2859	rBV	475144	756471	48.39%	6.719%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035075.D
 Acq On : 09 Apr 2024 12:15
 Operator : SY/MD
 Sample : P2017-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.477	2933	2935	2939	rVB2	479	296	0.02%	0.003%
78	10.510	2943	2945	2948	rBV	242	133	0.01%	0.001%
79	10.719	3008	3010	3012	rBB	522	238	0.02%	0.002%
80	10.744	3012	3018	3022	rBV3	451	391	0.03%	0.003%
81	10.786	3029	3031	3033	rBV2	428	218	0.01%	0.002%
82	10.831	3042	3045	3046	rBV	276	184	0.01%	0.002%
83	10.886	3059	3062	3064	rBV	340	173	0.01%	0.002%
84	10.960	3082	3085	3089	rBV2	323	223	0.01%	0.002%
85	11.037	3106	3109	3112	rBV	360	245	0.02%	0.002%
86	11.085	3122	3124	3127	rBV2	494	232	0.01%	0.002%
87	11.117	3132	3134	3135	rBV2	481	168	0.01%	0.001%
88	11.185	3143	3155	3187	rBV	540601	874228	55.92%	7.765%
89	11.506	3251	3255	3258	rBV2	320	231	0.01%	0.002%
90	11.558	3259	3271	3291	rBV	634025	998649	63.88%	8.871%
91	12.050	3417	3424	3426	rBV3	539	693	0.04%	0.006%
92	12.329	3509	3511	3512	rBV3	276	121	0.01%	0.001%
93	12.339	3512	3514	3518	rVV4	483	403	0.03%	0.004%
94	12.413	3535	3537	3542	rVB2	319	229	0.01%	0.002%
95	12.628	3602	3604	3607	rBV2	405	191	0.01%	0.002%
96	12.654	3610	3612	3614	rBV2	435	273	0.02%	0.002%
97	12.808	3658	3660	3662	rBV	441	261	0.02%	0.002%
98	13.143	3762	3764	3767	rBV3	334	178	0.01%	0.002%
99	13.210	3777	3785	3789	rBV5	1965	2651	0.17%	0.024%
100	13.905	3999	4001	4002	rBV	618	254	0.02%	0.002%




Sum of corrected areas: 11258028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035075.D
Acq On : 09 Apr 2024 12:15
Operator : SY/MD
Sample : P2017-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

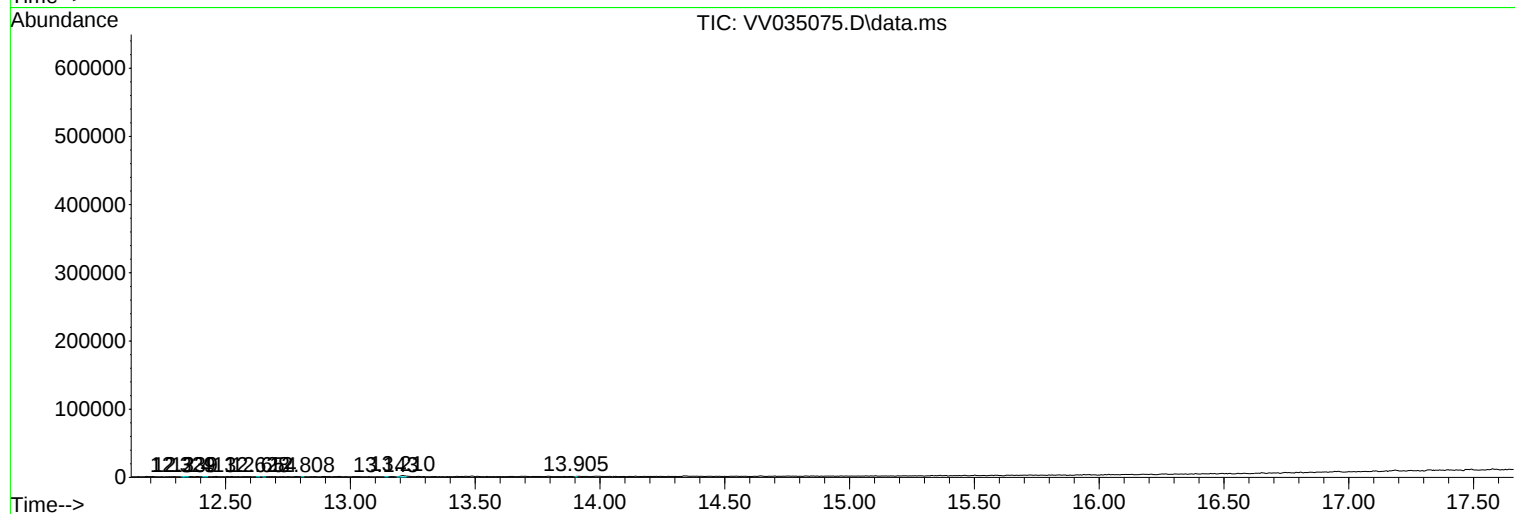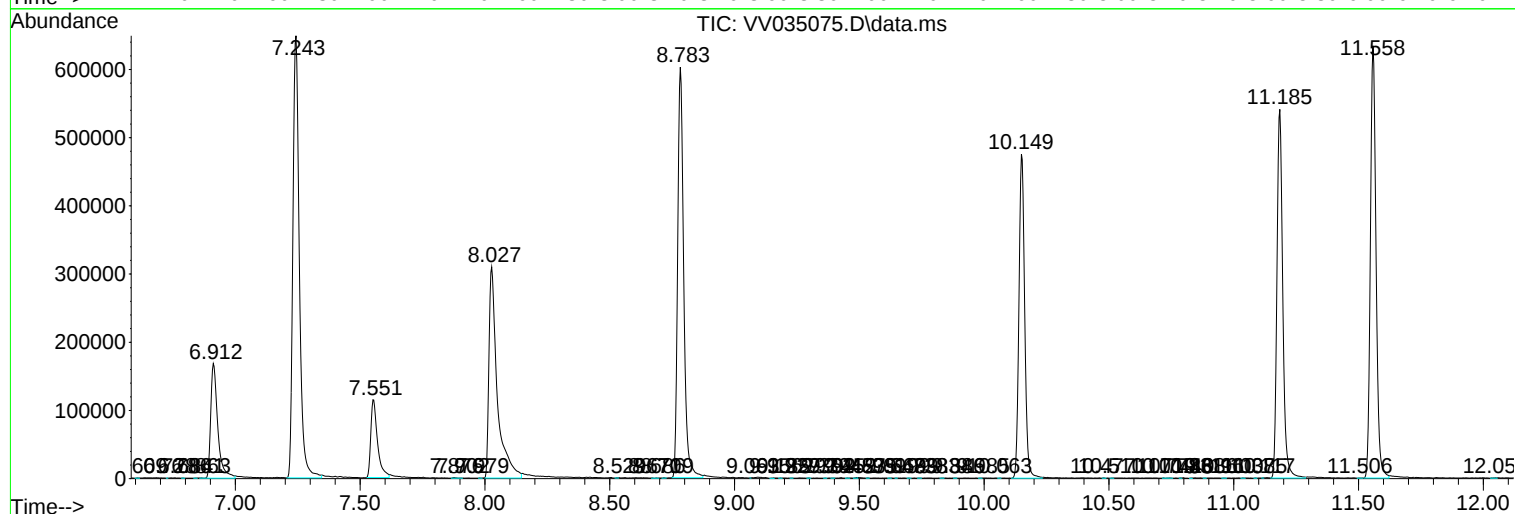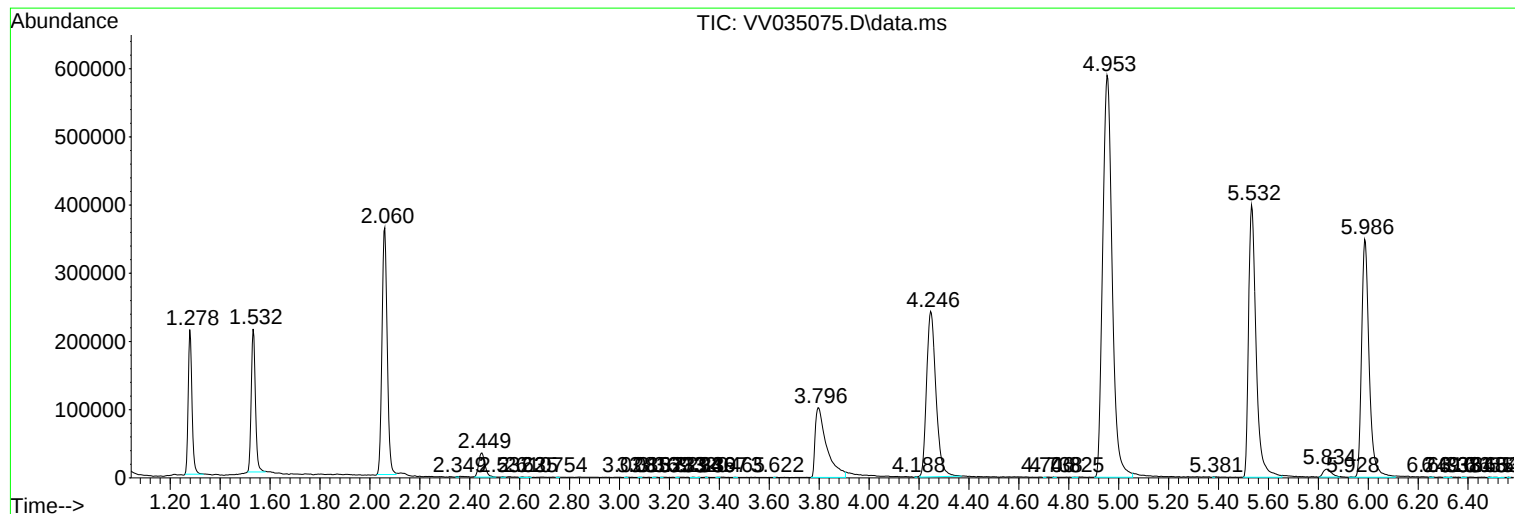

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035075.D
Acq On : 09 Apr 2024 12:15
Operator : SY/MD
Sample : P2017-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035075.D
Acq On : 09 Apr 2024 12:15
Operator : SY/MD
Sample : P2017-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------