

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035076.D
 Acq On : 09 Apr 2024 12:39
 Operator : SY/MD
 Sample : P2017-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	210506	222754	13.85%	1.918%
2	1.532	146	153	171	rVB	211748	246268	15.31%	2.120%
3	2.060	307	317	331	rBV	364476	528382	32.84%	4.549%
4	2.449	429	438	458	rVB	31166	54503	3.39%	0.469%
5	2.677	508	509	513	rBV	571	298	0.02%	0.003%
6	2.841	558	560	562	rBV2	233	105	0.01%	0.001%
7	2.870	568	569	571	rBV	261	113	0.01%	0.001%
8	2.950	591	594	597	rVB2	626	345	0.02%	0.003%
9	2.989	602	606	608	rBV2	459	250	0.02%	0.002%
10	3.069	629	631	632	rBV2	202	85	0.01%	0.001%
11	3.108	641	643	645	rBV	251	121	0.01%	0.001%
12	3.124	645	648	652	rVV2	331	242	0.02%	0.002%
13	3.178	662	665	667	rVB3	380	175	0.01%	0.002%
14	3.201	669	672	674	rVV4	360	215	0.01%	0.002%
15	3.252	685	688	691	rBV2	299	193	0.01%	0.002%
16	3.317	705	708	710	rBV2	242	149	0.01%	0.001%
17	3.378	721	727	729	rBV	229	198	0.01%	0.002%
18	3.436	740	745	748	rBV2	407	326	0.02%	0.003%
19	3.452	748	750	753	rBV2	317	184	0.01%	0.002%
20	3.468	753	755	756	rBV	170	69	0.00%	0.001%
21	3.506	764	767	769	rVB2	197	113	0.01%	0.001%
22	3.519	769	771	772	rBV	106	40	0.00%	0.000%
23	3.532	772	775	778	rBV2	238	160	0.01%	0.001%
24	3.548	778	780	782	rBV	177	91	0.01%	0.001%
25	3.613	798	800	807	rBV3	267	393	0.02%	0.003%
26	3.661	812	815	816	rBV2	114	61	0.00%	0.001%
27	3.696	822	826	828	rBV	332	294	0.02%	0.003%
28	3.757	844	845	846	rVB	320	62	0.00%	0.001%
29	3.796	848	857	904	rBV	108941	369041	22.94%	3.177%
30	4.246	981	997	1029	rBV	247779	660710	41.07%	5.688%
31	4.725	1144	1146	1148	rBV	380	180	0.01%	0.002%
32	4.818	1172	1175	1177	rBV2	301	204	0.01%	0.002%
33	4.953	1199	1217	1260	rBV2	600376	1608896	100.00%	13.852%
34	5.394	1352	1354	1356	rBV2	378	250	0.02%	0.002%
35	5.532	1386	1397	1439	rBV	412929	862768	53.62%	7.428%
36	5.831	1481	1490	1507	rBV3	12483	28664	1.78%	0.247%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035076.D
 Acq On : 09 Apr 2024 12:39
 Operator : SY/MD
 Sample : P2017-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.985	1525	1538	1565	rBV	351209	740911	46.05%	6.379%
38	6.339	1645	1648	1652	rBV3	736	566	0.04%	0.005%
39	6.407	1666	1669	1671	rBV	376	272	0.02%	0.002%
40	6.574	1719	1721	1723	rBV2	234	86	0.01%	0.001%
41	6.606	1727	1731	1734	rBV3	566	503	0.03%	0.004%
42	6.767	1780	1781	1783	rBV3	295	128	0.01%	0.001%
43	6.799	1789	1791	1795	rVB2	283	154	0.01%	0.001%
44	6.831	1799	1801	1804	rVB2	402	189	0.01%	0.002%
45	6.873	1812	1814	1816	rBV2	172	69	0.00%	0.001%
46	6.911	1816	1826	1850	rBV	170556	332379	20.66%	2.862%
47	7.243	1918	1929	1959	rBV	674877	1194851	74.27%	10.287%
48	7.551	2016	2025	2050	rBV	116527	220116	13.68%	1.895%
49	7.899	2131	2133	2136	rVB2	564	293	0.02%	0.003%
50	7.918	2137	2139	2142	rVV3	471	240	0.01%	0.002%
51	7.940	2144	2146	2147	rVB	319	105	0.01%	0.001%
52	7.979	2156	2158	2160	rBV2	267	154	0.01%	0.001%
53	8.027	2164	2173	2215	rBV3	326309	760943	47.30%	6.551%
54	8.574	2340	2343	2347	rVB3	932	595	0.04%	0.005%
55	8.638	2359	2363	2367	rBV3	483	361	0.02%	0.003%
56	8.696	2377	2381	2385	rBV4	569	568	0.04%	0.005%
57	8.783	2397	2408	2445	rBV	632057	1050245	65.28%	9.042%
58	9.169	2525	2528	2529	rBV2	464	238	0.01%	0.002%
59	9.304	2567	2570	2573	rVB2	363	265	0.02%	0.002%
60	9.333	2575	2579	2583	rVV2	272	264	0.02%	0.002%
61	9.410	2601	2603	2606	rBV	353	168	0.01%	0.001%
62	9.468	2620	2621	2622	rBV	198	38	0.00%	0.000%
63	9.493	2626	2629	2630	rBV	194	114	0.01%	0.001%
64	9.542	2641	2644	2648	rVB3	502	344	0.02%	0.003%
65	9.590	2654	2659	2662	rVB3	378	367	0.02%	0.003%
66	9.606	2662	2664	2668	rBV3	418	310	0.02%	0.003%
67	9.744	2705	2707	2711	rVB2	200	87	0.01%	0.001%
68	9.763	2711	2713	2716	rBV2	269	177	0.01%	0.002%
69	9.818	2727	2730	2731	rBV2	595	269	0.02%	0.002%
70	9.889	2750	2752	2756	rVB2	407	173	0.01%	0.001%
71	9.956	2770	2773	2774	rBV	223	88	0.01%	0.001%
72	9.992	2782	2784	2786	rBV	253	184	0.01%	0.002%
73	10.149	2817	2833	2856	rBV	490326	776484	48.26%	6.685%
74	10.397	2907	2910	2912	rBV3	363	160	0.01%	0.001%
75	10.423	2916	2918	2921	rBV2	415	282	0.02%	0.002%
76	10.513	2943	2946	2949	rVB2	503	316	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035076.D
 Acq On : 09 Apr 2024 12:39
 Operator : SY/MD
 Sample : P2017-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.651	2985	2989	2996	rBV2	322	374	0.02%	0.003%
78	10.680	2996	2998	3002	rVB2	180	125	0.01%	0.001%
79	10.699	3002	3004	3007	rBV	307	194	0.01%	0.002%
80	11.024	3101	3105	3110	rVB2	400	291	0.02%	0.003%
81	11.127	3135	3137	3140	rBV3	499	310	0.02%	0.003%
82	11.185	3143	3155	3187	rBV	570847	904617	56.23%	7.788%
83	11.558	3260	3271	3295	rBV	652117	1034567	64.30%	8.907%
84	11.860	3363	3365	3367	rBV	384	212	0.01%	0.002%
85	11.885	3370	3373	3376	rBV2	547	360	0.02%	0.003%
86	12.040	3418	3421	3424	rBV2	391	277	0.02%	0.002%
87	12.236	3480	3482	3486	rBV2	338	264	0.02%	0.002%
88	12.352	3516	3518	3519	rBV2	454	157	0.01%	0.001%
89	12.432	3540	3543	3546	rBV2	443	289	0.02%	0.002%
90	12.590	3590	3592	3594	rBV	409	272	0.02%	0.002%
91	12.651	3609	3611	3615	rBV2	376	223	0.01%	0.002%
92	12.834	3666	3668	3673	rVB2	450	320	0.02%	0.003%
93	13.207	3780	3784	3785	rBV2	1208	896	0.06%	0.008%
94	13.525	3882	3883	3886	rBV2	393	175	0.01%	0.002%




Sum of corrected areas: 11614881

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035076.D
Acq On : 09 Apr 2024 12:39
Operator : SY/MD
Sample : P2017-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

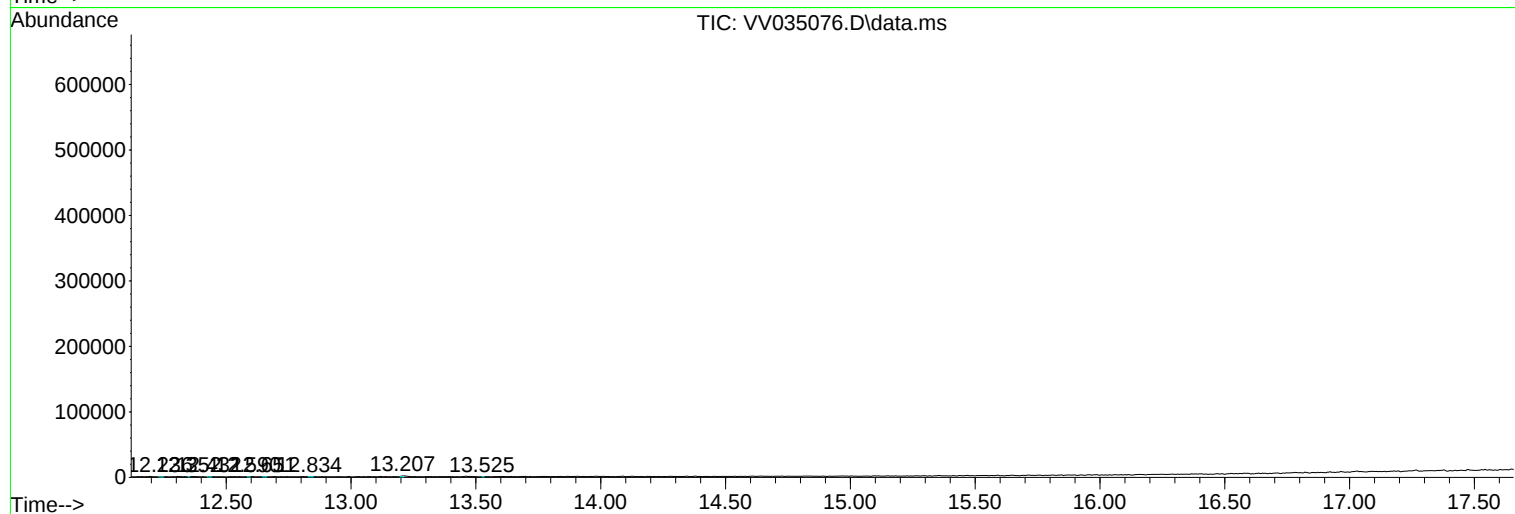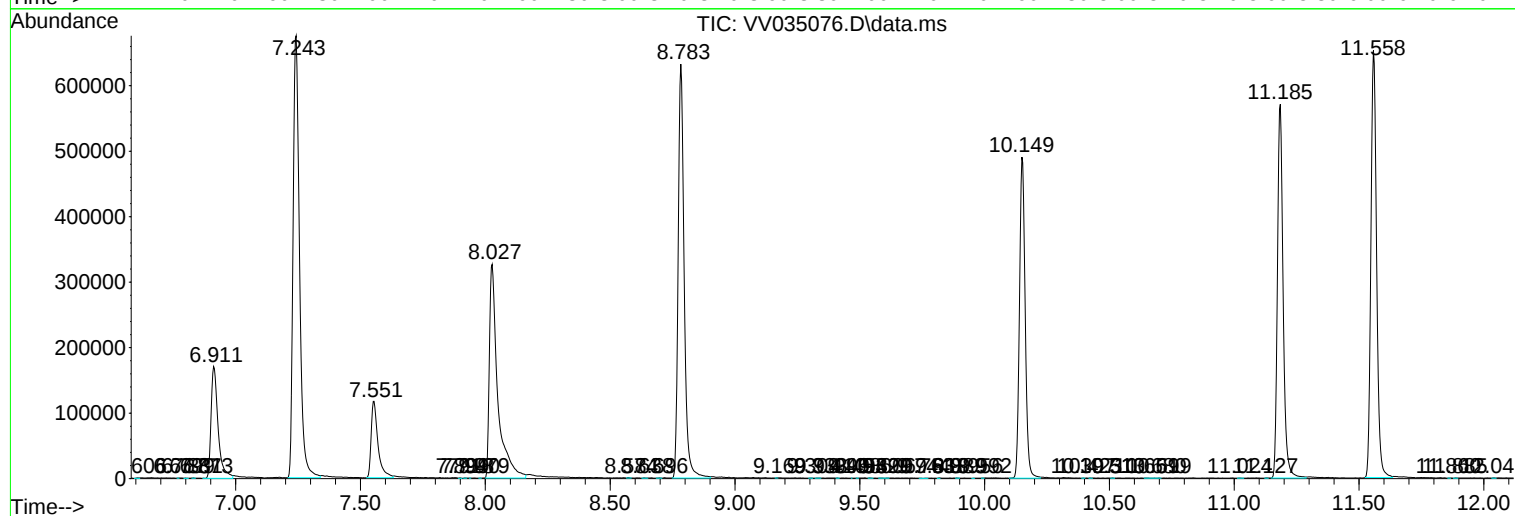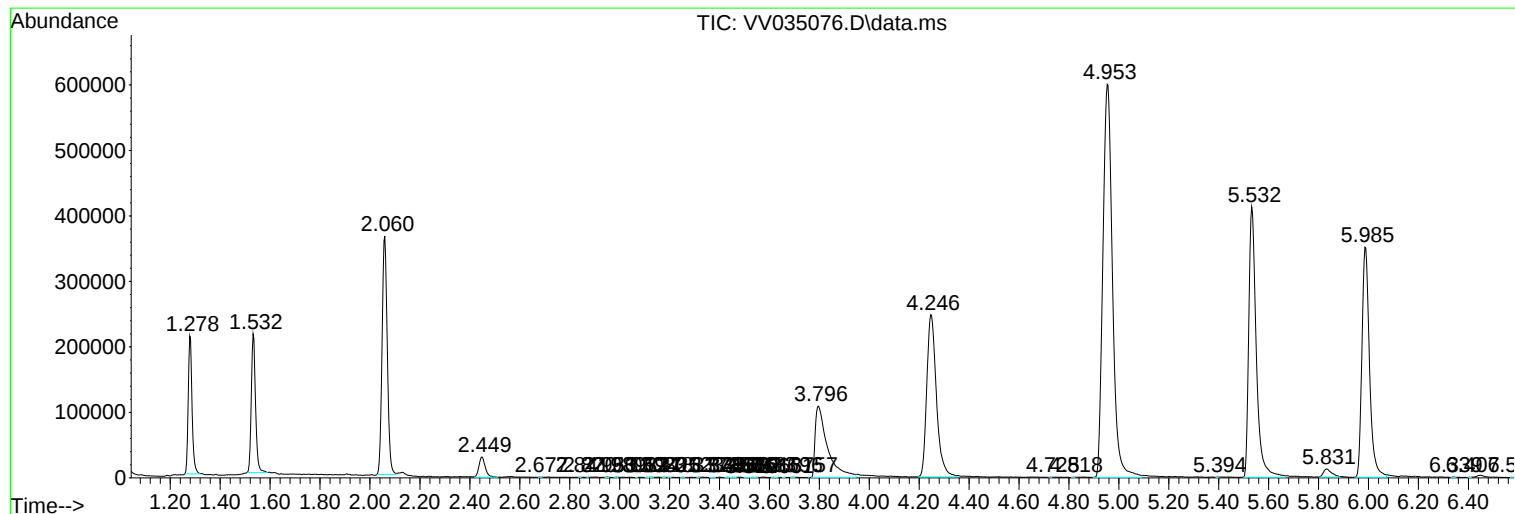

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035076.D
Acq On : 09 Apr 2024 12:39
Operator : SY/MD
Sample : P2017-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035076.D
Acq On : 09 Apr 2024 12:39
Operator : SY/MD
Sample : P2017-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------