

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035078.D
 Acq On : 09 Apr 2024 13:27
 Operator : SY/MD
 Sample : P2017-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	225275	242312	13.96%	1.935%
2	1.532	146	153	169	rVB	237135	271613	15.65%	2.169%
3	2.060	307	317	332	rBV	393797	568597	32.77%	4.540%
4	2.449	429	438	459	rVB	34669	58270	3.36%	0.465%
5	2.677	507	509	512	rBV2	416	331	0.02%	0.003%
6	2.757	532	534	538	rVB	853	381	0.02%	0.003%
7	2.780	538	541	543	rBV2	574	309	0.02%	0.002%
8	2.870	565	569	575	rBV3	344	358	0.02%	0.003%
9	2.963	596	598	599	rBV2	304	139	0.01%	0.001%
10	3.015	611	614	616	rBV3	314	191	0.01%	0.002%
11	3.050	623	625	626	rBV	237	110	0.01%	0.001%
12	3.072	630	632	633	rVB	538	177	0.01%	0.001%
13	3.082	633	635	636	rBV	319	154	0.01%	0.001%
14	3.146	652	655	658	rBV2	425	290	0.02%	0.002%
15	3.230	680	681	682	rBV2	305	106	0.01%	0.001%
16	3.253	686	688	690	rBV2	196	106	0.01%	0.001%
17	3.291	697	700	703	rBV2	264	178	0.01%	0.001%
18	3.310	703	706	707	rBV	268	130	0.01%	0.001%
19	3.391	728	731	733	rVB2	211	122	0.01%	0.001%
20	3.410	733	737	740	rBV2	288	241	0.01%	0.002%
21	3.445	745	748	750	rVB3	452	205	0.01%	0.002%
22	3.462	751	753	758	rVV2	197	209	0.01%	0.002%
23	3.542	776	778	782	rBV3	300	164	0.01%	0.001%
24	3.574	785	788	790	rBV2	255	159	0.01%	0.001%
25	3.622	801	803	806	rVB	241	111	0.01%	0.001%
26	3.642	806	809	811	rBV	214	112	0.01%	0.001%
27	3.658	811	814	816	rVB2	232	137	0.01%	0.001%
28	3.683	816	822	825	rVB2	293	217	0.01%	0.002%
29	3.793	847	856	893	rBV	124337	382073	22.02%	3.051%
30	4.246	983	997	1030	rBV	268217	720598	41.52%	5.754%
31	4.658	1123	1125	1127	rBV3	316	137	0.01%	0.001%
32	4.693	1134	1136	1139	rBV3	270	157	0.01%	0.001%
33	4.709	1139	1141	1143	rVB	332	131	0.01%	0.001%
34	4.732	1145	1148	1149	rBV2	581	285	0.02%	0.002%
35	4.953	1202	1217	1263	rBV2	649694	1735357	100.00%	13.856%
36	5.420	1360	1362	1365	rVB2	601	271	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035078.D
 Acq On : 09 Apr 2024 13:27
 Operator : SY/MD
 Sample : P2017-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.484	1379	1382	1386	rBV3	550	528	0.03%	0.004%
38	5.532	1386	1397	1439	rBV	422820	897220	51.70%	7.164%
39	5.831	1480	1490	1507	rBV2	13613	30203	1.74%	0.241%
40	5.986	1525	1538	1565	rBV	388190	807094	46.51%	6.444%
41	6.349	1648	1651	1653	rBV2	388	269	0.02%	0.002%
42	6.532	1704	1708	1711	rBV	659	459	0.03%	0.004%
43	6.548	1711	1713	1715	rBV	289	160	0.01%	0.001%
44	6.587	1722	1725	1726	rBV	213	136	0.01%	0.001%
45	6.751	1774	1776	1777	rBV	443	183	0.01%	0.001%
46	6.834	1800	1802	1805	rBV2	337	241	0.01%	0.002%
47	6.912	1814	1826	1859	rBV	188076	367114	21.15%	2.931%
48	7.243	1918	1929	1953	rBV	720716	1297152	74.75%	10.357%
49	7.551	2016	2025	2049	rBV2	126693	240352	13.85%	1.919%
50	7.844	2112	2116	2120	rVB2	372	282	0.02%	0.002%
51	7.886	2128	2129	2133	rVB2	478	279	0.02%	0.002%
52	7.908	2133	2136	2138	rBV3	946	597	0.03%	0.005%
53	7.940	2144	2146	2149	rBV3	406	291	0.02%	0.002%
54	8.027	2163	2173	2215	rBV2	372444	825105	47.55%	6.588%
55	8.468	2308	2310	2312	rBV2	625	261	0.02%	0.002%
56	8.635	2357	2362	2363	rBV2	321	267	0.02%	0.002%
57	8.670	2371	2373	2374	rBV	405	212	0.01%	0.002%
58	8.741	2393	2395	2396	rBV2	293	108	0.01%	0.001%
59	8.783	2397	2408	2436	rBV	655918	1087835	62.69%	8.686%
60	9.034	2484	2486	2488	rBV	424	168	0.01%	0.001%
61	9.088	2500	2503	2514	rVB9	1742	1995	0.11%	0.016%
62	9.204	2536	2539	2543	rVB2	499	337	0.02%	0.003%
63	9.227	2543	2546	2547	rBV2	369	255	0.01%	0.002%
64	9.281	2558	2563	2565	rVB2	572	545	0.03%	0.004%
65	9.294	2565	2567	2568	rBV	338	148	0.01%	0.001%
66	9.394	2594	2598	2600	rBV2	410	346	0.02%	0.003%
67	9.436	2608	2611	2613	rBV2	315	187	0.01%	0.001%
68	9.461	2616	2619	2620	rBV	298	184	0.01%	0.001%
69	9.487	2623	2627	2634	rBV4	1776	2188	0.13%	0.017%
70	9.593	2655	2660	2665	rBV3	302	320	0.02%	0.003%
71	9.751	2704	2709	2712	rBV2	320	307	0.02%	0.002%
72	9.831	2732	2734	2736	rBV	210	102	0.01%	0.001%
73	9.883	2742	2750	2757	rVB7	1123	1675	0.10%	0.013%
74	9.911	2757	2759	2762	rBV2	316	205	0.01%	0.002%
75	9.976	2777	2779	2782	rBV2	319	178	0.01%	0.001%
76	9.995	2782	2785	2787	rBV2	287	191	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035078.D
 Acq On : 09 Apr 2024 13:27
 Operator : SY/MD
 Sample : P2017-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.149	2821	2833	2862	rBV	539403	850030	48.98%	6.787%
78	10.368	2899	2901	2903	rBV	562	272	0.02%	0.002%
79	10.519	2946	2948	2952	rVB2	785	342	0.02%	0.003%
80	10.542	2952	2955	2956	rBV	625	337	0.02%	0.003%
81	10.667	2991	2994	3000	rVB3	558	474	0.03%	0.004%
82	10.776	3026	3028	3030	rBV	416	187	0.01%	0.001%
83	10.860	3048	3054	3059	rBV4	690	854	0.05%	0.007%
84	10.950	3080	3082	3084	rBV	214	121	0.01%	0.001%
85	10.969	3084	3088	3090	rVV	379	253	0.01%	0.002%
86	11.040	3107	3110	3112	rVV2	378	217	0.01%	0.002%
87	11.082	3120	3123	3124	rBV	178	118	0.01%	0.001%
88	11.133	3132	3139	3144	rBV5	1404	2017	0.12%	0.016%
89	11.185	3144	3155	3182	rBV	602614	962054	55.44%	7.682%
90	11.474	3243	3245	3248	rVB3	425	267	0.02%	0.002%
91	11.558	3258	3271	3298	rBV	728005	1151510	66.36%	9.194%
92	11.828	3351	3355	3358	rBV3	564	527	0.03%	0.004%
93	11.953	3392	3394	3395	rBV	335	113	0.01%	0.001%
94	12.175	3460	3463	3464	rBV	450	208	0.01%	0.002%
95	12.358	3518	3520	3522	rVB	416	185	0.01%	0.001%
96	12.374	3523	3525	3527	rBV	385	185	0.01%	0.001%
97	12.387	3527	3529	3531	rBV	420	155	0.01%	0.001%
98	12.738	3636	3638	3642	rBV3	386	254	0.01%	0.002%
99	13.210	3779	3785	3794	rVB5	2165	3190	0.18%	0.025%
100	13.342	3824	3826	3828	rBV2	363	136	0.01%	0.001%




Sum of corrected areas: 12524123

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035078.D
Acq On : 09 Apr 2024 13:27
Operator : SY/MD
Sample : P2017-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

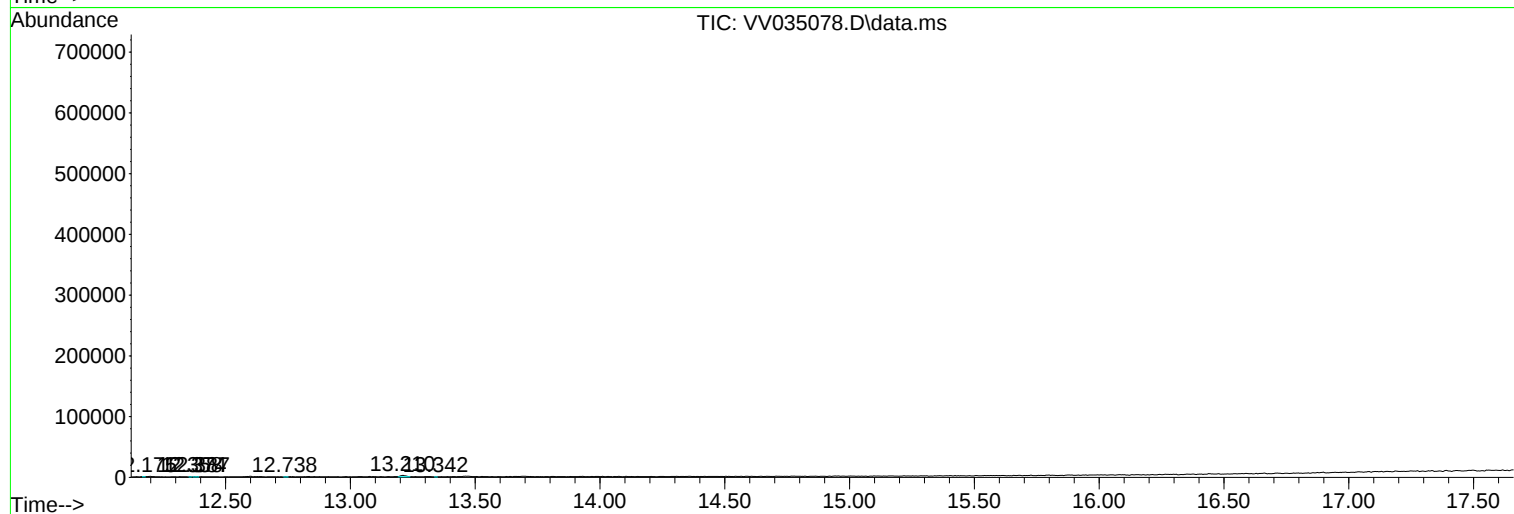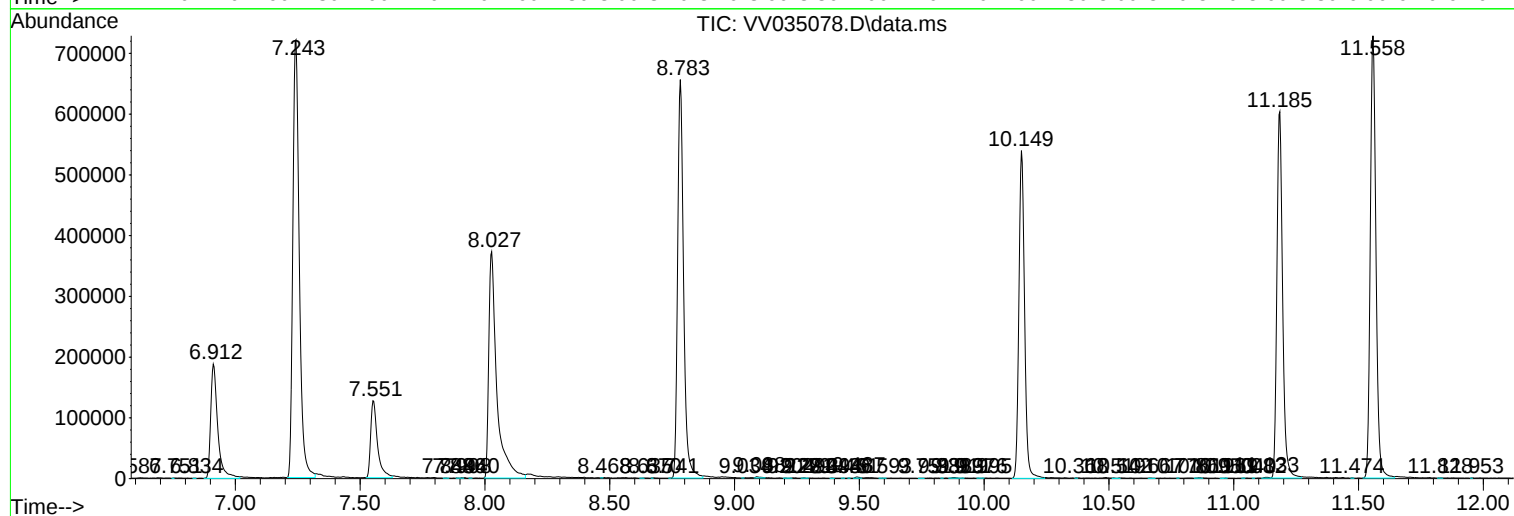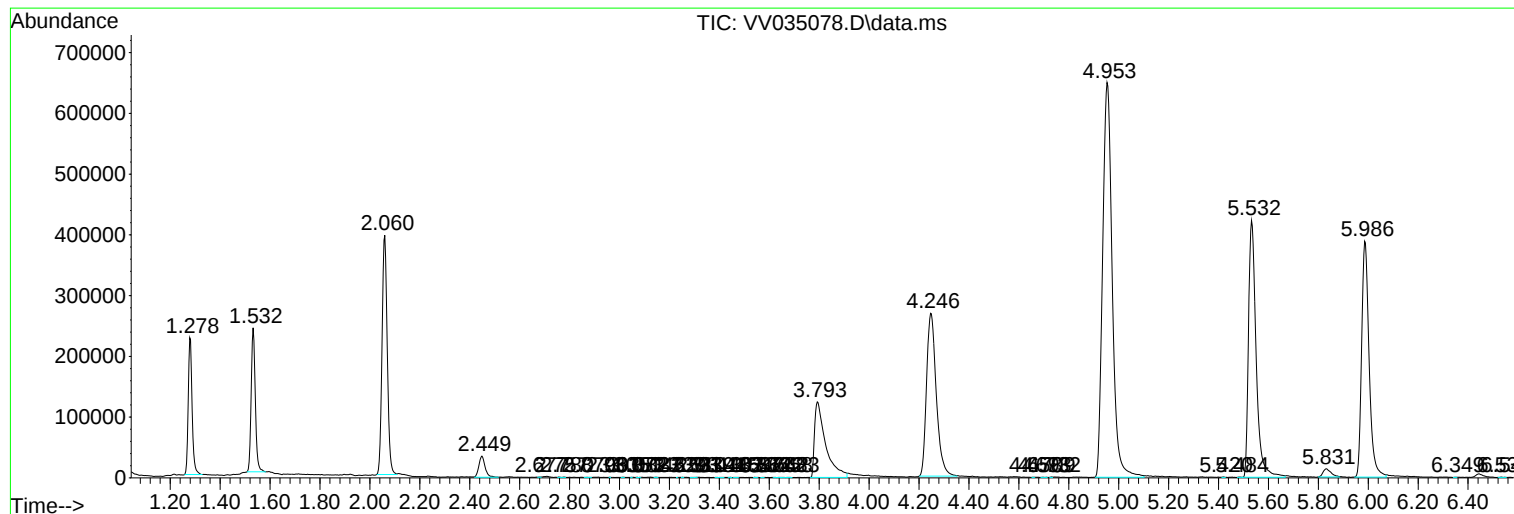

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035078.D
Acq On : 09 Apr 2024 13:27
Operator : SY/MD
Sample : P2017-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035078.D
Acq On : 09 Apr 2024 13:27
Operator : SY/MD
Sample : P2017-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------