

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035083.D
 Acq On : 09 Apr 2024 15:27
 Operator : SY/MD
 Sample : P2017-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035083.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	96	rVB	180762	194056	13.32%	1.874%
2	1.532	146	153	166	rBV	201312	225757	15.49%	2.181%
3	2.056	307	316	331	rBV	310667	451502	30.99%	4.361%
4	2.449	429	438	455	rVB	30488	53018	3.64%	0.512%
5	2.539	463	466	467	rBV	640	361	0.02%	0.003%
6	2.796	544	546	547	rBV2	328	90	0.01%	0.001%
7	2.828	554	556	558	rBV2	380	117	0.01%	0.001%
8	2.876	569	571	573	rVB2	320	113	0.01%	0.001%
9	2.934	586	589	591	rBV	373	217	0.01%	0.002%
10	2.973	595	601	602	rBV2	523	569	0.04%	0.005%
11	2.992	605	607	609	rBV	244	121	0.01%	0.001%
12	3.076	629	633	634	rBV	334	177	0.01%	0.002%
13	3.105	639	642	646	rVB2	568	291	0.02%	0.003%
14	3.127	646	649	653	rBV3	531	470	0.03%	0.005%
15	3.188	665	668	671	rVB3	344	233	0.02%	0.002%
16	3.207	672	674	676	rBV2	353	147	0.01%	0.001%
17	3.301	700	703	706	rVB	294	199	0.01%	0.002%
18	3.388	728	730	739	rVB2	444	474	0.03%	0.005%
19	3.458	748	752	754	rBV2	245	202	0.01%	0.002%
20	3.481	755	759	760	rVB2	312	177	0.01%	0.002%
21	3.523	768	772	774	rBV2	289	199	0.01%	0.002%
22	3.600	794	796	798	rVB2	360	131	0.01%	0.001%
23	3.635	805	807	812	rVB2	428	331	0.02%	0.003%
24	3.683	818	822	825	rBV2	106	89	0.01%	0.001%
25	3.703	825	828	831	rBV	301	241	0.02%	0.002%
26	3.764	845	847	848	rBV2	259	111	0.01%	0.001%
27	3.796	848	857	893	rBV	109198	350257	24.04%	3.383%
28	4.246	982	997	1028	rBV	232072	614912	42.20%	5.939%
29	4.619	1111	1113	1115	rBV2	414	180	0.01%	0.002%
30	4.683	1131	1133	1135	rBV2	363	158	0.01%	0.002%
31	4.728	1145	1147	1149	rBV	571	213	0.01%	0.002%
32	4.799	1167	1169	1172	rBV2	294	152	0.01%	0.001%
33	4.953	1201	1217	1249	rBV2	547176	1457072	100.00%	14.074%
34	5.288	1319	1321	1324	rVB2	834	388	0.03%	0.004%
35	5.532	1386	1397	1433	rBV	353677	749710	51.45%	7.241%
36	5.831	1481	1490	1505	rBV4	11742	25503	1.75%	0.246%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035083.D
 Acq On : 09 Apr 2024 15:27
 Operator : SY/MD
 Sample : P2017-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.985	1526	1538	1576	rBV	327849	688426	47.25%	6.649%
38	6.284	1629	1631	1633	rBV2	366	143	0.01%	0.001%
39	6.297	1633	1635	1638	rVB2	438	229	0.02%	0.002%
40	6.346	1648	1650	1654	rVB3	711	429	0.03%	0.004%
41	6.391	1662	1664	1665	rBV	331	172	0.01%	0.002%
42	6.445	1670	1681	1692	rBV6	3504	7256	0.50%	0.070%
43	6.551	1712	1714	1716	rVB	330	135	0.01%	0.001%
44	6.561	1716	1717	1719	rBV2	232	82	0.01%	0.001%
45	6.735	1767	1771	1774	rBV2	421	353	0.02%	0.003%
46	6.747	1774	1775	1777	rVB2	563	139	0.01%	0.001%
47	6.760	1777	1779	1785	rVB3	320	273	0.02%	0.003%
48	6.796	1785	1790	1795	rBV4	488	467	0.03%	0.005%
49	6.821	1795	1798	1801	rBV2	180	92	0.01%	0.001%
50	6.838	1801	1803	1807	rVB	177	88	0.01%	0.001%
51	6.857	1807	1809	1811	rBV2	249	107	0.01%	0.001%
52	6.911	1815	1826	1858	rBV	157316	310248	21.29%	2.997%
53	7.243	1918	1929	1954	rBV	577152	1029342	70.64%	9.942%
54	7.555	2017	2026	2060	rBV2	107912	206245	14.15%	1.992%
55	7.821	2107	2109	2110	rBV2	387	151	0.01%	0.001%
56	7.956	2149	2151	2153	rVB2	543	167	0.01%	0.002%
57	8.027	2164	2173	2211	rBV3	302029	709343	48.68%	6.852%
58	8.471	2309	2311	2314	rBV	390	264	0.02%	0.003%
59	8.625	2358	2359	2361	rBV	297	146	0.01%	0.001%
60	8.712	2385	2386	2388	rVB	425	115	0.01%	0.001%
61	8.725	2388	2390	2392	rVB	272	95	0.01%	0.001%
62	8.738	2392	2394	2396	rVB2	296	124	0.01%	0.001%
63	8.783	2396	2408	2435	rBV	543037	909364	62.41%	8.784%
64	9.149	2519	2522	2523	rBV2	333	188	0.01%	0.002%
65	9.291	2564	2566	2567	rBV	269	82	0.01%	0.001%
66	9.317	2572	2574	2575	rVB	358	100	0.01%	0.001%
67	9.336	2575	2580	2582	rBV3	316	307	0.02%	0.003%
68	9.474	2620	2623	2626	rBV2	387	245	0.02%	0.002%
69	9.596	2659	2661	2664	rVB2	206	108	0.01%	0.001%
70	9.651	2674	2678	2684	rBV3	450	395	0.03%	0.004%
71	9.715	2695	2698	2700	rBV2	321	182	0.01%	0.002%
72	9.754	2707	2710	2713	rBV2	363	204	0.01%	0.002%
73	9.770	2713	2715	2717	rBV2	234	122	0.01%	0.001%
74	9.847	2737	2739	2742	rBV2	565	238	0.02%	0.002%
75	9.927	2759	2764	2767	rBV3	632	580	0.04%	0.006%
76	10.011	2788	2790	2791	rBV	271	99	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035083.D
 Acq On : 09 Apr 2024 15:27
 Operator : SY/MD
 Sample : P2017-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.149	2821	2833	2858	rBV	457885	734813	50.43%	7.098%
78	10.339	2890	2892	2895	rBV	294	164	0.01%	0.002%
79	10.432	2918	2921	2924	rBV3	390	294	0.02%	0.003%
80	10.506	2942	2944	2947	rBV2	406	274	0.02%	0.003%
81	10.632	2980	2983	2984	rBV	248	120	0.01%	0.001%
82	10.661	2989	2992	2996	rBV2	378	262	0.02%	0.003%
83	10.718	3009	3010	3013	rBV2	224	109	0.01%	0.001%
84	10.744	3013	3018	3022	rBV3	620	703	0.05%	0.007%
85	11.014	3100	3102	3104	rBV2	301	186	0.01%	0.002%
86	11.104	3126	3130	3135	rBV3	368	345	0.02%	0.003%
87	11.127	3135	3137	3139	rBV2	522	257	0.02%	0.002%
88	11.185	3142	3155	3176	rBV	468228	747799	51.32%	7.223%
89	11.384	3214	3217	3219	rBV3	813	502	0.03%	0.005%
90	11.516	3256	3258	3259	rBV	400	154	0.01%	0.001%
91	11.558	3260	3271	3297	rVV	539983	870358	59.73%	8.407%
92	11.866	3366	3367	3369	rVB	431	107	0.01%	0.001%
93	12.046	3421	3423	3425	rBV2	377	142	0.01%	0.001%
94	12.307	3502	3504	3507	rBV	387	230	0.02%	0.002%
95	12.525	3569	3572	3575	rBV2	631	292	0.02%	0.003%
96	12.564	3582	3584	3587	rVB2	451	156	0.01%	0.002%
97	12.635	3603	3606	3608	rBV3	514	334	0.02%	0.003%
98	13.287	3807	3809	3811	rBV2	440	255	0.02%	0.002%
99	13.400	3841	3844	3845	rBV	491	237	0.02%	0.002%
100	13.561	3892	3894	3897	rBV2	454	190	0.01%	0.002%




Sum of corrected areas: 10353066

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035083.D
Acq On : 09 Apr 2024 15:27
Operator : SY/MD
Sample : P2017-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

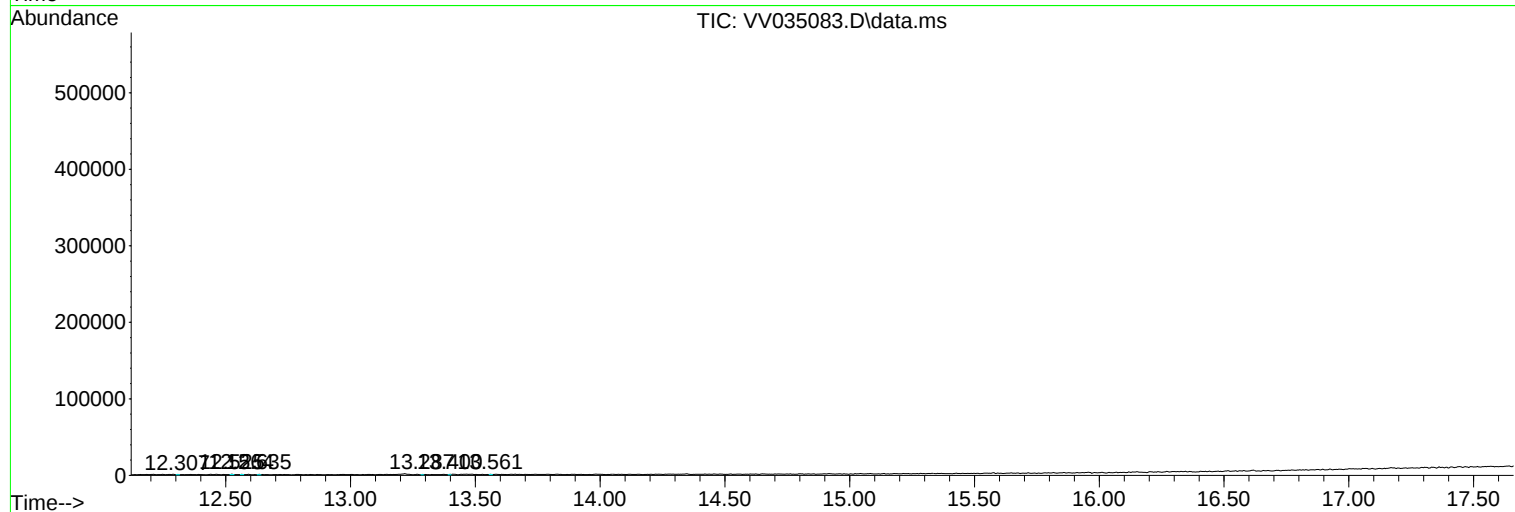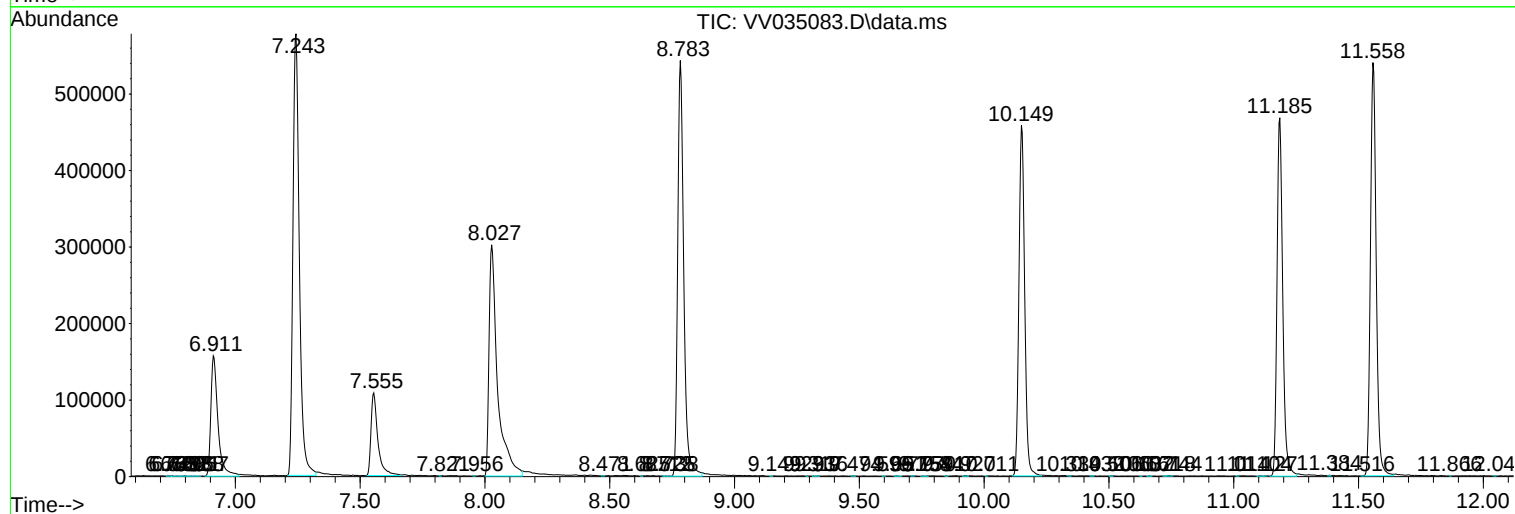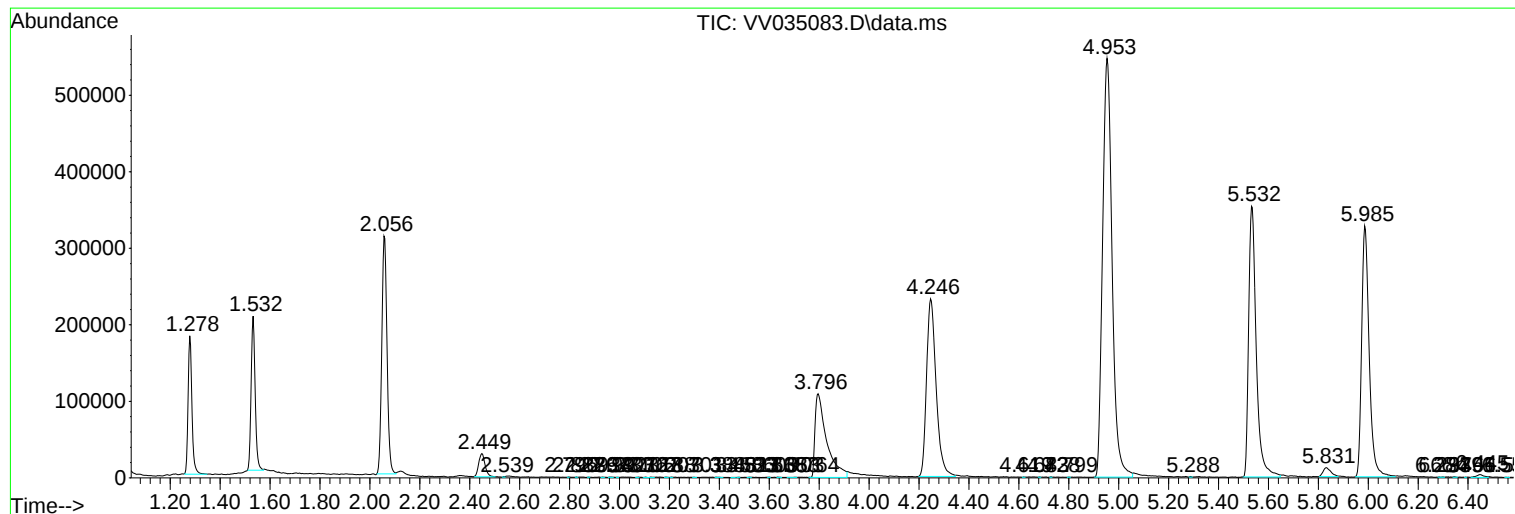

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035083.D
Acq On : 09 Apr 2024 15:27
Operator : SY/MD
Sample : P2017-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035083.D
Acq On : 09 Apr 2024 15:27
Operator : SY/MD
Sample : P2017-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc