

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035086.D
 Acq On : 09 Apr 2024 16:39
 Operator : SY/MD
 Sample : P2006-10DL2 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE9DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	179858	188152	11.32%	1.545%
2	1.529	146	152	168	rVB	201873	239468	14.41%	1.966%
3	2.056	307	316	334	rBV	311563	452141	27.20%	3.713%
4	2.555	465	471	472	rBV4	1150	1144	0.07%	0.009%
5	2.693	511	514	517	rBV3	578	370	0.02%	0.003%
6	2.764	531	536	539	rBV2	444	287	0.02%	0.002%
7	2.809	549	550	555	rBV2	244	180	0.01%	0.001%
8	2.886	571	574	575	rBV2	321	183	0.01%	0.002%
9	2.957	594	596	602	rBV3	492	495	0.03%	0.004%
10	3.050	622	625	627	rBV2	445	249	0.01%	0.002%
11	3.156	656	658	662	rVB3	514	383	0.02%	0.003%
12	3.191	666	669	672	rBV2	228	168	0.01%	0.001%
13	3.236	679	683	684	rBV	302	210	0.01%	0.002%
14	3.259	687	690	692	rBV	511	318	0.02%	0.003%
15	3.323	708	710	712	rBV	241	141	0.01%	0.001%
16	3.442	744	747	750	rBV2	288	216	0.01%	0.002%
17	3.465	751	754	760	rVB3	387	311	0.02%	0.003%
18	3.490	760	762	764	rBV	358	181	0.01%	0.001%
19	3.526	771	773	776	rVB3	347	170	0.01%	0.001%
20	3.593	791	794	797	rVB2	366	244	0.01%	0.002%
21	3.619	797	802	803	rBV2	324	184	0.01%	0.002%
22	3.635	805	807	809	rVB3	326	163	0.01%	0.001%
23	3.648	809	811	814	rBV2	311	200	0.01%	0.002%
24	3.693	823	825	828	rVB2	329	163	0.01%	0.001%
25	3.735	833	838	840	rBV3	327	214	0.01%	0.002%
26	3.751	840	843	844	rBV	256	178	0.01%	0.001%
27	3.793	848	856	898	rBV	116082	366644	22.06%	3.011%
28	4.246	982	997	1030	rBV	226740	588919	35.43%	4.836%
29	4.523	1077	1083	1088	rBV6	672	1098	0.07%	0.009%
30	4.696	1134	1137	1138	rBV	582	266	0.02%	0.002%
31	4.953	1201	1217	1230	rBV2	543581	1439603	86.61%	11.822%
32	5.291	1319	1322	1328	rVB4	946	838	0.05%	0.007%
33	5.400	1355	1356	1358	rBV	455	216	0.01%	0.002%
34	5.532	1386	1397	1432	rBV	383545	803724	48.36%	6.600%
35	5.985	1524	1538	1566	rBV	327633	682649	41.07%	5.606%
36	6.294	1632	1634	1638	rBV2	447	332	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035086.D
 Acq On : 09 Apr 2024 16:39
 Operator : SY/MD
 Sample : P2006-10DL2 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE9DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.339	1646	1648	1653	rVB3	507	338	0.02%	0.003%
38	6.397	1663	1666	1668	rBV	442	262	0.02%	0.002%
39	6.416	1668	1672	1675	rVV2	483	352	0.02%	0.003%
40	6.490	1692	1695	1698	rBV2	454	350	0.02%	0.003%
41	6.571	1718	1720	1724	rVB4	408	256	0.02%	0.002%
42	6.616	1731	1734	1736	rBV3	531	319	0.02%	0.003%
43	6.654	1742	1746	1748	rBV3	651	390	0.02%	0.003%
44	6.773	1780	1783	1786	rVB	331	173	0.01%	0.001%
45	6.789	1786	1788	1791	rBV2	325	191	0.01%	0.002%
46	6.805	1791	1793	1798	rVB4	601	379	0.02%	0.003%
47	6.847	1802	1806	1809	rBB2	436	236	0.01%	0.002%
48	6.870	1811	1813	1816	rBV	277	168	0.01%	0.001%
49	6.911	1816	1826	1862	rBV	155202	307114	18.48%	2.522%
50	7.143	1895	1898	1899	rBV2	633	344	0.02%	0.003%
51	7.243	1917	1929	1958	rBV	586872	1040189	62.58%	8.542%
52	7.555	2017	2026	2057	rBV	106222	203678	12.25%	1.673%
53	7.860	2119	2121	2123	rVB3	392	146	0.01%	0.001%
54	7.918	2137	2139	2142	rVB3	369	160	0.01%	0.001%
55	7.937	2142	2145	2147	rBV2	501	221	0.01%	0.002%
56	7.960	2147	2152	2153	rBV2	436	302	0.02%	0.002%
57	8.027	2164	2173	2213	rBV2	329547	745082	44.83%	6.119%
58	8.555	2335	2337	2339	rBV3	587	311	0.02%	0.003%
59	8.596	2347	2350	2354	rVB3	419	304	0.02%	0.002%
60	8.686	2373	2378	2380	rBV2	395	349	0.02%	0.003%
61	8.783	2397	2408	2412	rBV	635624	936300	56.33%	7.689%
62	9.101	2502	2507	2510	rBV5	1042	1014	0.06%	0.008%
63	9.165	2525	2527	2529	rBV	520	202	0.01%	0.002%
64	9.178	2529	2531	2533	rVV2	390	243	0.01%	0.002%
65	9.233	2546	2548	2550	rBV	584	286	0.02%	0.002%
66	9.281	2558	2563	2566	rBV4	746	880	0.05%	0.007%
67	9.400	2598	2600	2603	rVB2	291	151	0.01%	0.001%
68	9.554	2646	2648	2651	rBV	278	145	0.01%	0.001%
69	9.612	2664	2666	2669	rVB2	335	207	0.01%	0.002%
70	9.628	2669	2671	2675	rBV4	568	345	0.02%	0.003%
71	9.693	2689	2691	2693	rBV3	346	211	0.01%	0.002%
72	9.718	2696	2699	2701	rVV	254	153	0.01%	0.001%
73	9.744	2704	2707	2712	rVB3	408	399	0.02%	0.003%
74	9.918	2756	2761	2764	rBV	566	482	0.03%	0.004%
75	9.989	2779	2783	2785	rBV	514	399	0.02%	0.003%
76	10.104	2817	2819	2822	rVB	305	160	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035086.D
 Acq On : 09 Apr 2024 16:39
 Operator : SY/MD
 Sample : P2006-10DL2 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE9DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.149	2822	2833	2855	rBV	474209	748594	45.04%	6.147%
78	10.381	2901	2905	2910	rVB3	377	266	0.02%	0.002%
79	10.452	2925	2927	2932	rBV3	311	219	0.01%	0.002%
80	10.532	2950	2952	2954	rVB3	343	139	0.01%	0.001%
81	10.554	2954	2959	2961	rBV3	502	312	0.02%	0.003%
82	10.995	3092	3096	3098	rVB2	326	207	0.01%	0.002%
83	11.017	3099	3103	3104	rBV2	508	348	0.02%	0.003%
84	11.056	3112	3115	3118	rVB	272	206	0.01%	0.002%
85	11.120	3126	3135	3145	rBV	46182	76470	4.60%	0.628%
86	11.185	3145	3155	3184	rVB2	587647	1492718	89.81%	12.258%
87	11.423	3226	3229	3232	rBV3	595	416	0.03%	0.003%
88	11.561	3259	3272	3299	rBV3	722004	1662128	100.00%	13.649%
89	12.130	3446	3449	3455	rBV2	310	342	0.02%	0.003%
90	12.197	3465	3470	3475	rVB4	601	617	0.04%	0.005%
91	12.603	3590	3596	3602	rBV4	704	1019	0.06%	0.008%
92	12.651	3608	3611	3612	rBV2	606	338	0.02%	0.003%
93	12.689	3620	3623	3624	rBV	506	198	0.01%	0.002%
94	12.767	3644	3647	3648	rBV2	323	160	0.01%	0.001%
95	12.805	3657	3659	3661	rBV	399	249	0.01%	0.002%
96	12.873	3678	3680	3685	rVB	583	343	0.02%	0.003%
97	12.902	3686	3689	3690	rBV	270	137	0.01%	0.001%
98	13.201	3772	3782	3800	rBV2	84764	139036	8.36%	1.142%
99	13.683	3922	3932	3946	rBV2	23373	38949	2.34%	0.320%
100	13.863	3986	3988	3992	rBV3	630	411	0.02%	0.003%

Sum of corrected areas: 12177415




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035086.D
Acq On : 09 Apr 2024 16:39
Operator : SY/MD
Sample : P2006-10DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

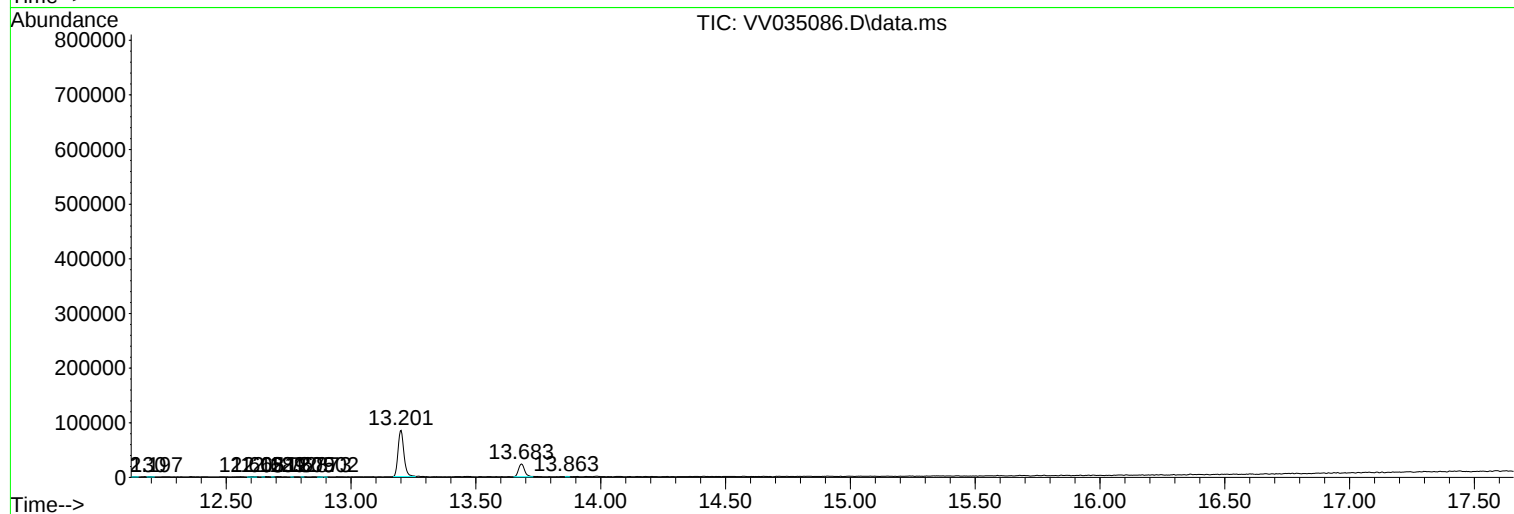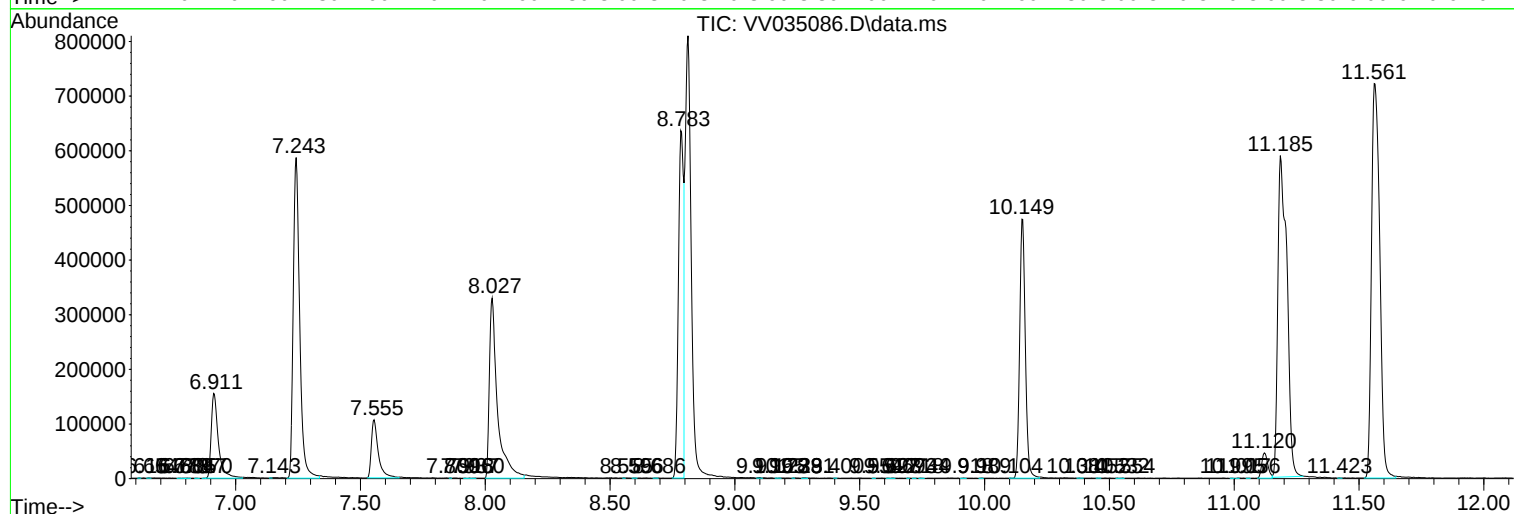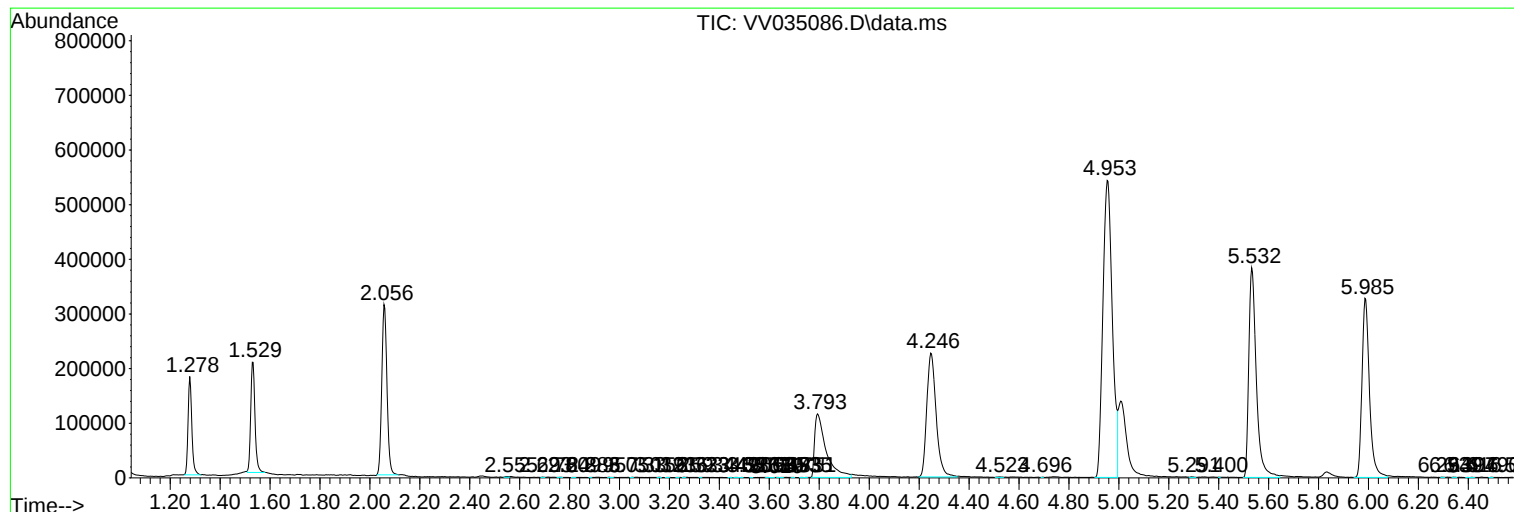

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035086.D
Acq On : 09 Apr 2024 16:39
Operator : SY/MD
Sample : P2006-10DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035086.D
Acq On : 09 Apr 2024 16:39
Operator : SY/MD
Sample : P2006-10DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE9DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
