

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035087.D
 Acq On : 09 Apr 2024 17:03
 Operator : SY/MD
 Sample : P2006-11DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rBV	183691	189418	4.09%	0.847%
2	1.529	146	152	170	rVB	212763	252184	5.44%	1.128%
3	2.056	307	316	335	rBV	322482	470594	10.15%	2.104%
4	2.754	529	533	539	rVB4	568	560	0.01%	0.003%
5	2.857	560	565	569	rBV3	442	462	0.01%	0.002%
6	2.966	596	599	600	rBV2	413	163	0.00%	0.001%
7	2.985	600	605	607	rBV4	447	414	0.01%	0.002%
8	3.056	626	627	629	rBV	242	83	0.00%	0.000%
9	3.079	633	634	638	rBV2	263	145	0.00%	0.001%
10	3.140	651	653	654	rBV2	215	91	0.00%	0.000%
11	3.153	654	657	660	rVV2	343	264	0.01%	0.001%
12	3.198	669	671	673	rBV	125	55	0.00%	0.000%
13	3.268	692	693	695	rVB	211	59	0.00%	0.000%
14	3.310	704	706	708	rBV2	246	125	0.00%	0.001%
15	3.375	725	726	729	rBV2	191	76	0.00%	0.000%
16	3.426	738	742	748	rVB4	428	334	0.01%	0.001%
17	3.458	748	752	754	rBV	371	304	0.01%	0.001%
18	3.542	775	778	783	rBV3	484	429	0.01%	0.002%
19	3.580	788	790	791	rVB3	85	32	0.00%	0.000%
20	3.661	809	815	818	rBV3	680	640	0.01%	0.003%
21	3.706	824	829	834	rVB3	422	289	0.01%	0.001%
22	3.728	834	836	838	rVB3	316	124	0.00%	0.001%
23	3.754	841	844	846	rBV3	434	277	0.01%	0.001%
24	3.789	847	855	890	rBV	117431	356866	7.70%	1.596%
25	4.169	971	973	976	rBV4	827	462	0.01%	0.002%
26	4.246	983	997	1034	rVB	232413	594644	12.83%	2.659%
27	4.596	1105	1106	1107	rBV	445	98	0.00%	0.000%
28	4.702	1137	1139	1141	rBV	429	151	0.00%	0.001%
29	4.837	1179	1181	1183	rBV	248	155	0.00%	0.001%
30	4.863	1187	1189	1194	rVB3	541	313	0.01%	0.001%
31	4.889	1194	1197	1198	rBV2	507	230	0.00%	0.001%
32	4.956	1202	1218	1227	rBV2	562253	1431721	30.90%	6.402%
33	5.429	1363	1365	1367	rVB	669	241	0.01%	0.001%
34	5.532	1386	1397	1429	rBV	407514	863456	18.63%	3.861%
35	5.837	1483	1492	1506	rVB8	7494	16624	0.36%	0.074%
36	5.989	1525	1539	1569	rBV	325994	693063	14.96%	3.099%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035087.D
 Acq On : 09 Apr 2024 17:03
 Operator : SY/MD
 Sample : P2006-11DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.333	1644	1646	1652	rVB3	589	501	0.01%	0.002%
38	6.368	1652	1657	1658	rBV3	340	185	0.00%	0.001%
39	6.381	1658	1661	1664	rBV2	397	318	0.01%	0.001%
40	6.400	1665	1667	1670	rVB2	431	256	0.01%	0.001%
41	6.538	1707	1710	1712	rBV2	317	179	0.00%	0.001%
42	6.548	1712	1713	1714	rVV2	282	94	0.00%	0.000%
43	6.558	1714	1716	1719	rVB	482	218	0.00%	0.001%
44	6.590	1724	1726	1728	rBV	301	136	0.00%	0.001%
45	6.680	1752	1754	1757	rBV3	302	164	0.00%	0.001%
46	6.709	1758	1763	1765	rBV3	443	357	0.01%	0.002%
47	6.799	1787	1791	1799	rVB5	633	793	0.02%	0.004%
48	6.911	1816	1826	1858	rBV	157198	310435	6.70%	1.388%
49	7.243	1918	1929	1959	rBV	610596	1090071	23.52%	4.874%
50	7.554	2017	2026	2058	rBV	110122	205817	4.44%	0.920%
51	7.850	2114	2118	2122	rBV3	791	717	0.02%	0.003%
52	7.892	2129	2131	2133	rBV2	366	186	0.00%	0.001%
53	7.937	2140	2145	2146	rBV2	291	247	0.01%	0.001%
54	7.956	2148	2151	2154	rVB3	685	462	0.01%	0.002%
55	7.972	2154	2156	2157	rBV	193	52	0.00%	0.000%
56	7.988	2158	2161	2163	rBV2	574	336	0.01%	0.002%
57	8.027	2164	2173	2221	rBV2	341669	741014	15.99%	3.313%
58	8.632	2359	2361	2362	rBV	375	175	0.00%	0.001%
59	8.812	2397	2417	2462	rBV2	2021531	4331297	93.47%	19.367%
60	9.175	2526	2530	2532	rBV3	831	742	0.02%	0.003%
61	9.358	2585	2587	2588	rVB	317	89	0.00%	0.000%
62	9.384	2593	2595	2598	rBV2	438	282	0.01%	0.001%
63	9.471	2620	2622	2625	rVB2	575	235	0.01%	0.001%
64	9.564	2649	2651	2654	rBV2	293	147	0.00%	0.001%
65	9.625	2668	2670	2671	rBV	379	91	0.00%	0.000%
66	9.750	2706	2709	2711	rBV2	356	199	0.00%	0.001%
67	9.795	2721	2723	2728	rBV2	307	228	0.00%	0.001%
68	9.869	2742	2746	2751	rBV3	863	870	0.02%	0.004%
69	9.943	2766	2769	2770	rBV	441	236	0.01%	0.001%
70	9.995	2782	2785	2789	rBV2	607	429	0.01%	0.002%
71	10.046	2799	2801	2803	rBV	374	159	0.00%	0.001%
72	10.072	2807	2809	2813	rVB2	262	165	0.00%	0.001%
73	10.091	2813	2815	2819	rBV2	233	155	0.00%	0.001%
74	10.152	2822	2834	2861	rBV	475566	758904	16.38%	3.393%
75	10.471	2931	2933	2935	rVB2	306	102	0.00%	0.000%
76	10.516	2944	2947	2952	rBV2	407	436	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035087.D
 Acq On : 09 Apr 2024 17:03
 Operator : SY/MD
 Sample : P2006-11DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.538	2952	2954	2957	rVV2	647	358	0.01%	0.002%
78	10.567	2961	2963	2964	rBV	215	66	0.00%	0.000%
79	10.612	2972	2977	2979	rBV2	377	329	0.01%	0.001%
80	10.644	2984	2987	2989	rBV	219	167	0.00%	0.001%
81	10.689	3000	3001	3002	rBV	220	72	0.00%	0.000%
82	10.728	3010	3013	3017	rBV2	388	417	0.01%	0.002%
83	10.770	3023	3026	3028	rBV	217	153	0.00%	0.001%
84	10.789	3030	3032	3034	rVB2	372	142	0.00%	0.001%
85	10.824	3040	3043	3049	rVB3	480	500	0.01%	0.002%
86	10.850	3049	3051	3053	rBV	236	164	0.00%	0.001%
87	10.921	3071	3073	3074	rBV	242	116	0.00%	0.001%
88	11.001	3095	3098	3100	rBV3	294	186	0.00%	0.001%
89	11.075	3119	3121	3124	rBV	347	218	0.00%	0.001%
90	11.117	3124	3134	3145	rBV	113510	184353	3.98%	0.824%
91	11.207	3145	3162	3189	rVB2	2196557	4243622	91.57%	18.975%
92	11.574	3260	3276	3301	rBV2	2428068	4634136	100.00%	20.721%
93	12.156	3455	3457	3460	rBV2	457	244	0.01%	0.001%
94	12.348	3512	3517	3518	rBV4	1862	1530	0.03%	0.007%
95	12.689	3620	3623	3624	rBV2	663	433	0.01%	0.002%
96	13.197	3769	3781	3809	rBV	522795	829294	17.90%	3.708%
97	13.397	3841	3843	3846	rBV2	792	514	0.01%	0.002%
98	13.680	3921	3931	3948	rBV	82456	132061	2.85%	0.590%
99	15.335	4440	4446	4459	rBV4	8776	12751	0.28%	0.057%




Sum of corrected areas: 22364451

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035087.D
Acq On : 09 Apr 2024 17:03
Operator : SY/MD
Sample : P2006-11DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

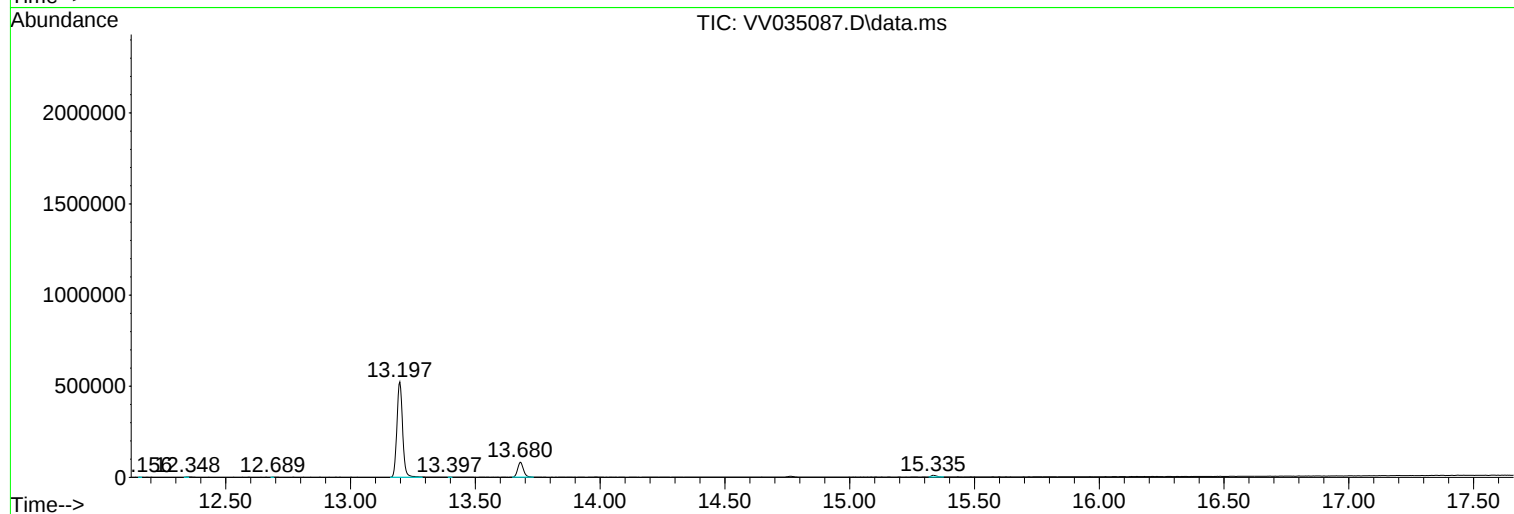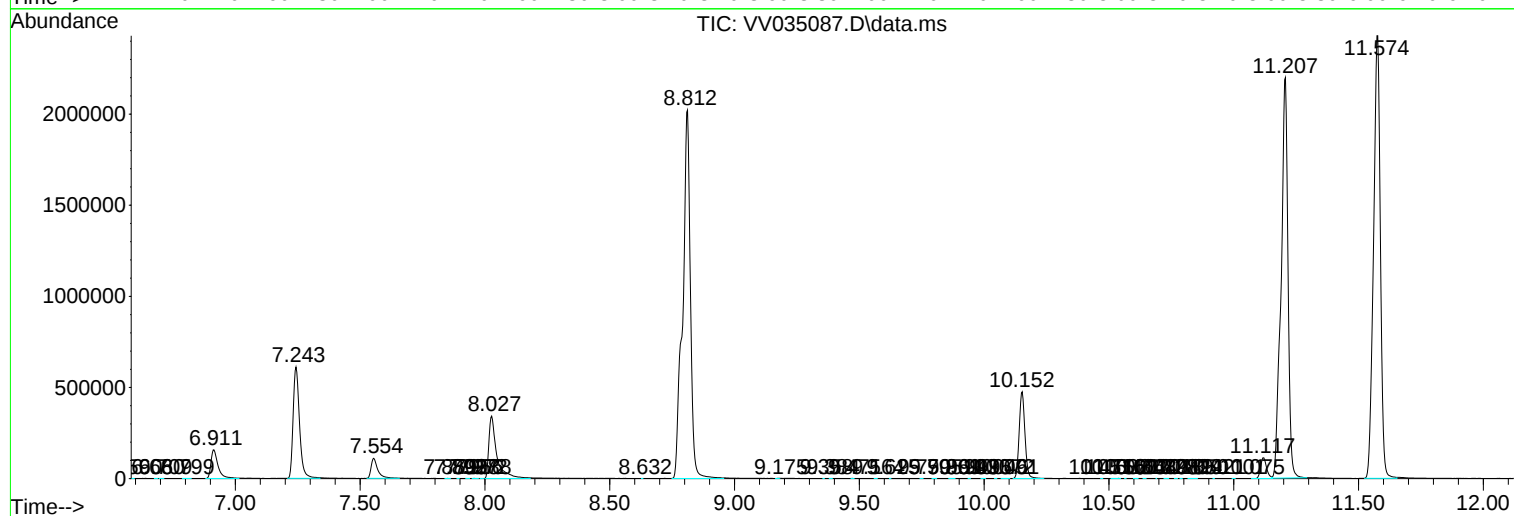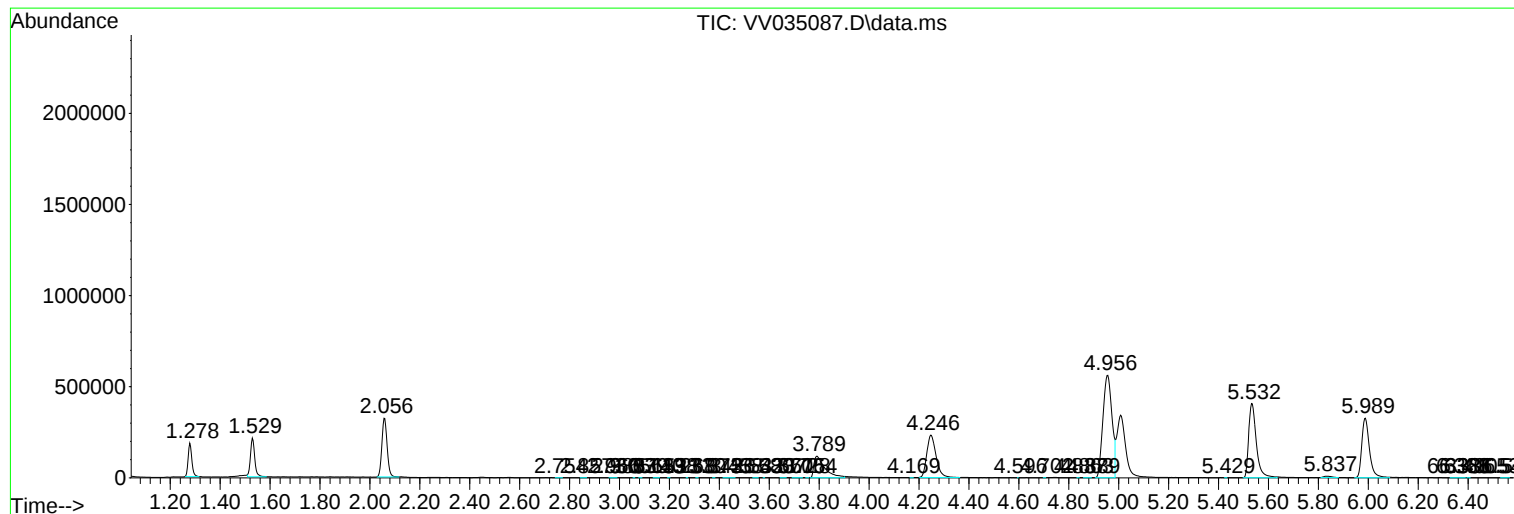

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035087.D
Acq On : 09 Apr 2024 17:03
Operator : SY/MD
Sample : P2006-11DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035087.D
Acq On : 09 Apr 2024 17:03
Operator : SY/MD
Sample : P2006-11DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
