

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035089.D
 Acq On : 09 Apr 2024 17:51
 Operator : SY/MD
 Sample : P2006-15DL2 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RH3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	176770	186759	11.15%	1.581%
2	1.529	146	152	167	rVB	199261	231054	13.79%	1.956%
3	2.056	307	316	332	rBV	310779	451866	26.97%	3.826%
4	2.378	412	416	417	rBV3	791	533	0.03%	0.005%
5	2.600	483	485	486	rBV3	347	150	0.01%	0.001%
6	2.642	494	498	500	rBV2	386	267	0.02%	0.002%
7	2.838	557	559	562	rVB2	455	260	0.02%	0.002%
8	2.857	562	565	567	rBV	512	296	0.02%	0.003%
9	2.883	571	573	578	rVB2	617	359	0.02%	0.003%
10	2.908	578	581	584	rBV	468	239	0.01%	0.002%
11	2.934	584	589	590	rBV3	290	261	0.02%	0.002%
12	2.966	597	599	601	rBV3	453	299	0.02%	0.003%
13	3.050	623	625	629	rVB3	418	246	0.01%	0.002%
14	3.111	641	644	650	rVB4	638	482	0.03%	0.004%
15	3.278	691	696	699	rVB3	409	355	0.02%	0.003%
16	3.301	699	703	704	rBV2	307	204	0.01%	0.002%
17	3.333	710	713	717	rBV	249	199	0.01%	0.002%
18	3.387	727	730	732	rVV3	307	158	0.01%	0.001%
19	3.432	741	744	747	rBV3	289	200	0.01%	0.002%
20	3.490	757	762	763	rBV2	249	164	0.01%	0.001%
21	3.603	794	797	798	rBV2	343	169	0.01%	0.001%
22	3.648	806	811	812	rBV2	281	188	0.01%	0.002%
23	3.789	844	855	896	rBV	118606	358446	21.40%	3.035%
24	4.246	983	997	1029	rBV	223557	576991	34.44%	4.885%
25	4.873	1189	1192	1197	rVB2	358	231	0.01%	0.002%
26	4.902	1199	1201	1202	rBV	345	153	0.01%	0.001%
27	4.953	1202	1217	1230	rBV2	540458	1431528	85.46%	12.120%
28	5.416	1359	1361	1363	rVB	515	240	0.01%	0.002%
29	5.436	1363	1367	1368	rBV4	564	326	0.02%	0.003%
30	5.532	1386	1397	1427	rBV	399708	840442	50.17%	7.116%
31	5.834	1480	1491	1507	rBV4	9756	24761	1.48%	0.210%
32	5.985	1521	1538	1568	rBV	323229	681057	40.66%	5.766%
33	6.436	1675	1678	1680	rBV2	418	223	0.01%	0.002%
34	6.574	1719	1721	1725	rBV	556	438	0.03%	0.004%
35	6.609	1730	1732	1734	rVV2	524	268	0.02%	0.002%
36	6.625	1734	1737	1742	rVB4	645	636	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035089.D
 Acq On : 09 Apr 2024 17:51
 Operator : SY/MD
 Sample : P2006-15DL2 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RH3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.657	1742	1747	1748	rBV2	306	271	0.02%	0.002%
38	6.677	1750	1753	1754	rVV2	471	229	0.01%	0.002%
39	6.699	1758	1760	1762	rBV2	463	219	0.01%	0.002%
40	6.757	1776	1778	1781	rVB2	723	361	0.02%	0.003%
41	6.776	1781	1784	1787	rBV4	442	273	0.02%	0.002%
42	6.792	1787	1789	1792	rVB2	509	212	0.01%	0.002%
43	6.837	1798	1803	1807	rVB3	404	374	0.02%	0.003%
44	6.915	1816	1827	1850	rBV	151870	298168	17.80%	2.525%
45	7.243	1916	1929	1962	rBV	581335	1049009	62.62%	8.882%
46	7.513	2011	2013	2016	rBV3	497	327	0.02%	0.003%
47	7.555	2017	2026	2059	rVV2	103222	203303	12.14%	1.721%
48	8.027	2163	2173	2218	rBV2	327833	725117	43.29%	6.139%
49	8.644	2361	2365	2367	rVB3	593	416	0.02%	0.004%
50	8.661	2367	2370	2371	rBV3	694	317	0.02%	0.003%
51	8.783	2397	2408	2412	rBV	666650	980519	58.53%	8.302%
52	9.185	2530	2533	2535	rBV3	647	302	0.02%	0.003%
53	9.249	2551	2553	2554	rBV	626	223	0.01%	0.002%
54	9.349	2578	2584	2588	rBV3	515	633	0.04%	0.005%
55	9.368	2588	2590	2594	rVV2	432	267	0.02%	0.002%
56	9.390	2594	2597	2601	rVB2	439	323	0.02%	0.003%
57	9.413	2601	2604	2606	rBV3	380	249	0.01%	0.002%
58	9.464	2618	2620	2623	rBV3	371	244	0.01%	0.002%
59	9.593	2655	2660	2664	rVB4	491	495	0.03%	0.004%
60	9.619	2664	2668	2669	rBV	428	211	0.01%	0.002%
61	9.625	2669	2670	2676	rVB4	619	406	0.02%	0.003%
62	9.712	2694	2697	2699	rVV3	429	250	0.01%	0.002%
63	9.738	2703	2705	2711	rVB2	310	266	0.02%	0.002%
64	9.767	2711	2714	2717	rVB2	401	251	0.01%	0.002%
65	9.802	2722	2725	2727	rVB2	342	188	0.01%	0.002%
66	9.818	2727	2730	2732	rBV	310	151	0.01%	0.001%
67	9.879	2746	2749	2751	rBV2	354	176	0.01%	0.001%
68	10.062	2803	2806	2810	rVB	295	151	0.01%	0.001%
69	10.085	2810	2813	2815	rBV	443	251	0.01%	0.002%
70	10.152	2822	2834	2862	rBV	464163	738943	44.11%	6.256%
71	10.371	2899	2902	2905	rBV3	512	363	0.02%	0.003%
72	10.448	2923	2926	2927	rBV2	329	152	0.01%	0.001%
73	10.468	2929	2932	2937	rVV2	476	312	0.02%	0.003%
74	10.522	2944	2949	2952	rVV3	306	279	0.02%	0.002%
75	10.635	2982	2984	2987	rVB2	289	154	0.01%	0.001%
76	10.667	2992	2994	2997	rVB2	653	290	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035089.D
 Acq On : 09 Apr 2024 17:51
 Operator : SY/MD
 Sample : P2006-15DL2 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RH3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.683	2997	2999	3003	rBV	337	267	0.02%	0.002%
78	10.738	3012	3016	3018	rBV	270	190	0.01%	0.002%
79	10.802	3034	3036	3040	rVB2	444	279	0.02%	0.002%
80	10.841	3045	3048	3049	rBV	354	174	0.01%	0.001%
81	10.915	3069	3071	3074	rVB2	597	281	0.02%	0.002%
82	10.937	3075	3078	3080	rBV2	299	186	0.01%	0.002%
83	11.050	3109	3113	3116	rBV3	355	255	0.02%	0.002%
84	11.066	3116	3118	3122	rBV2	431	250	0.01%	0.002%
85	11.120	3126	3135	3145	rBV	49095	81340	4.86%	0.689%
86	11.185	3145	3155	3160	rBV	607662	1007166	60.12%	8.527%
87	11.513	3254	3257	3259	rBV3	472	332	0.02%	0.003%
88	11.564	3259	3273	3296	rBV3	714367	1675160	100.00%	14.183%
89	11.802	3343	3347	3352	rBV5	690	682	0.04%	0.006%
90	11.966	3394	3398	3402	rBV2	542	483	0.03%	0.004%
91	12.053	3423	3425	3428	rVB	376	172	0.01%	0.001%
92	12.072	3429	3431	3437	rVB3	388	295	0.02%	0.002%
93	12.345	3514	3516	3526	rVB5	902	747	0.04%	0.006%
94	12.818	3660	3663	3666	rBV	395	204	0.01%	0.002%
95	12.908	3687	3691	3694	rBV3	627	467	0.03%	0.004%
96	13.197	3771	3781	3801	rBV	120008	192176	11.47%	1.627%
97	13.522	3880	3882	3884	rBV2	590	307	0.02%	0.003%
98	13.683	3923	3932	3946	rBV2	33505	53507	3.19%	0.453%
99	13.802	3966	3969	3973	rBV4	464	453	0.03%	0.004%
100	14.535	4194	4197	4200	rVB4	802	492	0.03%	0.004%




Sum of corrected areas: 11810958

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035089.D
Acq On : 09 Apr 2024 17:51
Operator : SY/MD
Sample : P2006-15DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH3DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

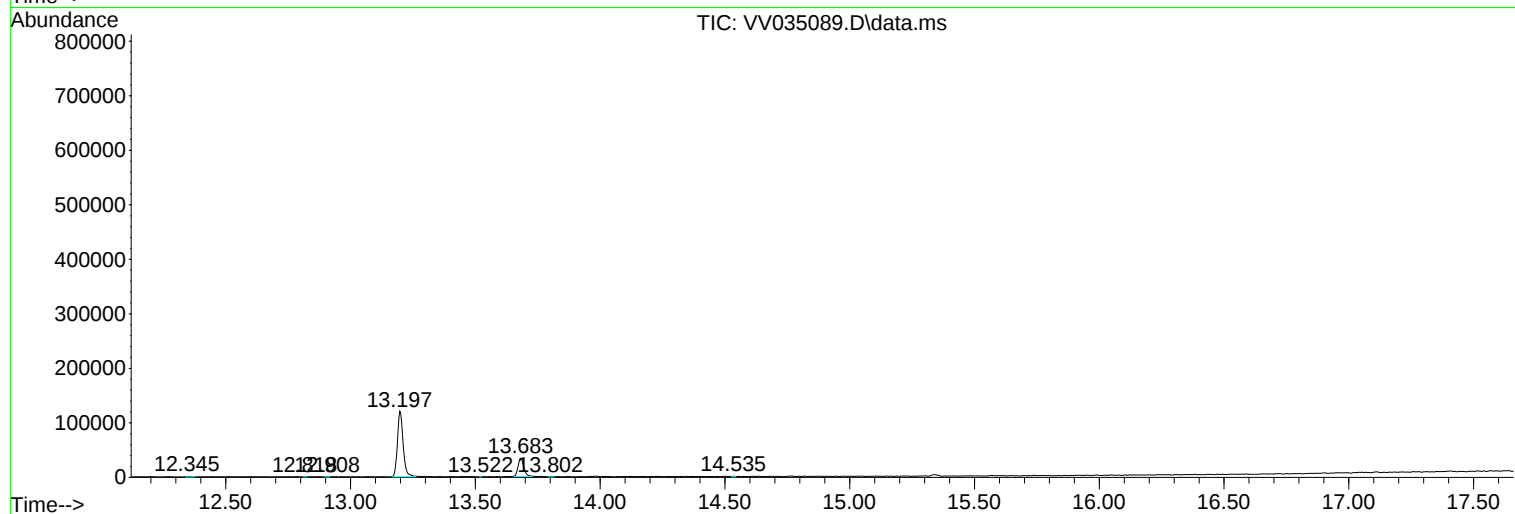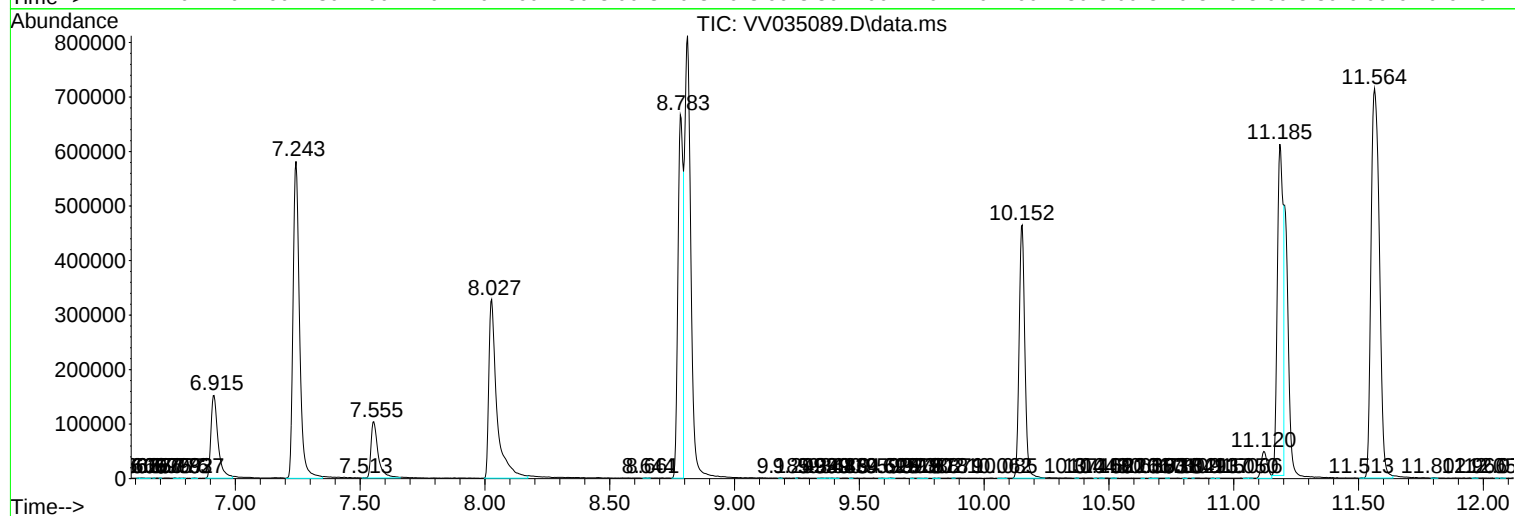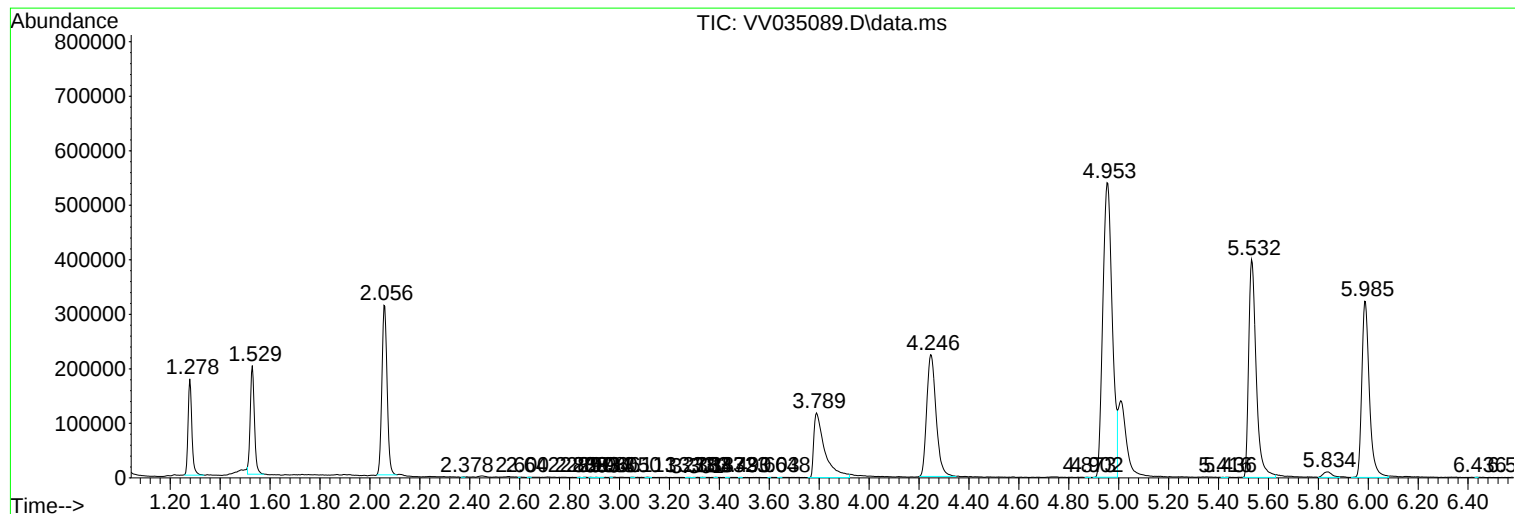

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035089.D
Acq On : 09 Apr 2024 17:51
Operator : SY/MD
Sample : P2006-15DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH3DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035089.D
Acq On : 09 Apr 2024 17:51
Operator : SY/MD
Sample : P2006-15DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RH3DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc