

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035090.D
 Acq On : 09 Apr 2024 18:15
 Operator : SY/MD
 Sample : P2006-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	179342	190421	13.15%	1.775%
2	1.529	146	152	169	rVB	206831	245729	16.97%	2.291%
3	2.056	307	316	335	rVB	317314	462140	31.92%	4.309%
4	2.558	469	472	477	rVB3	654	565	0.04%	0.005%
5	2.590	477	482	484	rBV3	788	603	0.04%	0.006%
6	2.751	529	532	534	rBV2	463	314	0.02%	0.003%
7	2.941	585	591	597	rBV5	610	696	0.05%	0.006%
8	2.973	597	601	603	rBV4	588	409	0.03%	0.004%
9	3.002	607	610	613	rBV4	357	281	0.02%	0.003%
10	3.043	620	623	628	rBV3	418	376	0.03%	0.004%
11	3.169	659	662	664	rVB2	441	176	0.01%	0.002%
12	3.188	665	668	669	rBV	387	203	0.01%	0.002%
13	3.243	681	685	689	rBV2	476	369	0.03%	0.003%
14	3.304	701	704	707	rBV3	352	206	0.01%	0.002%
15	3.346	714	717	721	rVB	503	328	0.02%	0.003%
16	3.423	739	741	744	rBV2	422	274	0.02%	0.003%
17	3.465	751	754	757	rBV2	330	179	0.01%	0.002%
18	3.484	758	760	766	rVB	306	255	0.02%	0.002%
19	3.513	766	769	771	rBV	357	192	0.01%	0.002%
20	3.558	778	783	787	rBV2	295	257	0.02%	0.002%
21	3.600	794	796	800	rBV2	586	438	0.03%	0.004%
22	3.622	800	803	807	rVB3	408	187	0.01%	0.002%
23	3.645	807	810	817	rBV2	590	529	0.04%	0.005%
24	3.693	823	825	828	rVB2	279	161	0.01%	0.002%
25	3.760	843	846	847	rBV	323	203	0.01%	0.002%
26	3.793	847	856	897	rBV	111104	335692	23.19%	3.130%
27	4.246	983	997	1024	rBV	224524	575834	39.78%	5.369%
28	4.805	1164	1171	1173	rBV3	495	532	0.04%	0.005%
29	4.953	1198	1217	1264	rBV2	538437	1447691	100.00%	13.497%
30	5.355	1340	1342	1345	rBV3	519	227	0.02%	0.002%
31	5.445	1366	1370	1373	rBV3	560	383	0.03%	0.004%
32	5.481	1378	1381	1385	rVB5	800	612	0.04%	0.006%
33	5.532	1385	1397	1433	rBV	388950	822512	56.82%	7.668%
34	5.834	1484	1491	1505	rVB5	6895	13935	0.96%	0.130%
35	5.934	1519	1522	1525	rBV3	520	444	0.03%	0.004%
36	5.989	1526	1539	1568	rBV	321288	677145	46.77%	6.313%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035090.D
 Acq On : 09 Apr 2024 18:15
 Operator : SY/MD
 Sample : P2006-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.317	1638	1641	1643	rBV	392	211	0.01%	0.002%
38	6.352	1650	1652	1656	rVB3	778	437	0.03%	0.004%
39	6.387	1660	1663	1667	rVB3	637	392	0.03%	0.004%
40	6.455	1678	1684	1687	rBV3	457	429	0.03%	0.004%
41	6.474	1687	1690	1692	rBV3	388	316	0.02%	0.003%
42	6.526	1703	1706	1710	rVB2	479	375	0.03%	0.003%
43	6.545	1710	1712	1714	rBV	420	164	0.01%	0.002%
44	6.645	1741	1743	1749	rBV3	763	683	0.05%	0.006%
45	6.702	1759	1761	1764	rBV2	625	415	0.03%	0.004%
46	6.760	1778	1779	1781	rBV	354	164	0.01%	0.002%
47	6.812	1790	1795	1799	rBV2	469	339	0.02%	0.003%
48	6.873	1810	1814	1816	rBV3	405	311	0.02%	0.003%
49	6.915	1816	1827	1851	rBV2	149138	297525	20.55%	2.774%
50	7.243	1918	1929	1962	rBV	586097	1045395	72.21%	9.746%
51	7.555	2017	2026	2049	rBV	103967	194763	13.45%	1.816%
52	7.841	2112	2115	2118	rBV2	378	298	0.02%	0.003%
53	7.911	2135	2137	2139	rBV2	405	190	0.01%	0.002%
54	7.956	2149	2151	2153	rBV2	428	193	0.01%	0.002%
55	7.992	2159	2162	2164	rBV2	380	271	0.02%	0.003%
56	8.027	2164	2173	2222	rVV2	316721	725792	50.13%	6.767%
57	8.503	2319	2321	2322	rBV	508	203	0.01%	0.002%
58	8.600	2347	2351	2352	rBV4	357	229	0.02%	0.002%
59	8.609	2352	2354	2356	rBV3	396	205	0.01%	0.002%
60	8.670	2368	2373	2376	rBV4	660	567	0.04%	0.005%
61	8.696	2379	2381	2384	rVB2	384	195	0.01%	0.002%
62	8.731	2390	2392	2394	rBV2	351	191	0.01%	0.002%
63	8.783	2397	2408	2446	rBV	600162	1072272	74.07%	9.997%
64	9.249	2550	2553	2555	rBV2	322	192	0.01%	0.002%
65	9.265	2555	2558	2561	rVB	505	296	0.02%	0.003%
66	9.297	2565	2568	2570	rBV2	381	261	0.02%	0.002%
67	9.378	2589	2593	2596	rBV3	305	276	0.02%	0.003%
68	9.503	2629	2632	2633	rBV	507	246	0.02%	0.002%
69	9.567	2649	2652	2656	rVB2	515	331	0.02%	0.003%
70	9.651	2674	2678	2684	rVB4	573	549	0.04%	0.005%
71	9.699	2689	2693	2696	rVV2	339	271	0.02%	0.003%
72	9.731	2701	2703	2709	rVB	526	428	0.03%	0.004%
73	9.853	2737	2741	2745	rBV2	261	247	0.02%	0.002%
74	9.882	2748	2750	2756	rVB2	467	374	0.03%	0.003%
75	9.915	2756	2760	2762	rBV	359	217	0.01%	0.002%
76	9.934	2762	2766	2769	rBV3	600	582	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
 Data File : VV035090.D
 Acq On : 09 Apr 2024 18:15
 Operator : SY/MD
 Sample : P2006-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.153	2822	2834	2856	rBV	461564	733377	50.66%	6.837%
78	10.384	2904	2906	2909	rVV	348	163	0.01%	0.002%
79	10.419	2915	2917	2919	rBV	333	180	0.01%	0.002%
80	10.490	2938	2939	2944	rBV	352	195	0.01%	0.002%
81	10.532	2948	2952	2957	rBV3	410	432	0.03%	0.004%
82	10.596	2970	2972	2976	rBV3	469	291	0.02%	0.003%
83	10.915	3068	3071	3074	rBV2	335	206	0.01%	0.002%
84	11.127	3132	3137	3143	rVV6	1863	2957	0.20%	0.028%
85	11.185	3144	3155	3188	rVV	532514	884682	61.11%	8.248%
86	11.558	3259	3271	3291	rBV	573355	944735	65.26%	8.808%
87	12.037	3417	3420	3423	rBV3	245	214	0.01%	0.002%
88	12.075	3429	3432	3434	rBV3	423	264	0.02%	0.002%
89	12.156	3455	3457	3459	rBV2	356	166	0.01%	0.002%
90	12.281	3494	3496	3500	rVB2	600	363	0.03%	0.003%
91	12.760	3642	3645	3649	rBV2	520	470	0.03%	0.004%
92	12.831	3664	3667	3669	rBV	463	269	0.02%	0.003%
93	12.892	3684	3686	3688	rBV2	458	208	0.01%	0.002%
94	12.921	3694	3695	3700	rVB	363	160	0.01%	0.001%
95	13.001	3717	3720	3723	rBV2	357	259	0.02%	0.002%
96	13.204	3775	3783	3798	rBV3	13284	22450	1.55%	0.209%
97	13.342	3822	3826	3828	rBV3	482	446	0.03%	0.004%
98	13.512	3876	3879	3884	rBV2	587	468	0.03%	0.004%
99	13.689	3926	3934	3940	rBV6	3557	5500	0.38%	0.051%
100	14.027	4037	4039	4041	rBV3	555	267	0.02%	0.002%




Sum of corrected areas: 10726015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035090.D
Acq On : 09 Apr 2024 18:15
Operator : SY/MD
Sample : P2006-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

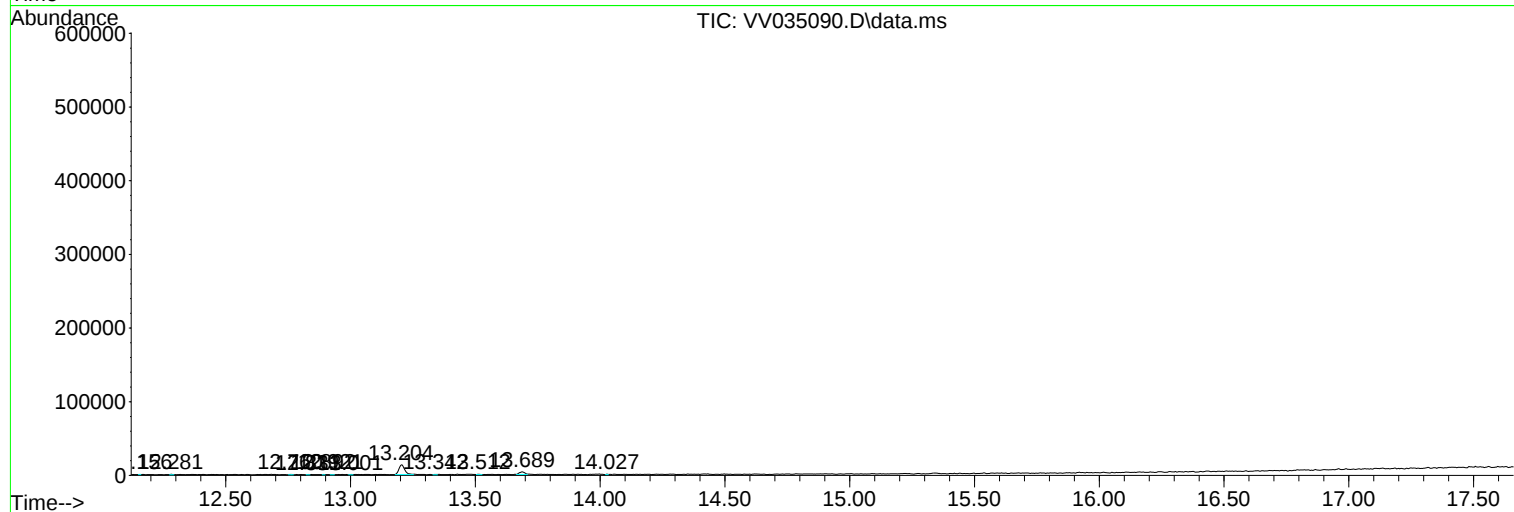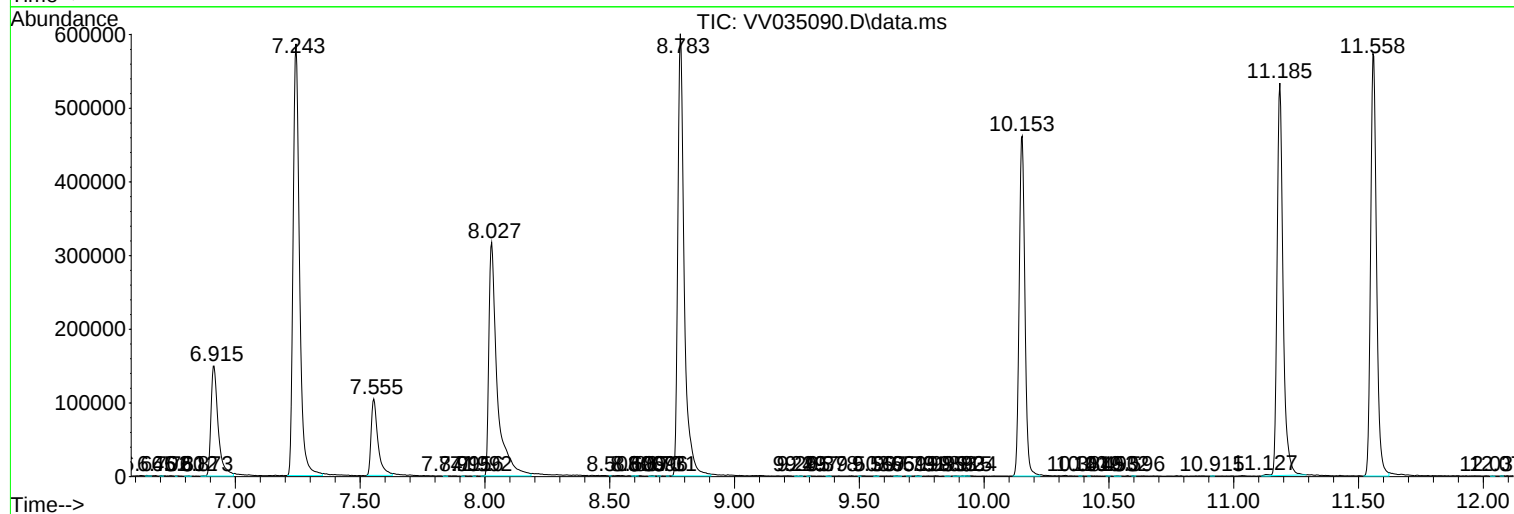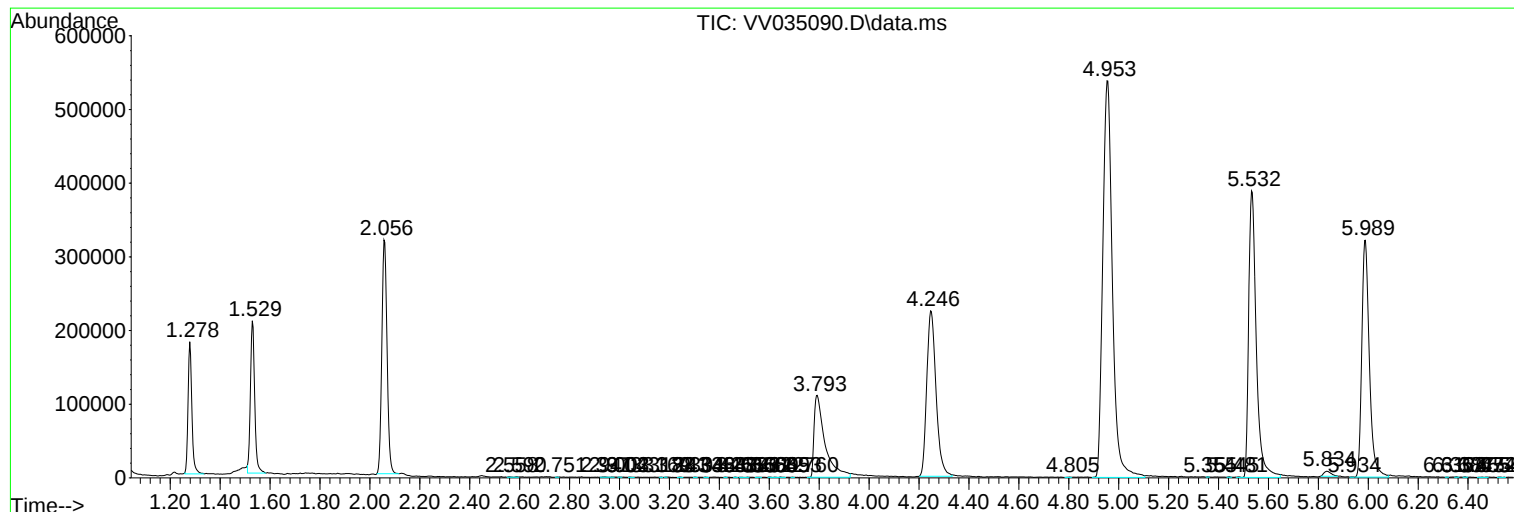

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035090.D
Acq On : 09 Apr 2024 18:15
Operator : SY/MD
Sample : P2006-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035090.D
Acq On : 09 Apr 2024 18:15
Operator : SY/MD
Sample : P2006-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------