


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040924\
Data File : VV035067.D
Acq On : 09 Apr 2024 08:32
Operator : SY/MD
Sample : BFB283
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB283

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Wed Apr 10 04:53:36 2024

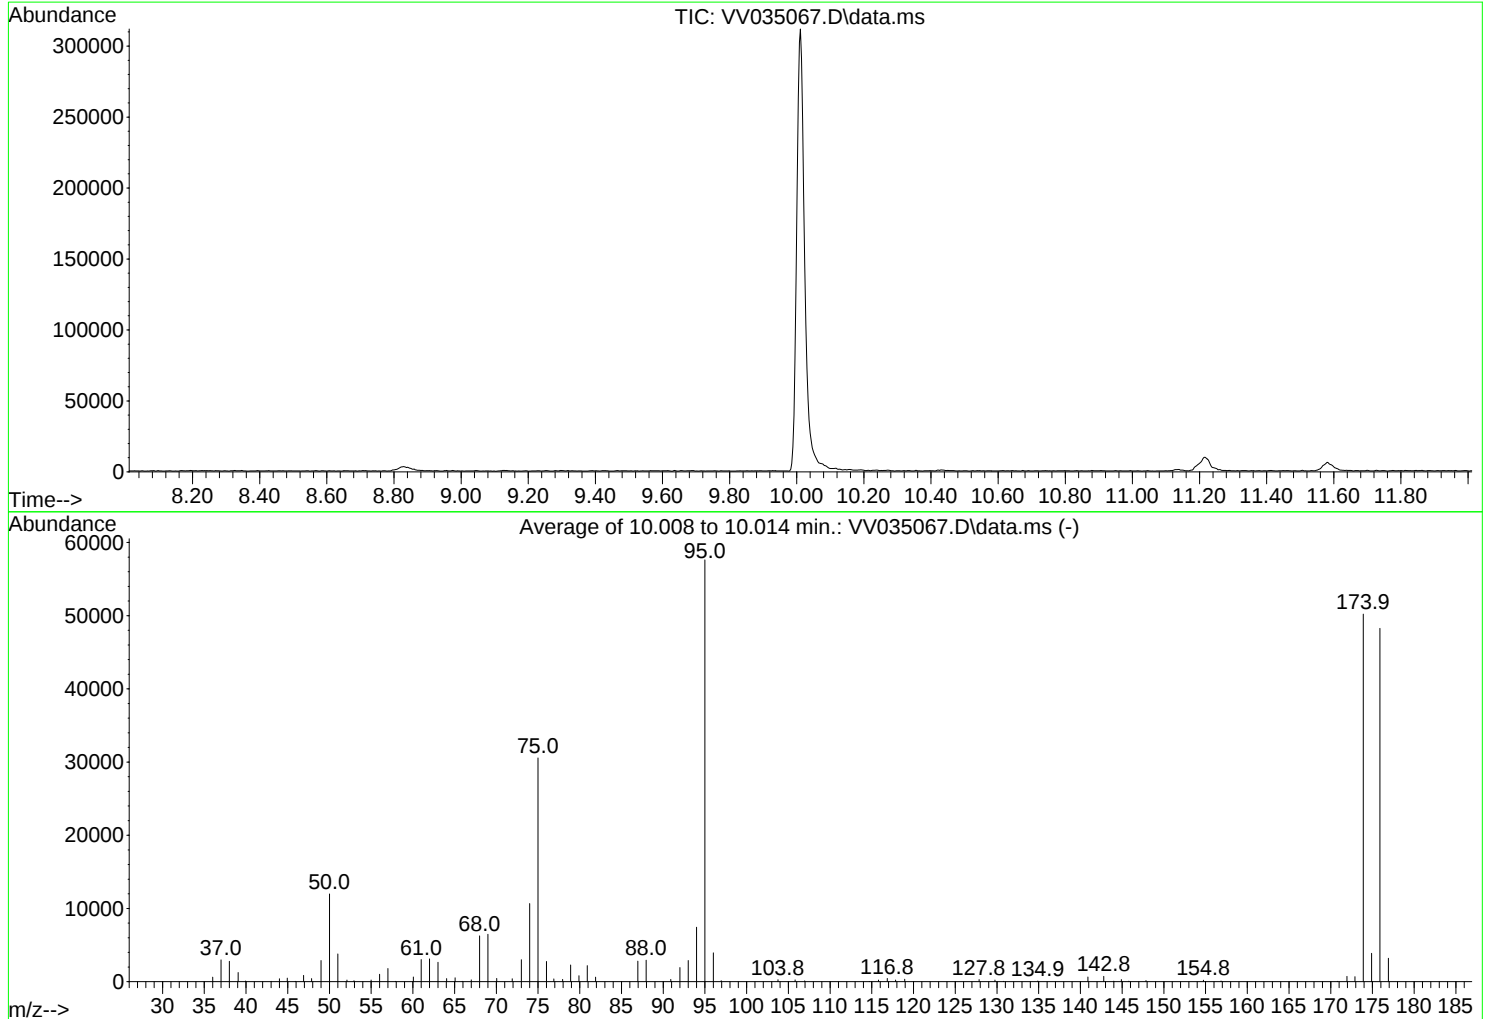

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	11970	PASS
75	95	30	80	53.0	30552	PASS
95	95	100	100	100.0	57629	PASS
96	95	5	9	6.8	3928	PASS
173	174	0.00	2	1.4	684	PASS
174	95	50	120	87.1	50219	PASS
175	174	5	9	7.7	3865	PASS
176	174	95	105	96.1	48259	PASS
177	176	5	10	6.6	3187	PASS

m/z	Abundance
39.90	186.0
44.00	388.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
36.00	598.0
37.00	3115.0
38.00	2927.0
39.00	1227.0
40.00	298.0
44.00	721.0
44.90	491.0
46.90	797.0
47.80	423.0
49.00	2882.0
50.00	12263.0
51.00	3956.0
52.10	217.0
52.90	102.0
55.00	216.0
56.00	959.0
57.00	1796.0
60.10	683.0
61.00	3158.0
62.00	3170.0
63.00	2590.0
64.00	484.0
65.10	496.0
65.90	108.0
66.90	252.0
68.00	6577.0
69.00	6472.0
70.10	448.0
71.90	411.0
73.00	3006.0
74.00	11054.0
75.00	30768.0
76.00	2795.0
76.90	406.0
78.00	284.0
78.90	2339.0
79.90	761.0
80.90	2197.0
81.90	585.0
86.90	2791.0
87.90	3059.0
90.90	276.0
92.00	1981.0
93.00	2821.0
94.00	7631.0
95.00	57656.0
96.00	3942.0
96.90	153.0
103.80	218.0
105.80	251.0
107.00	106.0
115.80	197.0
116.80	455.0
117.90	204.0
118.90	307.0
127.90	235.0
129.70	228.0
130.80	143.0
134.90	134.0
140.90	687.0
142.80	692.0
144.00	118.0
144.90	272.0
145.80	108.0
147.90	100.0
154.70	185.0
156.80	148.0
171.90	749.0
173.00	649.0
173.90	49392.0
174.90	4022.0
175.90	47536.0
176.90	3105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
36.00	620.0
37.00	3088.0
38.00	2828.0
39.10	1299.0
40.00	266.0
43.00	101.0
44.00	805.0
44.90	507.0
45.90	104.0
46.90	876.0
47.90	420.0
49.00	2951.0
50.00	12418.0
51.00	3898.0
52.10	217.0
53.00	148.0
55.00	229.0
56.00	1041.0
57.00	1858.0
60.00	634.0
61.00	3127.0
62.00	3229.0
63.00	2748.0
64.10	412.0
65.00	537.0
67.00	234.0
68.00	6445.0
69.00	6732.0
70.10	442.0
71.90	405.0
73.00	3105.0
74.00	10880.0
75.00	31512.0
76.00	2847.0
76.90	376.0
78.00	309.0
78.90	2365.0
79.90	860.0
80.90	2255.0
81.90	644.0
86.90	2859.0
87.90	3032.0
90.90	313.0
92.00	2011.0
93.00	2956.0
94.00	7686.0
95.00	59472.0
96.00	4046.0
96.90	137.0
103.70	267.0
105.80	267.0
107.00	114.0
114.70	100.0
115.80	218.0
116.90	430.0
117.90	232.0
118.90	330.0
127.90	289.0
129.70	246.0
134.90	110.0
140.90	679.0
142.80	769.0
144.00	113.0
144.90	279.0
145.80	100.0
147.80	159.0
154.80	209.0
156.90	131.0
171.90	753.0
172.90	716.0
173.90	52024.0
174.90	3973.0
175.90	50008.0
176.90	3255.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
36.00	625.0
37.00	2741.0
38.00	2549.0
39.10	1234.0
40.00	234.0
44.00	814.0
45.00	477.0
46.90	866.0
47.90	383.0
49.00	2825.0
50.00	11229.0
51.00	3487.0
52.10	208.0
53.00	133.0
55.00	218.0
56.00	1025.0
57.00	1742.0
57.90	109.0
60.00	580.0
61.00	2781.0
62.00	2947.0
63.00	2594.0
64.10	334.0
65.00	528.0
67.10	215.0
68.00	5747.0
69.00	6221.0
70.00	433.0
71.90	371.0
73.00	2853.0
74.00	10047.0
75.00	29376.0
76.00	2658.0
76.90	351.0
77.90	306.0
78.90	2149.0
79.90	814.0
80.90	2113.0
81.90	634.0
87.00	2723.0
88.00	2732.0
90.90	318.0
92.00	1780.0
93.00	2867.0
94.00	6982.0
95.00	55760.0
96.00	3797.0
97.00	104.0
103.70	295.0
105.80	240.0
106.90	102.0
115.80	232.0
116.90	416.0
117.80	247.0
119.00	356.0
127.80	313.0
129.80	202.0
140.90	565.0
142.80	719.0
144.90	279.0
147.80	199.0
154.80	196.0
170.80	103.0
172.00	684.0
172.80	688.0
173.90	49240.0
174.90	3600.0
175.90	47232.0
176.90	3201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283