

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV041019\
 Data File : VV010225.D
 Acq On : 10 Apr 2019 22:16
 Operator : SY/MD
 Sample : K2246-21
 Misc : 5.02G/10mL/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 08:06:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 07:05:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	264017	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	261368	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	113429	25.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.32	65	63551	20.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.64%
7) Chloroethane-d5	1.57	69	61072	23.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.52%
10) 1,1-Dichloroethene-d2	2.13	63	124223	16.06	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.24%
20) 2-Butanone-d5	3.93	46	43309	56.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.62%
24) Chloroform-d	4.40	84	130010	21.56	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.24%
26) 1,2-Dichloroethane-d4	5.08	65	84892	24.72	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.88%
29) Benzene-d6	5.10	84	282924	22.45	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.80%
33) 1,2-Dichloropropane-d6	6.12	67	83527	22.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.12%
37) Toluene-d8	7.36	98	277052	22.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.16%
38) trans-1,3-Dichloropropene-	7.66	79	35690	22.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.36%
39) 2-Hexanone-d5	8.13	63	30020	46.37	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.74%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	79148	23.52	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.08%
61) 1,2-Dichlorobenzene-d4	11.67	152	103639	24.74	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.96%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	9739	1.884 ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV041019\
Data File : VV010225.D
Acq On : 10 Apr 2019 22:16
Operator : SY/MD
Sample : K2246-21
Misc : 5.02G/10mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 08:06:01 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM041019S.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 07:05:16 2019
Response via : Initial Calibration

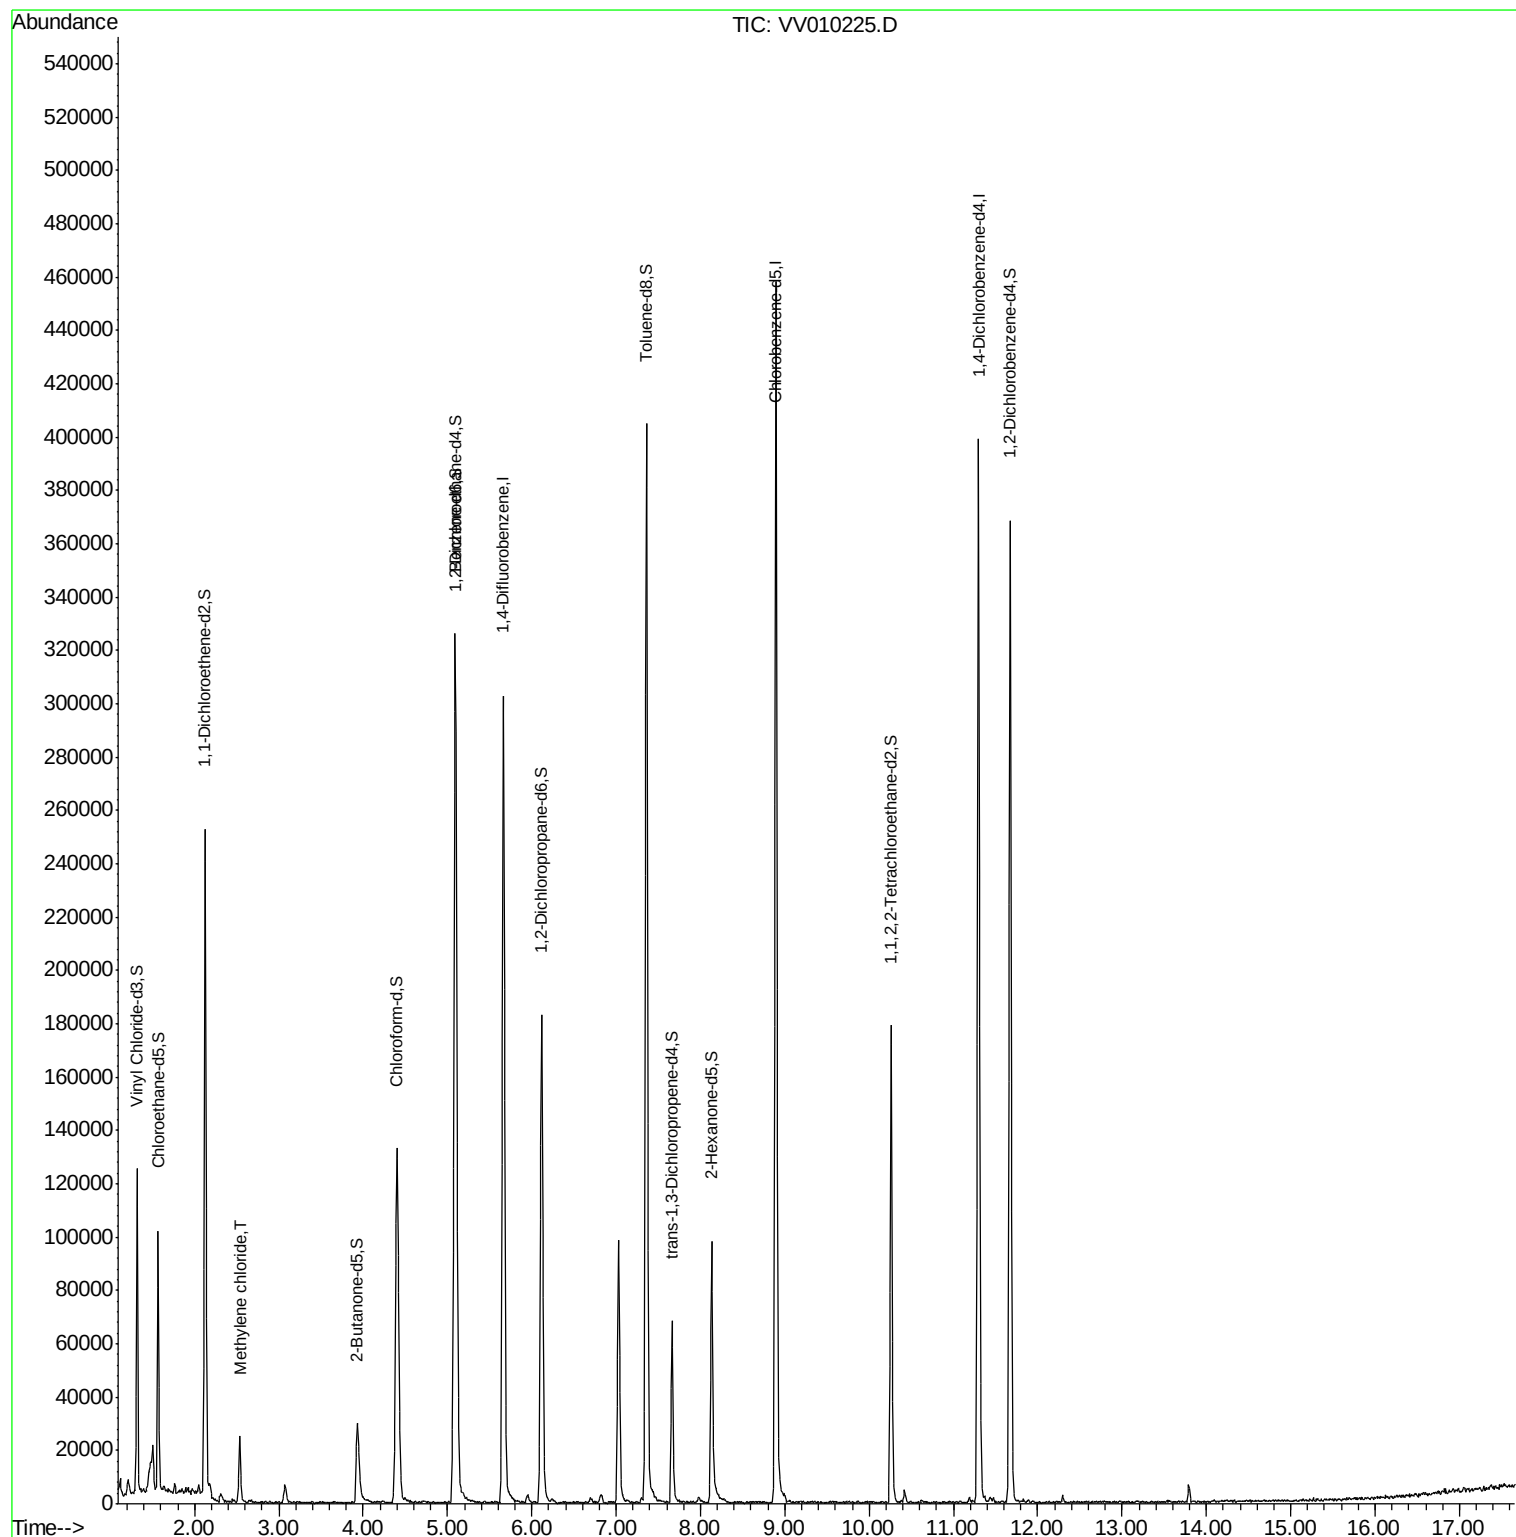

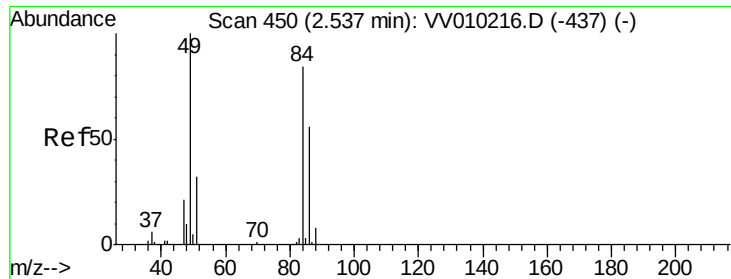

#16
 Methylene chloride
 Concen: 1.884 ug/L
 RT: 2.54 min Scan# 450
 Delta R.T. 0.00 min
 Lab File: VV010225.D
 Acq: 10 Apr 2019 22:16

Tot Ion: 84 Resp: 9739
 Ion Ratio Lower Upper
 84 100
 49 118.1 79.9 148.5
 86 64.3 44.5 82.7

