


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV041020\
 Data File : VV015448.D
 Acq On : 10 Apr 2020 09:41
 Operator : SY/MD
 Sample : BFB33
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB33

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Apr 13 05:05:59 2020

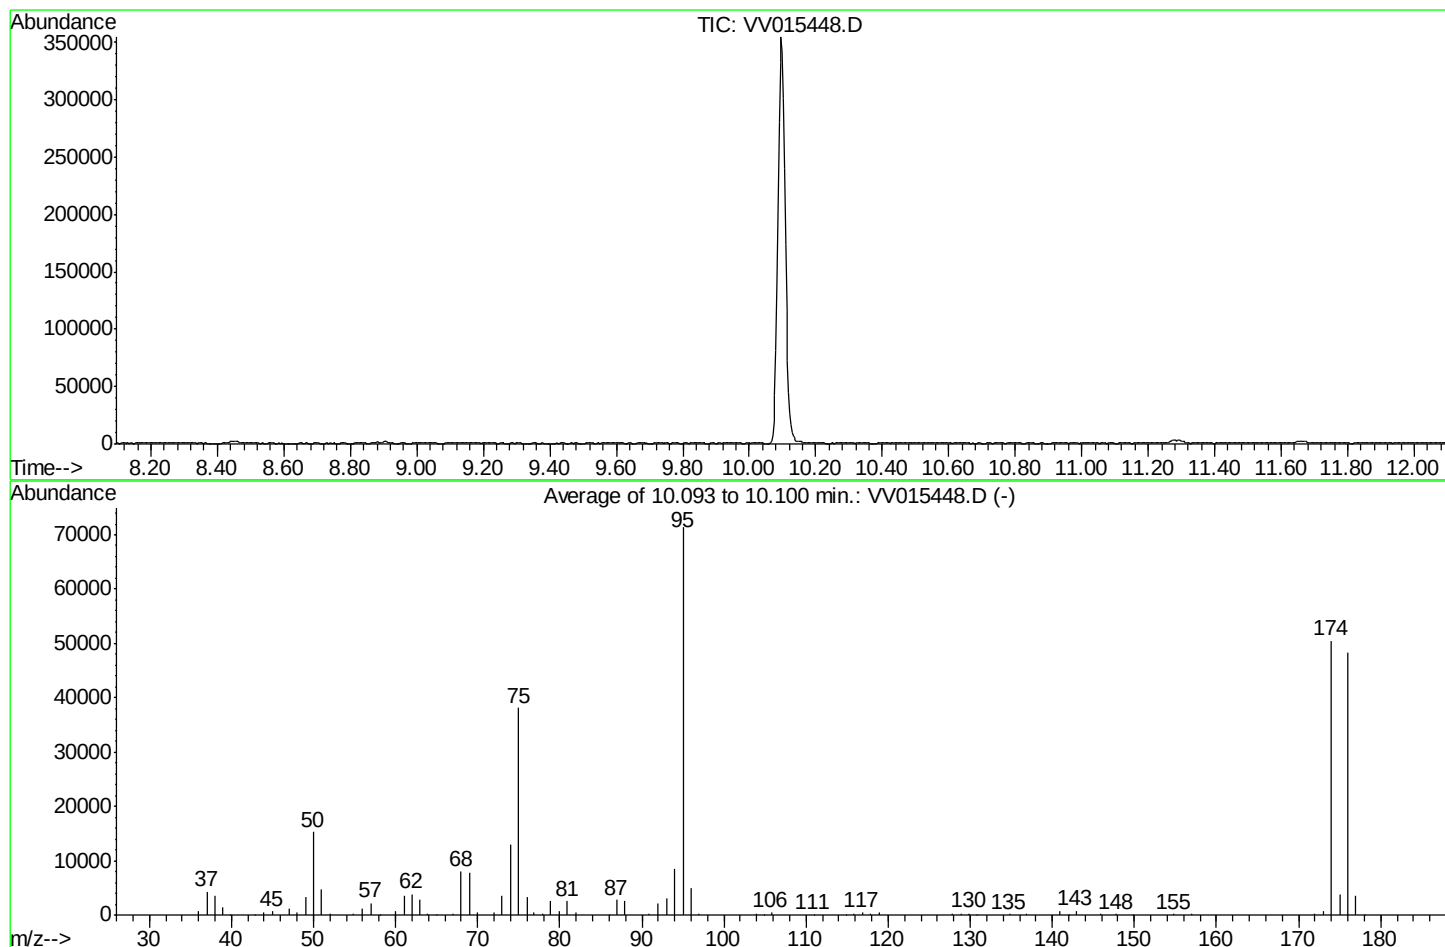

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	15309	PASS
75	95	30	80	53.5	38178	PASS
95	95	100	100	100.0	71378	PASS
96	95	5	9	6.8	4850	PASS
173	174	0.00	2	1.3	659	PASS
174	95	50	120	70.7	50466	PASS
175	174	5	9	7.7	3878	PASS
176	174	95	101	95.6	48232	PASS
177	176	5	9	7.1	3435	PASS

m/z	Abundance
36.00	756.0
37.00	4302.0
38.00	3626.0
39.00	1412.0
39.90	343.0
44.00	792.0
45.00	654.0
47.00	1006.0
48.00	516.0
49.00	3421.0
50.00	15452.0
51.00	4520.0
52.00	254.0
54.90	249.0
56.00	1185.0
57.00	2113.0
58.10	113.0
59.90	826.0
61.00	3615.0
62.00	3748.0
63.00	2699.0
63.90	347.0
64.90	102.0
66.90	220.0
68.00	7693.0
69.00	7651.0
70.00	575.0
71.90	439.0
73.00	3508.0
74.00	12954.0
75.00	37352.0
76.00	3363.0
76.90	401.0
77.90	269.0
78.90	2386.0
79.90	773.0
80.90	2485.0
81.90	501.0
86.10	106.0
86.90	2613.0
87.90	2417.0
90.90	311.0
92.00	2112.0
93.00	2912.0
94.00	8284.0
95.00	69608.0
96.00	4781.0
97.00	180.0
103.90	361.0
104.90	108.0
105.80	328.0
110.90	117.0
115.80	332.0
116.90	412.0
117.90	317.0
118.90	428.0
127.80	241.0
128.80	168.0
129.90	233.0
134.80	153.0
136.80	137.0
140.90	731.0
142.90	714.0
145.90	118.0
147.80	166.0
154.80	198.0
156.90	130.0
171.90	210.0
173.00	626.0
174.00	47776.0
175.00	3741.0
176.00	45576.0
177.00	3359.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.00	796.0
37.00	4438.0
38.00	3730.0
39.00	1516.0
39.90	359.0
42.90	109.0
44.00	874.0
45.00	638.0
47.00	1127.0
48.00	563.0
49.00	3556.0
50.00	15810.0
51.00	4800.0
52.10	211.0
54.90	279.0
56.00	1267.0
57.00	2234.0
58.10	123.0
59.90	782.0
61.00	3677.0
62.00	3971.0
63.00	2941.0
64.00	377.0
66.90	214.0
68.00	8231.0
69.00	7990.0
70.00	615.0
71.90	454.0
73.00	3627.0
74.00	13445.0
75.00	39376.0
76.00	3492.0
76.90	461.0
77.80	276.0
78.90	2585.0
79.90	815.0
80.90	2674.0
81.90	507.0
85.90	119.0
86.90	2851.0
88.00	2606.0
90.90	284.0
92.00	2220.0
93.00	3211.0
94.00	8861.0
95.00	73472.0
96.00	5027.0
97.00	171.0
103.90	363.0
104.90	121.0
105.80	382.0
110.90	127.0
115.80	316.0
116.80	456.0
117.90	362.0
118.90	445.0
127.80	281.0
128.90	158.0
129.80	284.0
130.90	102.0
134.80	148.0
136.90	136.0
140.90	832.0
142.00	122.0
142.90	814.0
145.90	139.0
147.80	212.0
149.80	107.0
154.90	230.0
156.90	163.0
172.00	216.0
173.00	696.0
174.00	52224.0
175.00	4012.0
176.00	49712.0
177.00	3548.0
178.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.00	751.0
37.00	4115.0
38.00	3425.0
39.00	1432.0
39.90	346.0
42.90	107.0
44.00	924.0
45.00	617.0
47.00	1104.0
48.00	526.0
49.00	3304.0
50.00	14667.0
51.00	4575.0
52.00	161.0
54.90	279.0
56.00	1254.0
57.00	2183.0
58.10	114.0
60.00	706.0
61.00	3539.0
62.00	3629.0
63.00	2843.0
64.00	348.0
67.00	223.0
68.00	7902.0
69.00	7649.0
70.00	607.0
72.00	435.0
73.00	3373.0
74.00	12738.0
75.00	37808.0
76.00	3264.0
76.90	502.0
77.80	255.0
78.90	2523.0
79.90	729.0
80.90	2605.0
81.90	480.0
85.90	136.0
86.90	2747.0
87.90	2593.0
90.90	260.0
92.00	2148.0
93.00	3241.0
94.00	8502.0
95.00	71056.0
96.00	4742.0
97.00	132.0
103.90	338.0
104.90	112.0
105.80	385.0
114.90	106.0
115.80	292.0
116.90	443.0
117.90	324.0
118.90	393.0
127.80	274.0
128.80	138.0
129.90	310.0
130.80	111.0
134.80	134.0
137.00	132.0
140.90	787.0
141.90	131.0
142.90	869.0
145.80	132.0
147.80	220.0
149.80	117.0
154.90	225.0
157.00	179.0
172.10	233.0
173.00	657.0
174.00	51400.0
175.00	3882.0
176.00	49408.0
177.00	3399.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

Scan 2788 (10.055 min): VV015448.D
BFB33

m/z	Abundance
39.90	236.0
43.90	293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33