

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041023\
 Data File : VW030465.D
 Acq On : 10 Apr 2023 13:51
 Operator : SY/MD
 Sample : 02254-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD8

Quant Time: Apr 11 06:28:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 11 06:24:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	128925	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	125357	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	62494	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	30579	3.581	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.600%
7) Chloroethane-d5	1.536	69	35141	4.241	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.800%
11) 1,1-Dichloroethene-d2	2.066	63	57453	2.836	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.800%#
20) 2-Butanone-d5	3.812	46	93088	42.178	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.360%
24) Chloroform-d	4.262	84	93384	4.519	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%
26) 1,2-Dichloroethane-d4	4.954	65	45638	4.681	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%
32) Benzene-d6	4.970	84	160211	4.535	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.800%
36) 1,2-Dichloropropane-d6	5.998	67	50830	4.596	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.000%
41) Toluene-d8	7.252	98	137271	4.232	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.600%
43) trans-1,3-Dichloroprop...	7.561	79	16460	3.953	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.000%
46) 2-Hexanone-d5	8.034	63	69748	41.686	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.380%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	37421	4.293	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.800%
66) 1,2-Dichlorobenzene-d4	11.571	152	55645	4.982	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.600%
Target Compounds						
					Qvalue	
13) Acetone	2.140	43	5225	2.476	ug/L	62
42) Toluene	7.330	91	8721	0.184	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030465.D
Acq On : 10 Apr 2023 13:51
Operator : SY/MD
Sample : 02254-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD8

Quant Time: Apr 11 06:28:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 11 06:24:59 2023
Response via : Initial Calibration

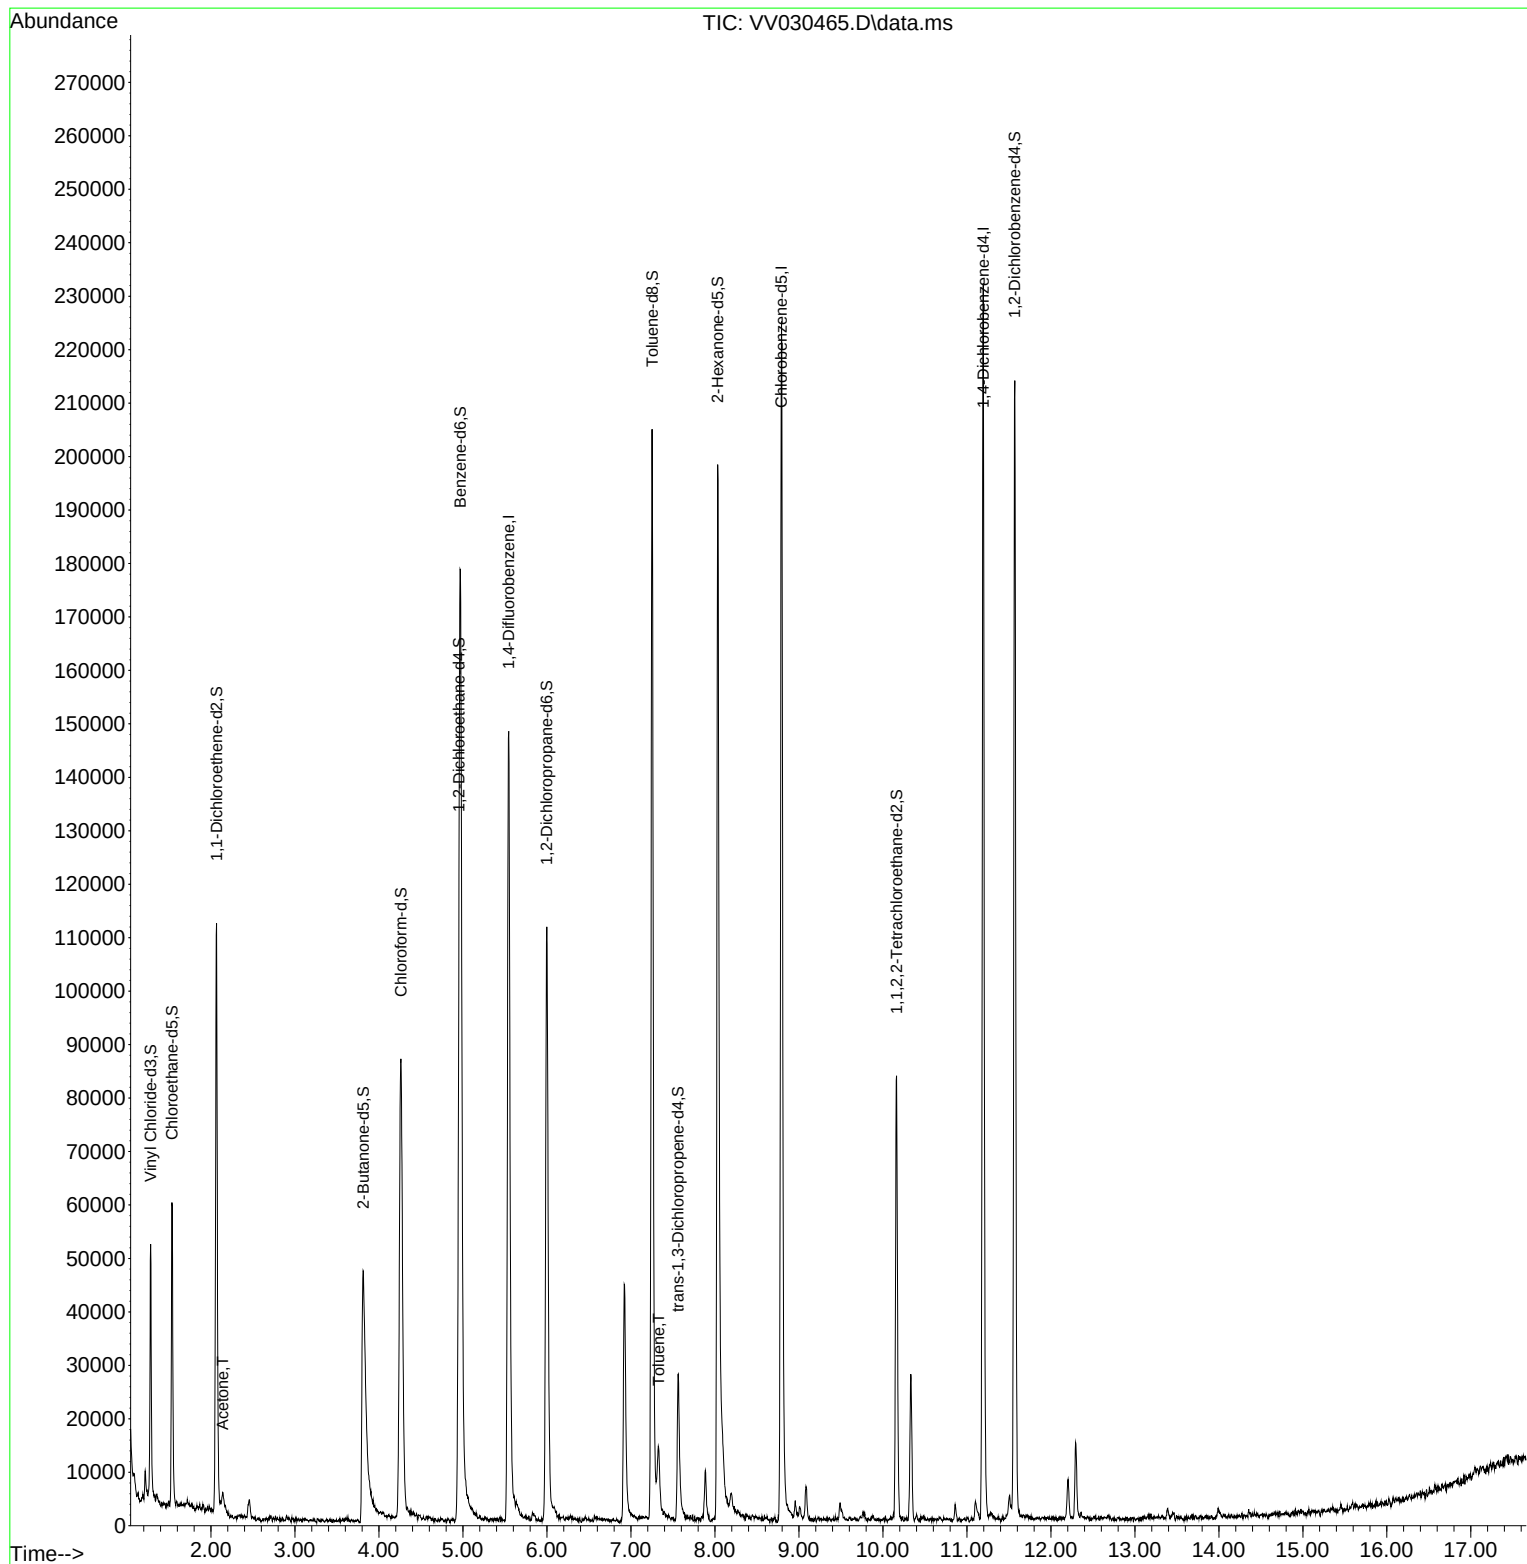

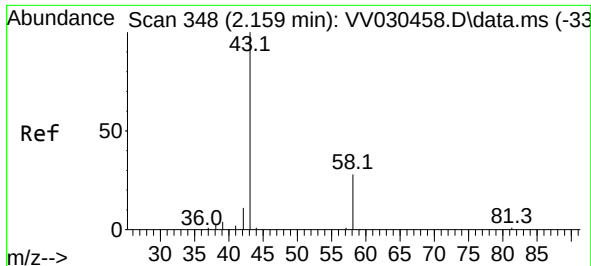

#13

Acetone

Concen: 2.476 ug/L

RT: 2.140 min Scan# 34

Delta R.T. -0.019 min

Lab File: VV030465.D

Acq: 10 Apr 2023 13:51

Instrument :

MSVOA_V

ClientSampleId :





C0AD8

Tgt Ion: 43 Resp: 5225

Ion Ratio Lower Upper

43 100

58 38.2 0.0 40.8

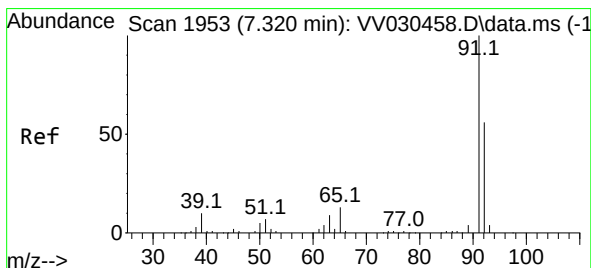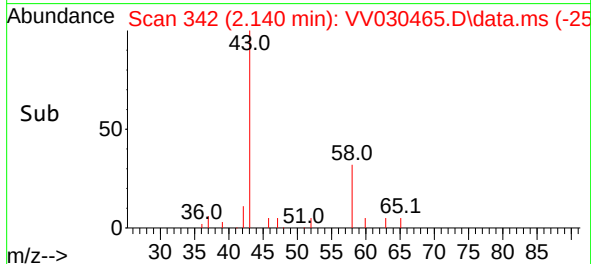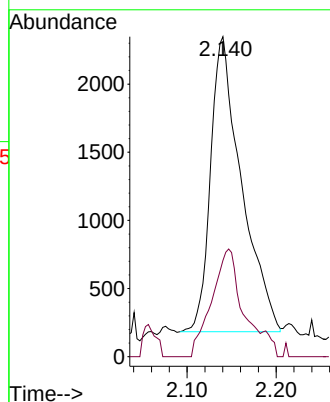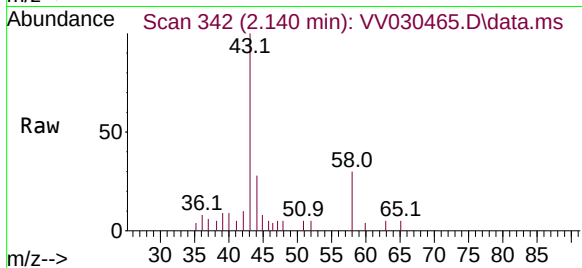

#42

Toluene

Concen: 0.184 ug/L

RT: 7.330 min Scan# 1956

Delta R.T. 0.010 min

Lab File: VV030465.D

Acq: 10 Apr 2023 13:51

Tgt Ion: 91 Resp: 8721

Ion Ratio Lower Upper

91 100

92 58.6 40.4 75.0

