

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041023\
 Data File : VW030473.D
 Acq On : 10 Apr 2023 17:24
 Operator : SY/MD
 Sample : 02225-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Quant Time: Apr 11 06:30:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 11 06:24:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	118815	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	117262	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	58080	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	27245	3.462	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.200%
7) Chloroethane-d5	1.539	69	30471	3.990	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.800%
11) 1,1-Dichloroethene-d2	2.063	63	50417	2.700	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.000%#
20) 2-Butanone-d5	3.821	46	86128	42.345	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.700%
24) Chloroform-d	4.259	84	82635	4.339	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%
26) 1,2-Dichloroethane-d4	4.953	65	40741	4.534	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.600%
32) Benzene-d6	4.973	84	142117	4.301	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
36) 1,2-Dichloropropane-d6	5.998	67	45986	4.445	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.000%
41) Toluene-d8	7.252	98	121510	4.004	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.000%
43) trans-1,3-Dichloroprop...	7.564	79	15110	3.879	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.600%
46) 2-Hexanone-d5	8.037	63	63855	40.798	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.600%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	35215	4.319	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	11.570	152	49535	4.772	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.400%
Target Compounds						Qvalue
29) 1,1,1-Trichloroethane	4.526	97	5660	0.300	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030473.D
Acq On : 10 Apr 2023 17:24
Operator : SY/MD
Sample : 02225-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Time: Apr 11 06:30:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 11 06:24:59 2023
Response via : Initial Calibration

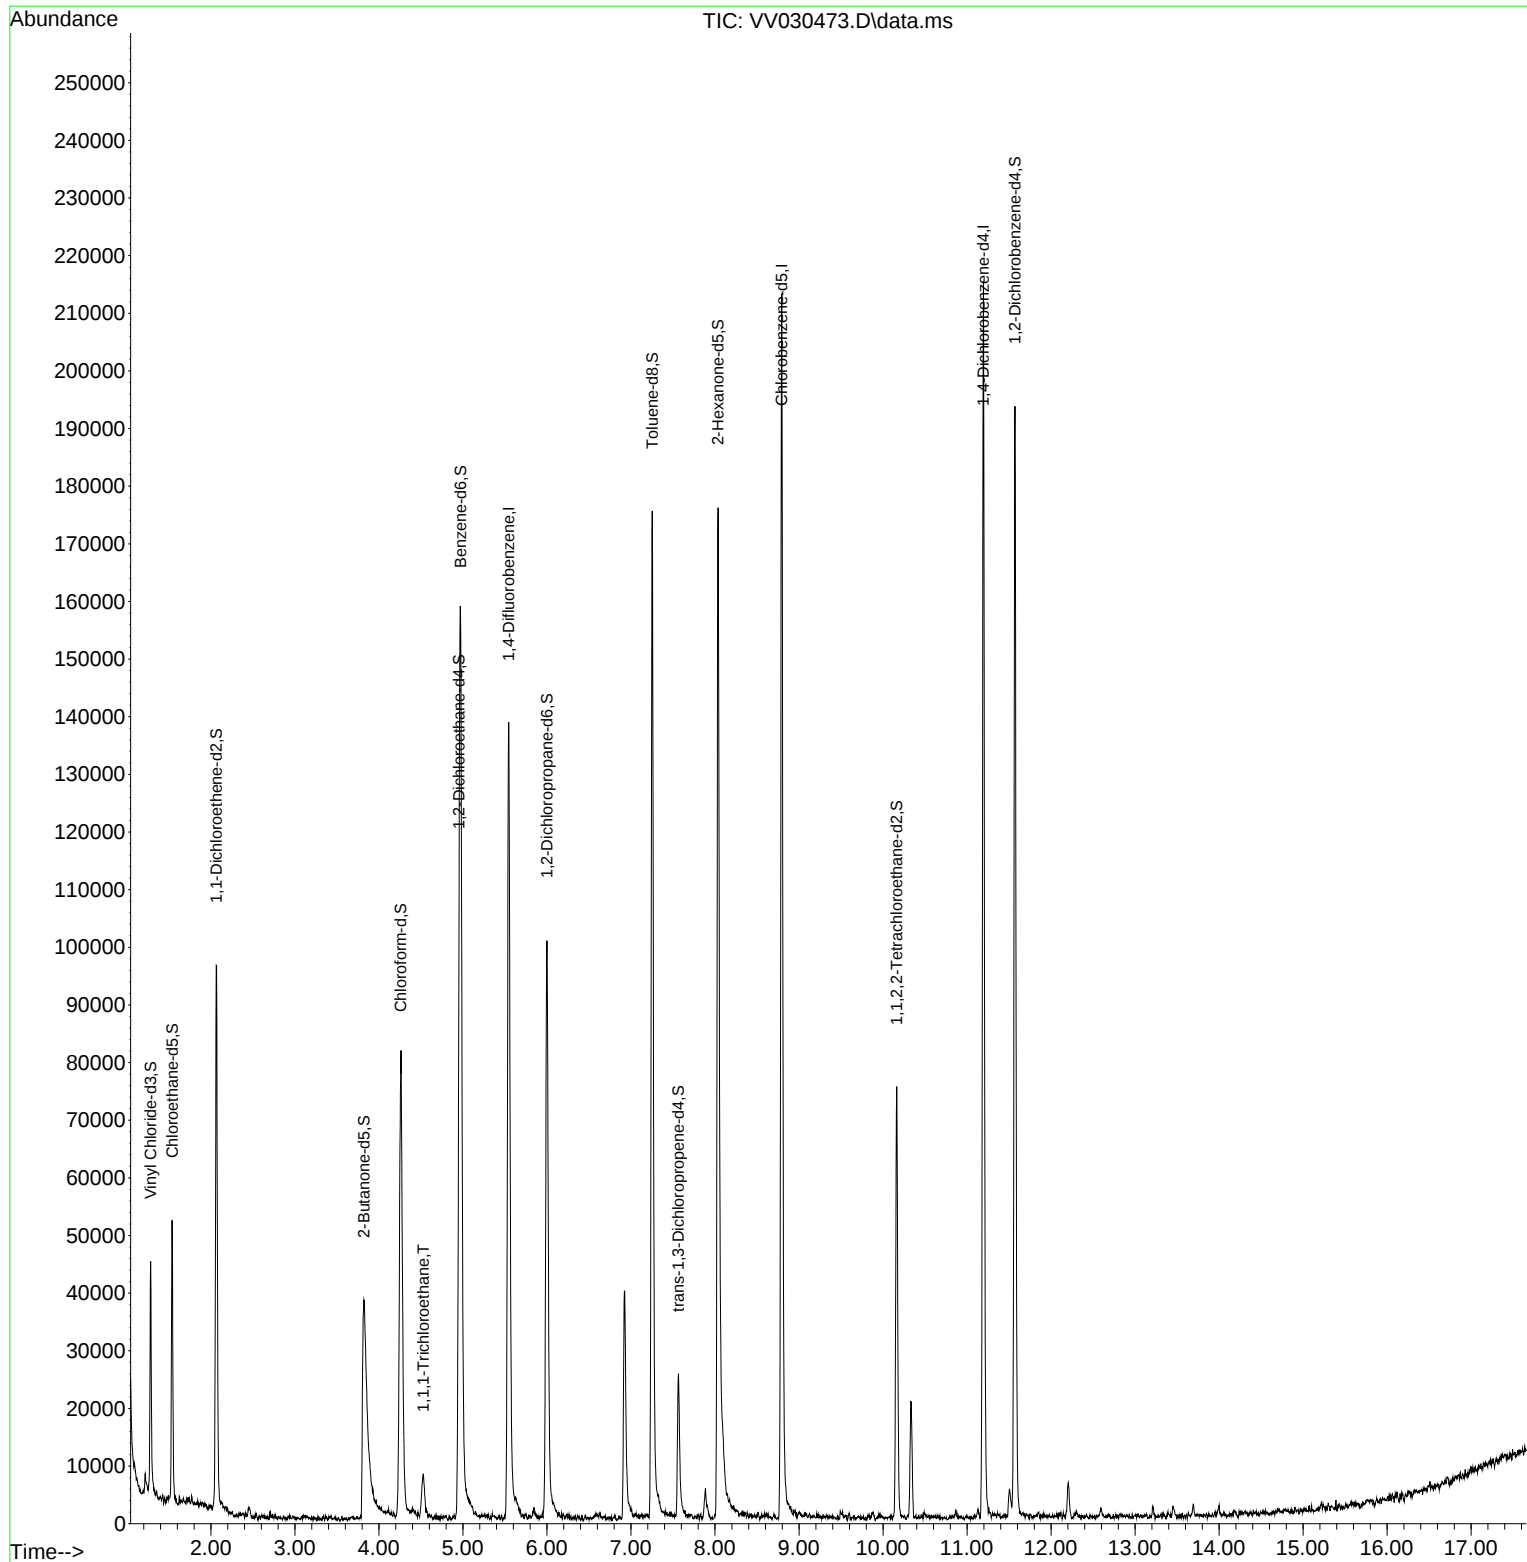

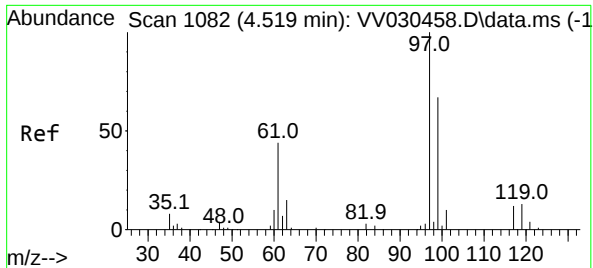

#29
 1,1,1-Trichloroethane
 Concen: 0.300 ug/L
 RT: 4.526 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV030473.D
 Acq: 10 Apr 2023 17:24

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Tgt Ion: 97 Resp: 5660

Ion	Ratio	Lower	Upper
97	100		
99	69.7	50.9	76.3
61	47.7	35.9	53.9

