

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
 Data File : VV030460.D
 Acq On : 10 Apr 2023 11:51
 Operator : SY/MD
 Sample : 02250-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDY0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	47374	52710	11.93%	1.399%
2	1.535	147	154	167	rVB	53846	64554	14.61%	1.713%
3	2.063	309	318	329	rBV	100053	146783	33.23%	3.895%
4	3.815	851	863	898	rBV	36856	150201	34.00%	3.986%
5	4.256	985	1000	1022	rBV	83849	217831	49.31%	5.780%
6	4.966	1203	1221	1244	rBV2	169136	441783	100.00%	11.723%
7	5.542	1385	1400	1419	rBV2	136505	292398	66.19%	7.759%
8	5.998	1528	1542	1559	rBV	107006	225525	51.05%	5.984%
9	6.921	1814	1829	1844	rBV	42978	82966	18.78%	2.202%
10	7.249	1919	1931	1944	rBV	187240	338177	76.55%	8.974%
11	7.326	1946	1955	1972	rVB	49685	96420	21.83%	2.559%
12	7.561	2017	2028	2044	rBV2	26265	52524	11.89%	1.394%
13	7.882	2119	2128	2130	rBV5	3817	4822	1.09%	0.128%
14	8.034	2163	2175	2203	rBV	180751	370683	83.91%	9.836%
15	8.792	2397	2411	2431	rBV	217337	365155	82.65%	9.690%
16	9.506	2621	2633	2646	rBV8	4678	10457	2.37%	0.277%
17	10.159	2826	2836	2852	rBV	78194	124917	28.28%	3.315%
18	10.333	2879	2890	2901	rVB	18159	29074	6.58%	0.771%
19	11.194	3146	3158	3175	rBV	216183	346169	78.36%	9.186%
20	11.567	3263	3274	3291	rBV	203159	324856	73.53%	8.620%
21	12.201	3464	3471	3484	rVB2	6224	9937	2.25%	0.264%
22	12.297	3492	3501	3510	rBV10	9916	16119	3.65%	0.428%
23	12.625	3596	3603	3609	rVB5	3266	4449	1.01%	0.118%




Sum of corrected areas: 3768510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030460.D
Acq On : 10 Apr 2023 11:51
Operator : SY/MD
Sample : 02250-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

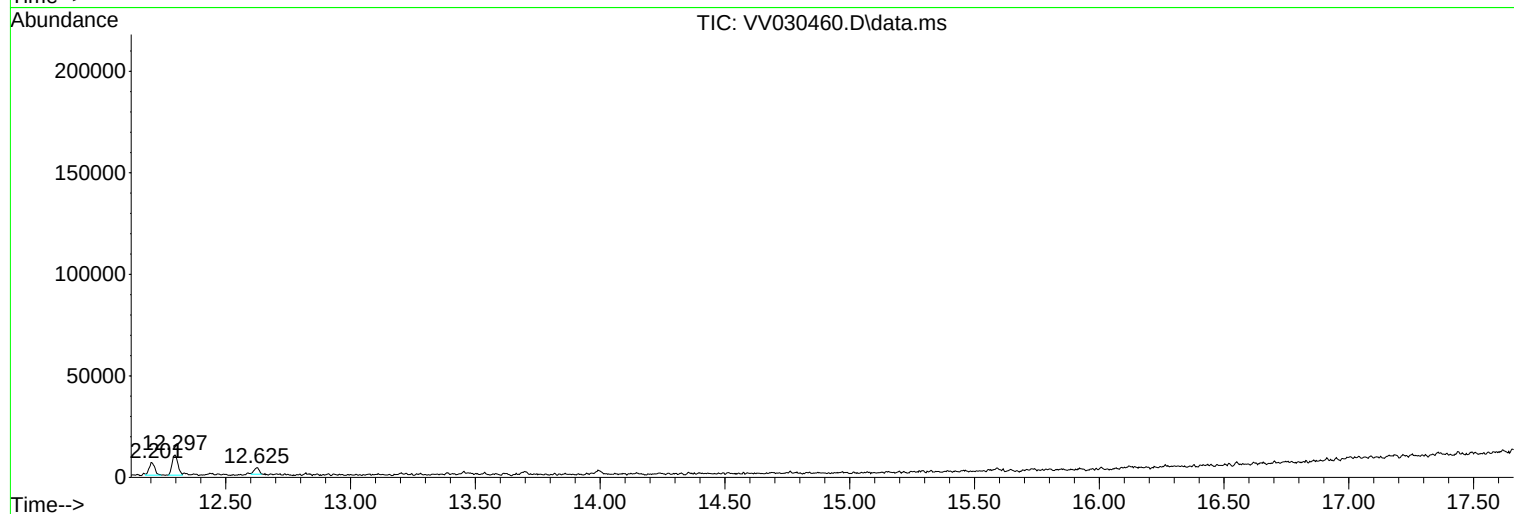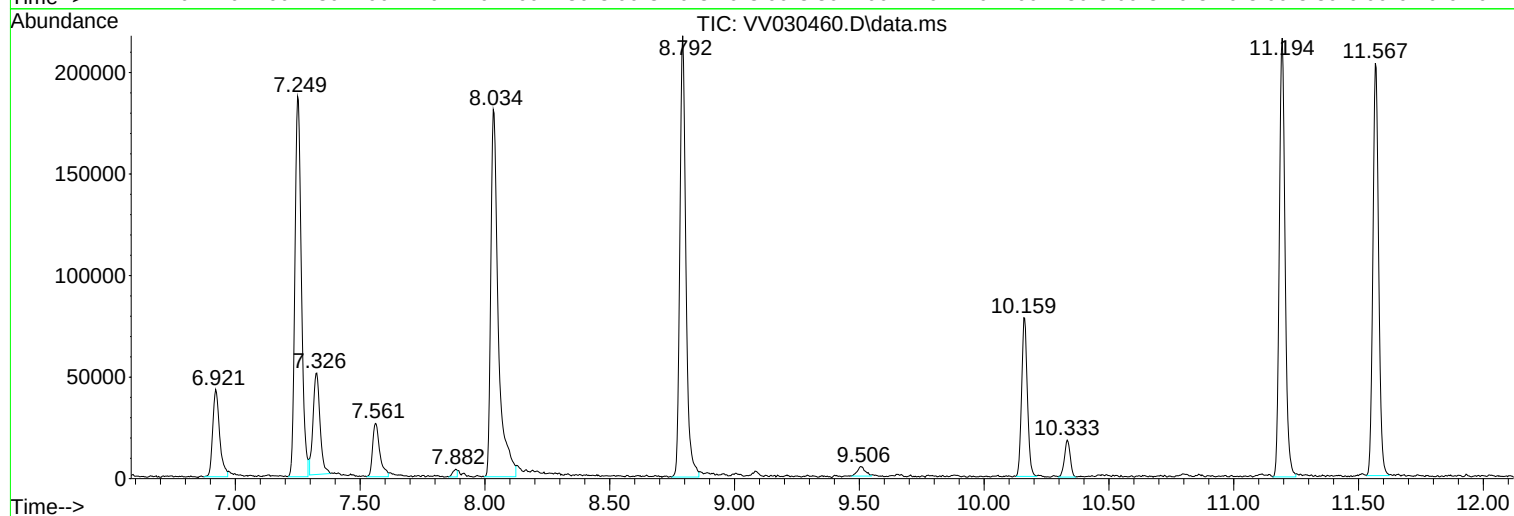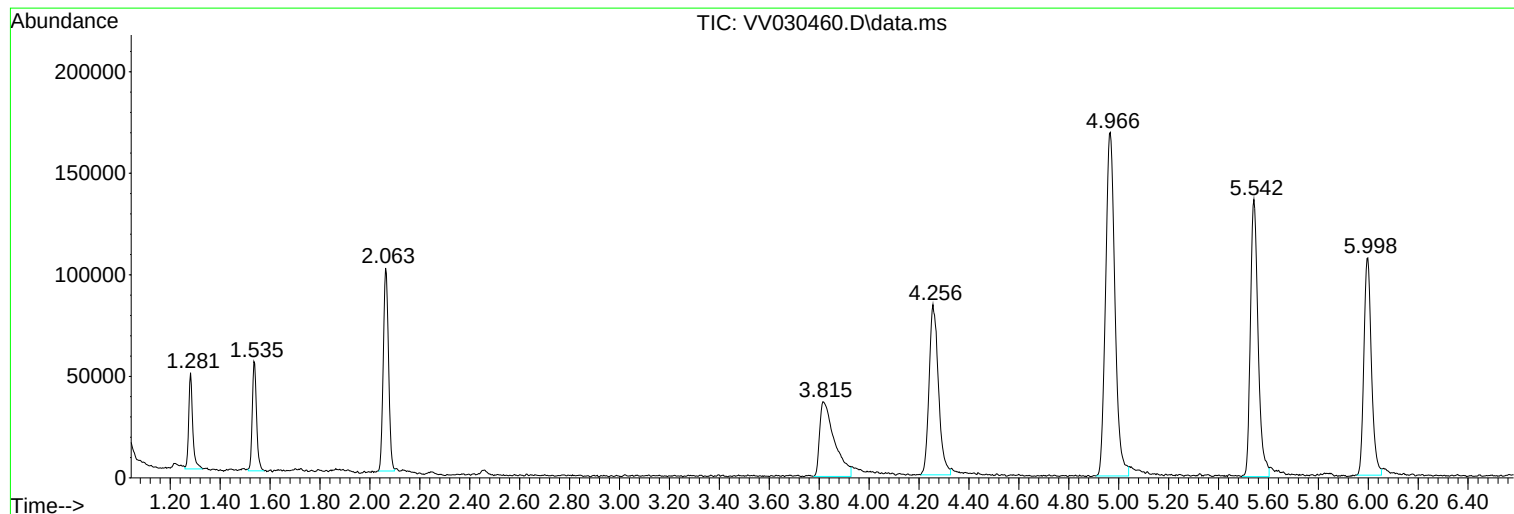

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030460.D
Acq On : 10 Apr 2023 11:51
Operator : SY/MD
Sample : 02250-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030460.D
Acq On : 10 Apr 2023 11:51
Operator : SY/MD
Sample : 02250-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc