

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
 Data File : VV030465.D
 Acq On : 10 Apr 2023 13:51
 Operator : SY/MD
 Sample : 02254-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	61	rBV	5374	6161	1.31%	0.155%
2	1.282	67	75	87	rVB	47125	52216	11.09%	1.316%
3	1.536	146	154	168	rBV	56809	69202	14.70%	1.744%
4	2.066	308	319	331	rBV	109701	160190	34.03%	4.036%
5	2.458	432	441	449	rVB6	3475	6248	1.33%	0.157%
6	3.812	851	862	890	rBV	47140	157186	33.39%	3.960%
7	4.262	986	1002	1023	rBV	85530	226995	48.22%	5.719%
8	4.966	1204	1221	1246	rBV3	177781	470770	100.00%	11.861%
9	5.545	1387	1401	1420	rBV	147803	314997	66.91%	7.936%
10	5.998	1528	1542	1563	rBV	110890	236357	50.21%	5.955%
11	6.921	1819	1829	1847	rBV	43985	87131	18.51%	2.195%
12	7.252	1917	1932	1947	rBV	203916	364485	77.42%	9.183%
13	7.326	1950	1955	1967	rVB2	12062	22312	4.74%	0.562%
14	7.564	2018	2029	2049	rBV2	27443	55604	11.81%	1.401%
15	7.886	2121	2129	2141	rVB3	8880	13819	2.94%	0.348%
16	8.034	2164	2175	2205	rBV	197358	398791	84.71%	10.047%
17	8.793	2400	2411	2431	rBV	223911	384719	81.72%	9.693%
18	9.085	2493	2502	2513	rVB5	6171	10258	2.18%	0.258%
19	10.162	2827	2837	2856	rVB	83189	134421	28.55%	3.387%
20	10.333	2880	2890	2903	rVB2	27511	45209	9.60%	1.139%
21	11.101	3123	3129	3141	rBV10	3532	7164	1.52%	0.180%
22	11.194	3146	3158	3175	rBV	231196	364550	77.44%	9.185%
23	11.510	3245	3256	3259	rBV7	3831	5523	1.17%	0.139%
24	11.571	3264	3275	3290	rVB	211773	338696	71.95%	8.533%
25	12.204	3459	3472	3483	rBV3	7502	13074	2.78%	0.329%
26	12.294	3490	3500	3511	rBV5	14264	23011	4.89%	0.580%




Sum of corrected areas: 3969089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030465.D
Acq On : 10 Apr 2023 13:51
Operator : SY/MD
Sample : 02254-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

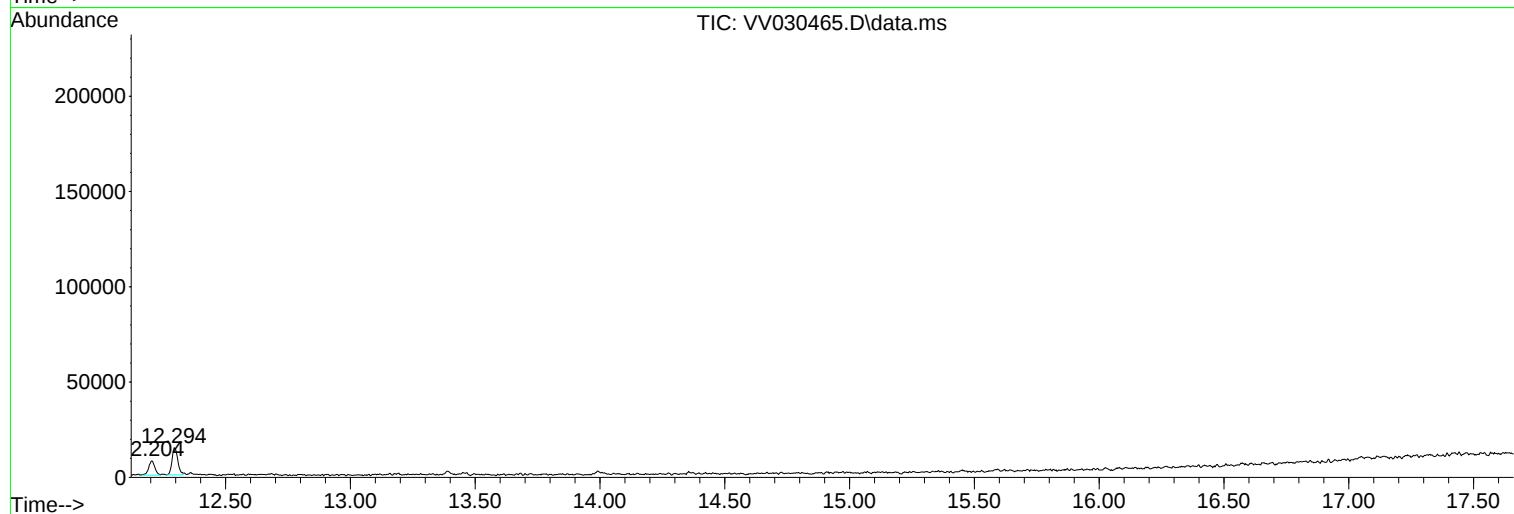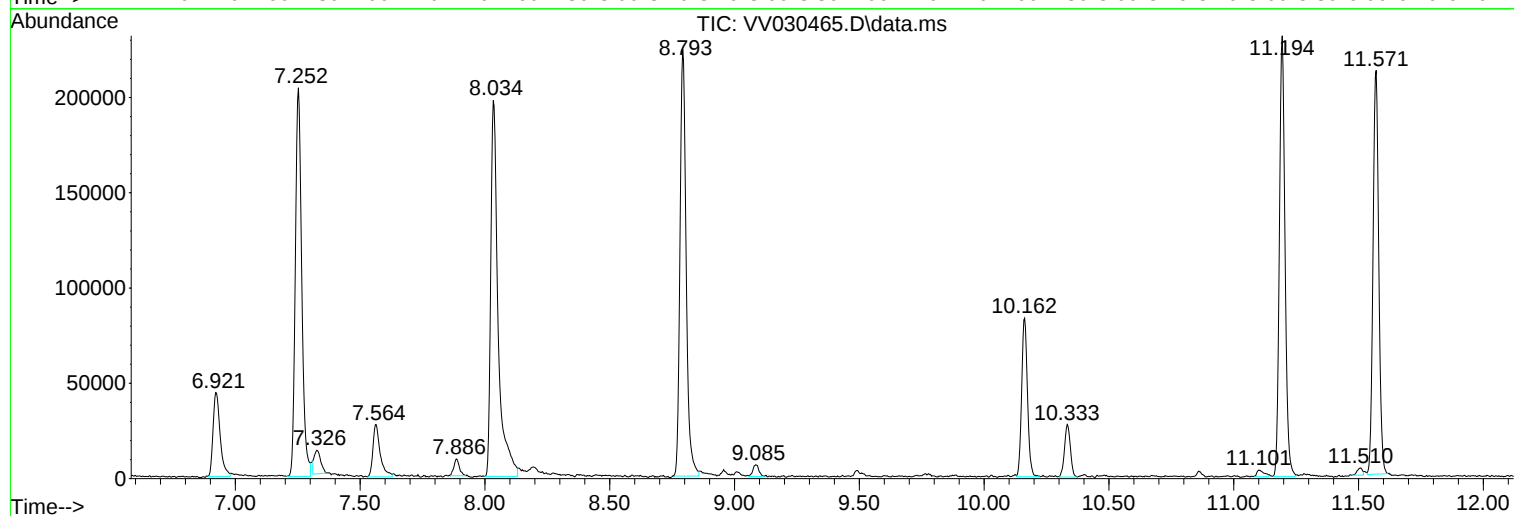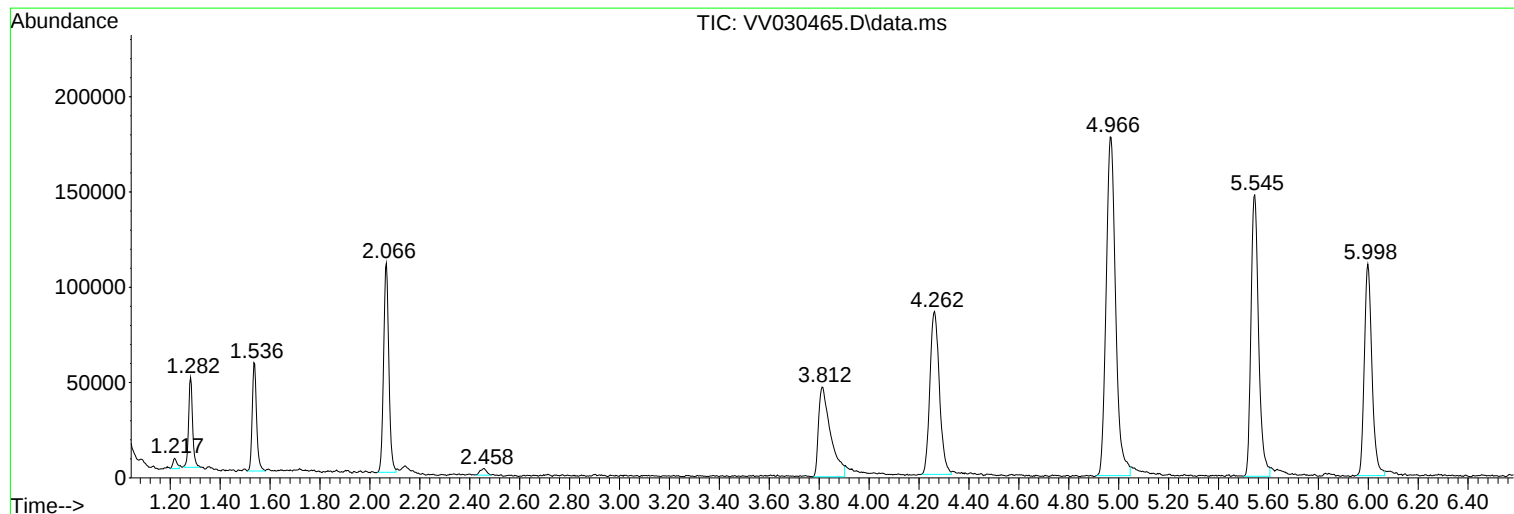

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030465.D
Acq On : 10 Apr 2023 13:51
Operator : SY/MD
Sample : 02254-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030465.D
Acq On : 10 Apr 2023 13:51
Operator : SY/MD
Sample : 02254-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------