

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
 Data File : VV030468.D
 Acq On : 10 Apr 2023 15:05
 Operator : SY/MD
 Sample : 02225-14DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	63	rBV4	3120	5148	1.18%	0.133%
2	1.282	68	75	87	rVB	43042	48356	11.09%	1.249%
3	1.536	147	154	172	rVB	51239	64911	14.88%	1.676%
4	2.063	305	318	334	rBV	102893	153282	35.15%	3.958%
5	2.455	427	440	457	rVB	25598	45729	10.49%	1.181%
6	3.117	630	646	665	rBV	134989	290842	66.69%	7.510%
7	3.828	854	867	902	rBV2	34808	153128	35.11%	3.954%
8	4.259	985	1001	1024	rBV	79508	207851	47.66%	5.367%
9	4.966	1205	1221	1244	rBV5	167965	436109	100.00%	11.261%
10	5.542	1388	1400	1424	rBV	128491	274697	62.99%	7.093%
11	5.998	1529	1542	1560	rBV2	103561	220483	50.56%	5.693%
12	6.921	1819	1829	1854	rBV	41401	82274	18.87%	2.124%
13	7.252	1920	1932	1962	rBV	184051	339565	77.86%	8.768%
14	7.561	2018	2028	2039	rBV2	26160	47201	10.82%	1.219%
15	7.886	2116	2129	2137	rBV5	2820	5454	1.25%	0.141%
16	8.037	2165	2176	2214	rBV	179590	391434	89.76%	10.107%
17	8.792	2399	2411	2434	rBV	196064	340588	78.10%	8.794%
18	10.162	2823	2837	2851	rBV2	79006	128937	29.57%	3.329%
19	10.333	2882	2890	2900	rVB4	5911	9696	2.22%	0.250%
20	11.194	3143	3158	3179	rBV	196619	315582	72.36%	8.148%
21	11.571	3264	3275	3294	rBV	192246	306578	70.30%	7.916%
22	13.988	4019	4027	4035	rBV5	3272	5042	1.16%	0.130%




Sum of corrected areas: 3872887

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030468.D
Acq On : 10 Apr 2023 15:05
Operator : SY/MD
Sample : 02225-14DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

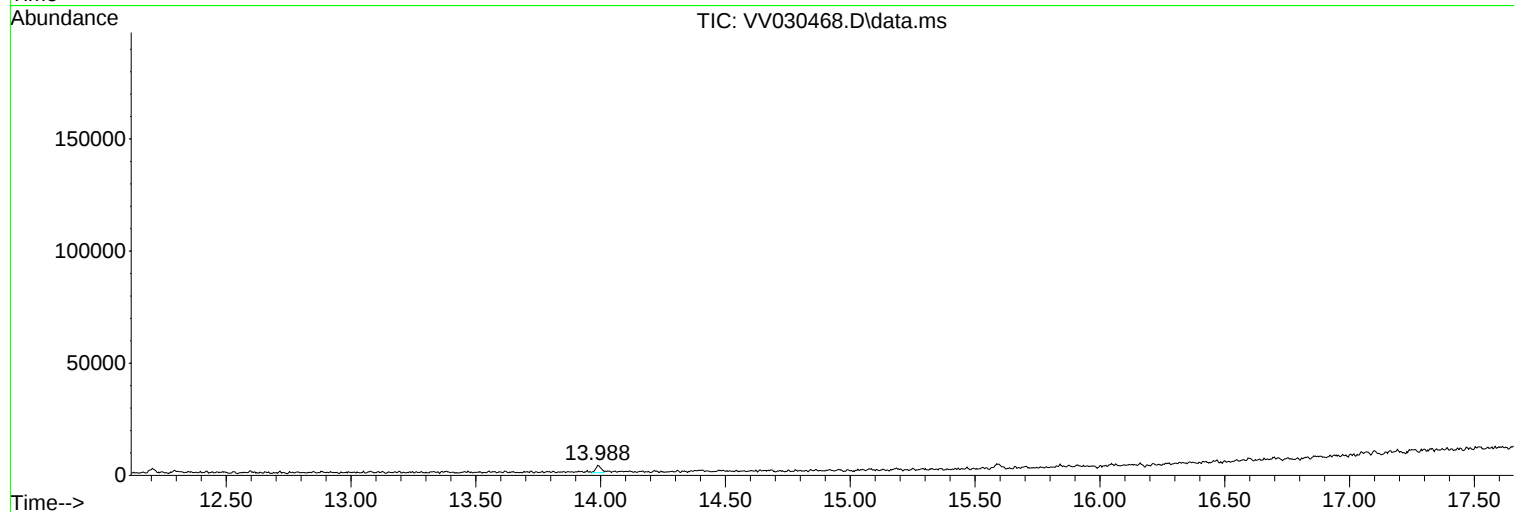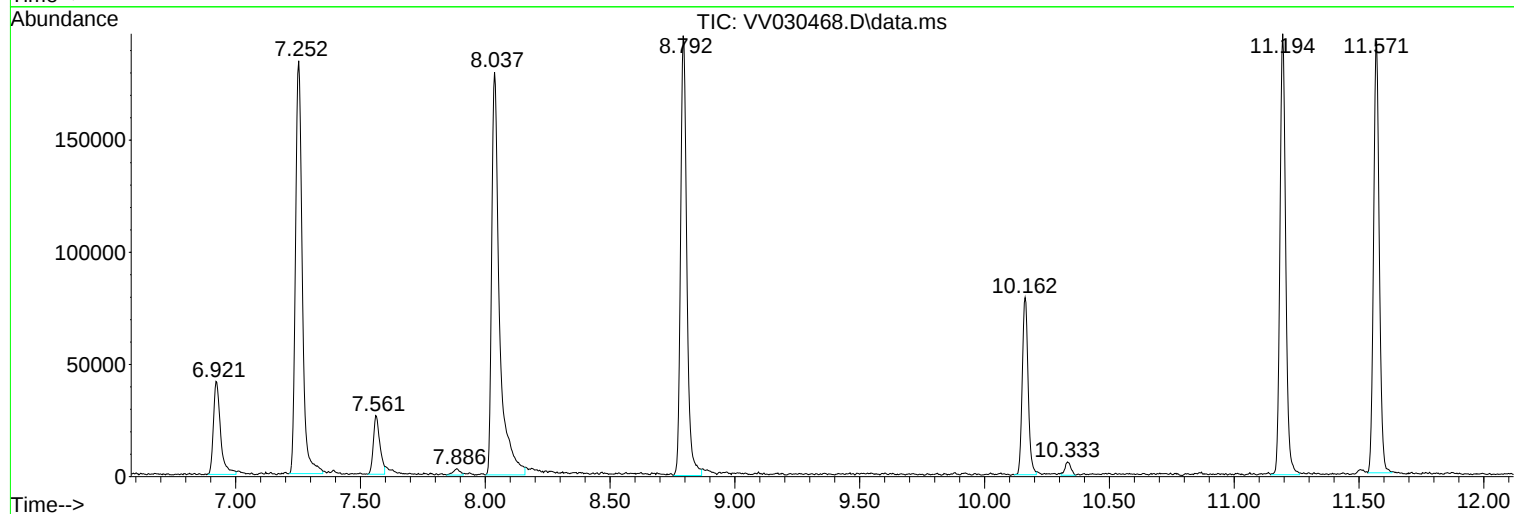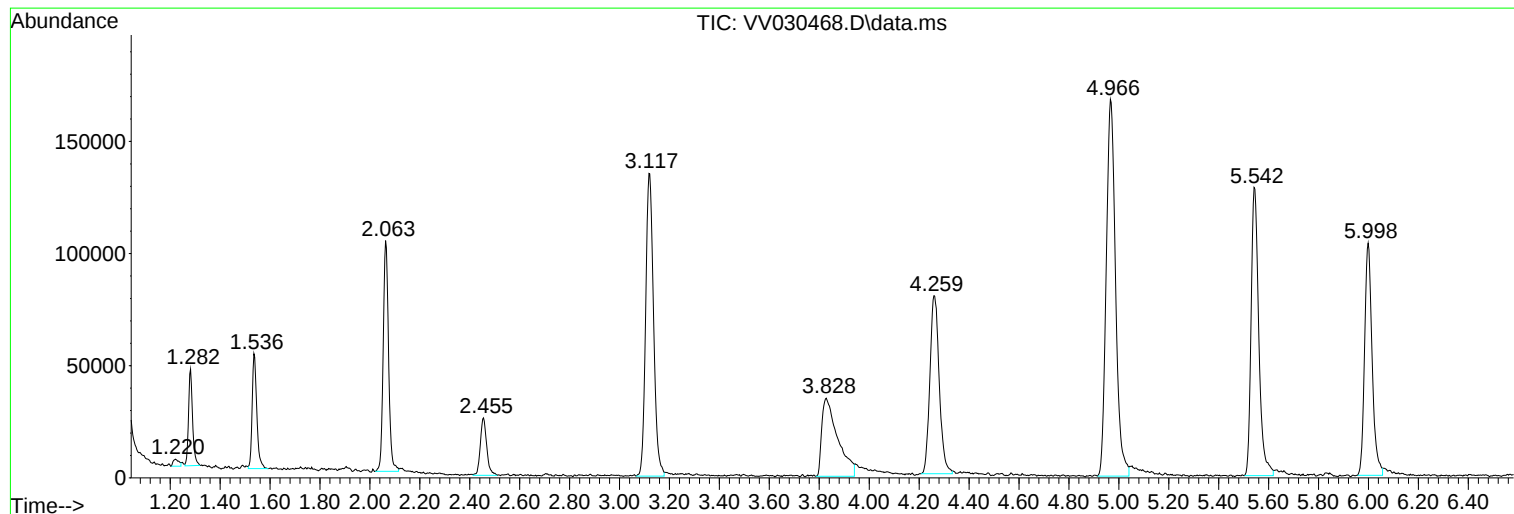

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030468.D
Acq On : 10 Apr 2023 15:05
Operator : SY/MD
Sample : 02225-14DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030468.D
Acq On : 10 Apr 2023 15:05
Operator : SY/MD
Sample : 02225-14DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc