

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
 Data File : VV030470.D
 Acq On : 10 Apr 2023 15:53
 Operator : SY/MD
 Sample : 02225-16DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rVB	43129	48212	7.13%	1.061%
2	1.536	147	154	167	rVB	48878	58653	8.68%	1.291%
3	2.069	305	320	344	rVB4	250786	429581	63.54%	9.457%
4	2.452	429	439	450	rBV	28251	47747	7.06%	1.051%
5	3.121	633	647	661	rBV2	17013	37788	5.59%	0.832%
6	3.831	852	868	898	rBV	30820	136694	20.22%	3.009%
7	4.259	981	1001	1025	rBV2	82561	206932	30.61%	4.556%
8	4.523	1058	1083	1105	rBV	263585	676034	100.00%	14.883%
9	4.969	1201	1222	1249	rBV2	163970	430179	63.63%	9.470%
10	5.542	1388	1400	1422	rBV	137872	293946	43.48%	6.471%
11	5.998	1526	1542	1560	rBV	100094	215520	31.88%	4.745%
12	6.921	1816	1829	1849	rBV	40332	82660	12.23%	1.820%
13	7.252	1920	1932	1948	rBV	178941	321428	47.55%	7.076%
14	7.561	2019	2028	2050	rBV2	24667	50068	7.41%	1.102%
15	8.037	2165	2176	2209	rBV	169543	370664	54.83%	8.160%
16	8.792	2399	2411	2434	rBV	211060	360063	53.26%	7.927%
17	10.162	2826	2837	2853	rBV	75902	122293	18.09%	2.692%
18	10.333	2882	2890	2901	rVB3	7456	11751	1.74%	0.259%
19	11.194	3145	3158	3174	rBV	214874	338738	50.11%	7.457%
20	11.570	3264	3275	3293	rBV	189683	303381	44.88%	6.679%




Sum of corrected areas: 4542332

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030470.D
Acq On : 10 Apr 2023 15:53
Operator : SY/MD
Sample : 02225-16DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

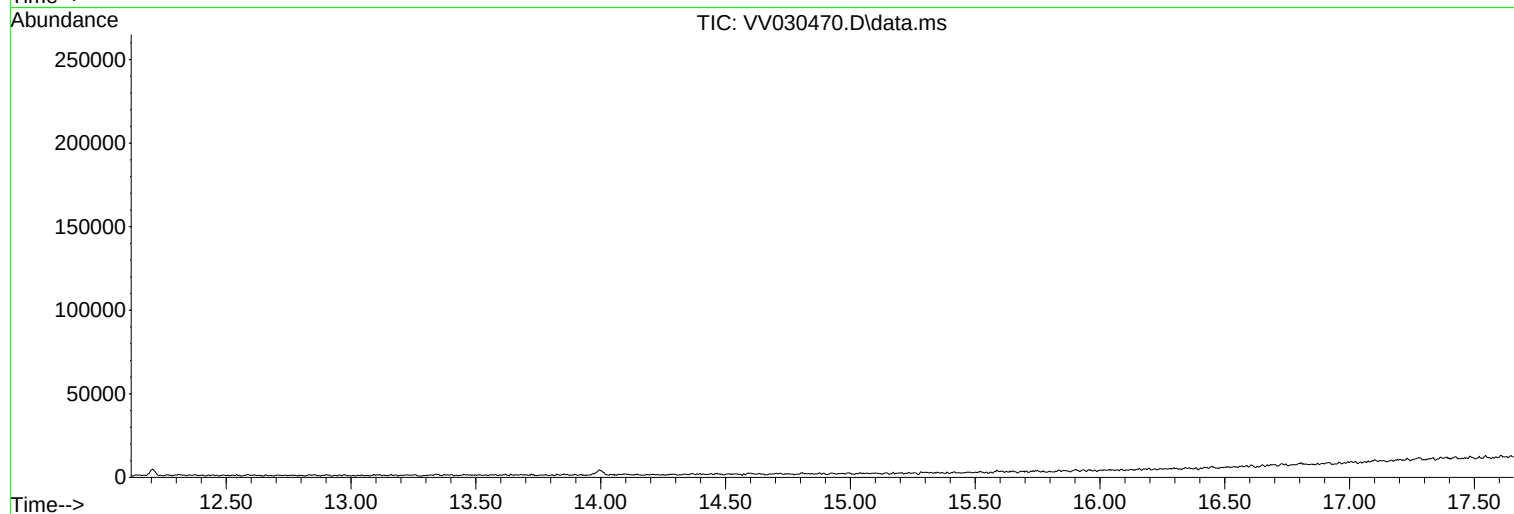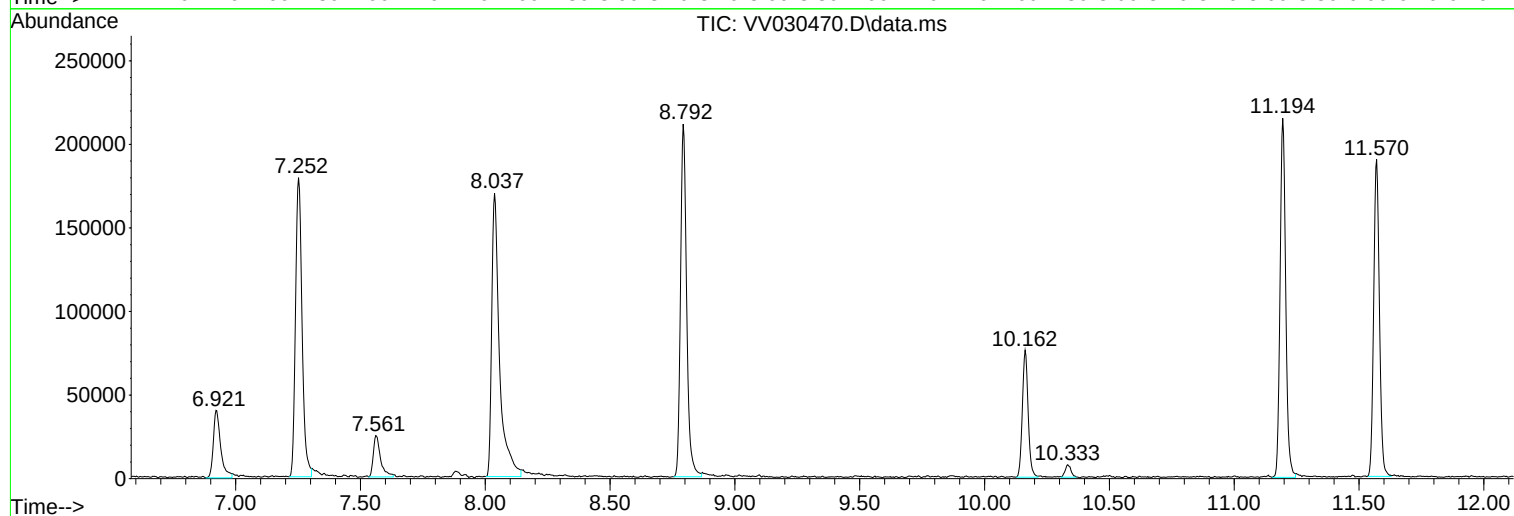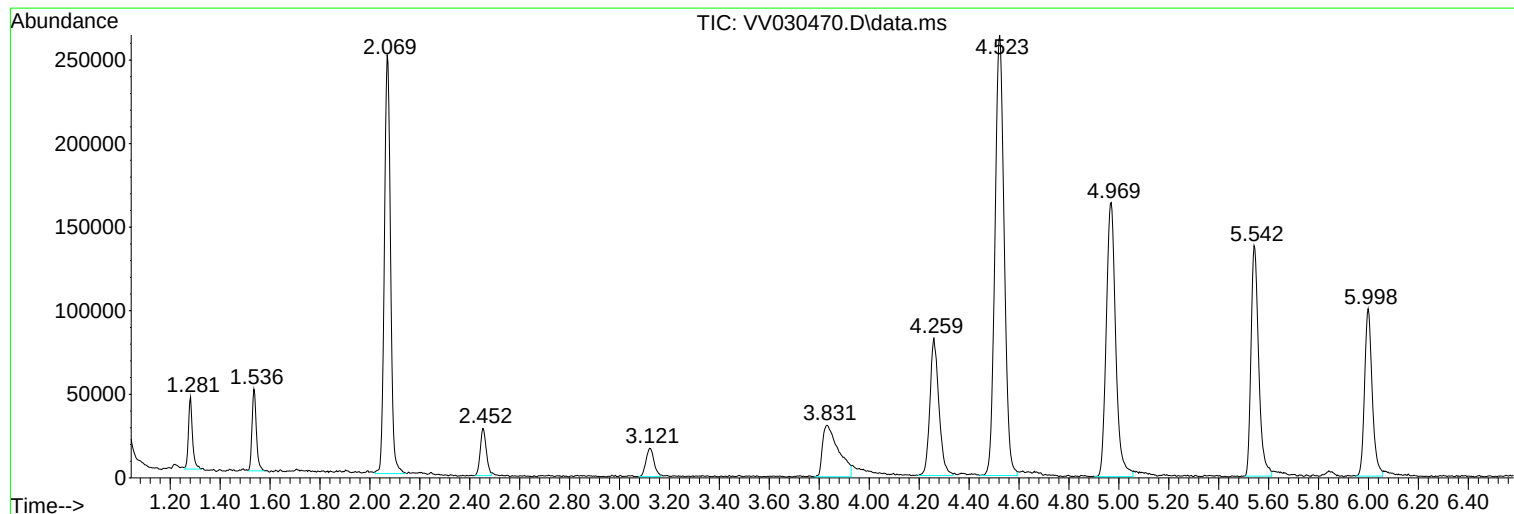

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030470.D
Acq On : 10 Apr 2023 15:53
Operator : SY/MD
Sample : 02225-16DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030470.D
Acq On : 10 Apr 2023 15:53
Operator : SY/MD
Sample : 02225-16DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------