

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
 Data File : VV030472.D
 Acq On : 10 Apr 2023 16:59
 Operator : SY/MD
 Sample : 02194-15DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.221	49	56	63	rBV5	3449	5924	1.07%	0.116%
2	1.282	68	75	85	rVB	39434	44742	8.12%	0.875%
3	1.536	146	154	173	rVB	50308	61482	11.15%	1.203%
4	2.063	308	318	332	rBV2	102826	156130	28.32%	3.055%
5	2.455	429	440	457	rBV	84445	143084	25.96%	2.800%
6	2.712	511	520	528	rBV5	5268	9155	1.66%	0.179%
7	3.127	636	649	656	rBV9	2792	5877	1.07%	0.115%
8	3.828	849	867	900	rBV2	130392	398169	72.23%	7.791%
9	4.262	983	1002	1025	rBV2	81604	206440	37.45%	4.040%
10	4.532	1072	1086	1097	rVB10	3474	8182	1.48%	0.160%
11	4.970	1206	1222	1249	rBV2	168703	434573	78.84%	8.504%
12	5.545	1386	1401	1425	rBV	174840	372477	67.57%	7.288%
13	5.844	1481	1494	1516	rBV2	137963	289394	52.50%	5.663%
14	5.998	1530	1542	1570	rBV2	100279	216088	39.20%	4.228%
15	6.924	1819	1830	1848	rBV	41560	82670	15.00%	1.618%
16	7.252	1920	1932	1952	rBV	181656	329598	59.79%	6.449%
17	7.564	2017	2029	2041	rBV	25837	48597	8.82%	0.951%
18	7.915	2122	2138	2162	rBV	317387	551237	100.00%	10.786%
19	8.040	2166	2177	2216	rBV	176692	393340	71.36%	7.697%
20	8.793	2399	2411	2437	rBV	261081	449072	81.47%	8.787%
21	10.162	2826	2837	2851	rBV	76386	126047	22.87%	2.466%
22	10.336	2882	2891	2897	rBV4	3974	6001	1.09%	0.117%
23	11.194	3146	3158	3181	rVV	259709	422136	76.58%	8.260%
24	11.571	3261	3275	3290	rBV	186562	314166	56.99%	6.147%
25	13.207	3774	3784	3793	rBV4	7256	11506	2.09%	0.225%
26	13.448	3850	3859	3872	rVB2	7271	12252	2.22%	0.240%
27	13.689	3925	3934	3944	rVB4	8366	12142	2.20%	0.238%




Sum of corrected areas: 5110481

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030472.D
Acq On : 10 Apr 2023 16:59
Operator : SY/MD
Sample : 02194-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

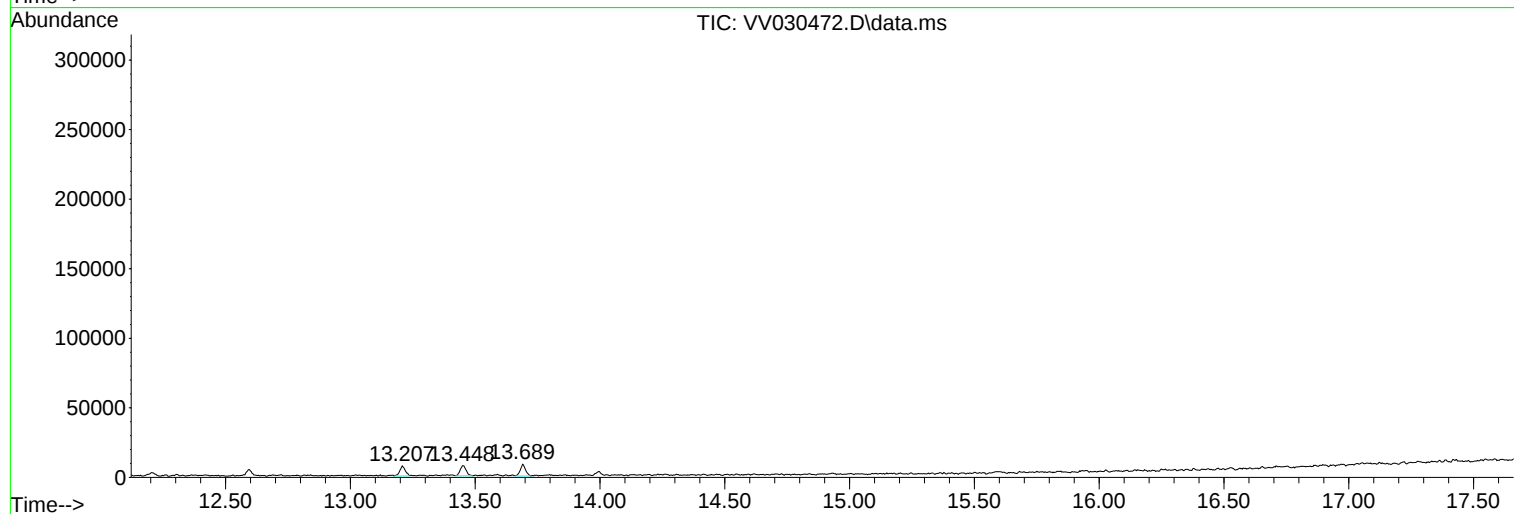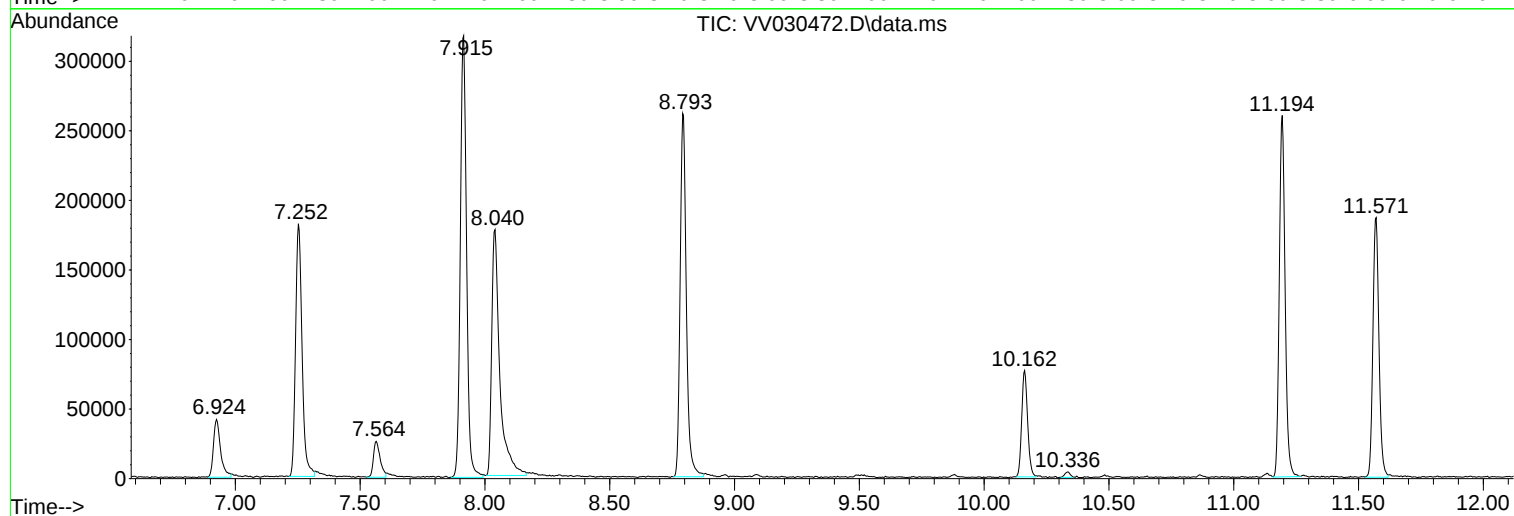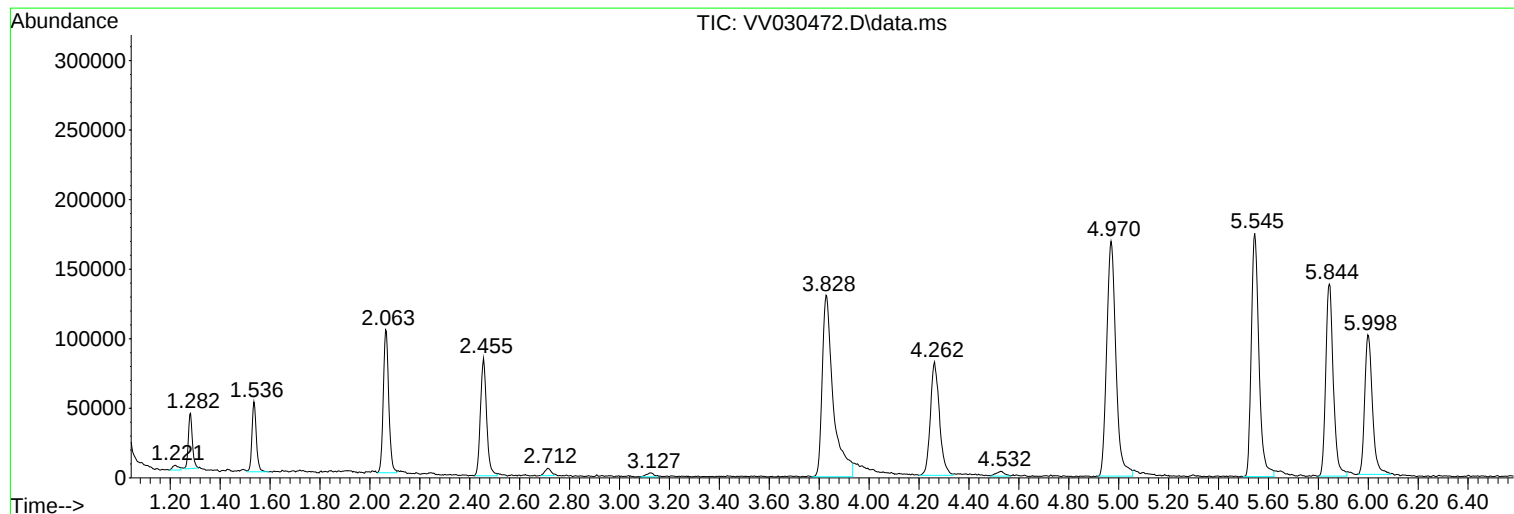

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030472.D
Acq On : 10 Apr 2023 16:59
Operator : SY/MD
Sample : 02194-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030472.D
Acq On : 10 Apr 2023 16:59
Operator : SY/MD
Sample : 02194-15DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------