

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
 Data File : VV030473.D
 Acq On : 10 Apr 2023 17:24
 Operator : SY/MD
 Sample : 02225-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	88	rVB	39913	45387	10.77%	1.279%
2	1.539	147	155	164	rVB	48107	56386	13.38%	1.588%
3	2.063	307	318	334	rBV	93667	137519	32.64%	3.874%
4	3.821	854	865	894	rBV	37808	145800	34.61%	4.107%
5	4.262	984	1002	1025	rBV2	80790	202214	48.00%	5.696%
6	4.526	1071	1084	1094	rBV4	7440	17820	4.23%	0.502%
7	4.966	1202	1221	1249	rBV2	158399	421294	100.00%	11.868%
8	5.545	1387	1401	1424	rBV	138110	293076	69.57%	8.256%
9	5.998	1528	1542	1564	rBV	100105	214512	50.92%	6.043%
10	6.921	1819	1829	1844	rBV	39513	79192	18.80%	2.231%
11	7.252	1920	1932	1953	rBV	174711	322449	76.54%	9.083%
12	7.564	2020	2029	2051	rBV2	24659	47613	11.30%	1.341%
13	7.886	2118	2129	2134	rBV2	5258	8208	1.95%	0.231%
14	8.037	2165	2176	2208	rBV	174842	367278	87.18%	10.346%
15	8.792	2400	2411	2432	rBV	212571	362878	86.13%	10.222%
16	10.162	2826	2837	2852	rBV	74490	121491	28.84%	3.422%
17	10.332	2880	2890	2900	rVB	20224	34100	8.09%	0.961%
18	11.194	3145	3158	3176	rBV	214649	343980	81.65%	9.690%
19	11.506	3247	3255	3263	rBV8	4745	9094	2.16%	0.256%
20	11.570	3263	3275	3293	rVB	192293	307727	73.04%	8.668%
21	12.204	3462	3472	3485	rVB2	6295	11934	2.83%	0.336%




Sum of corrected areas: 3549952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030473.D
Acq On : 10 Apr 2023 17:24
Operator : SY/MD
Sample : 02225-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

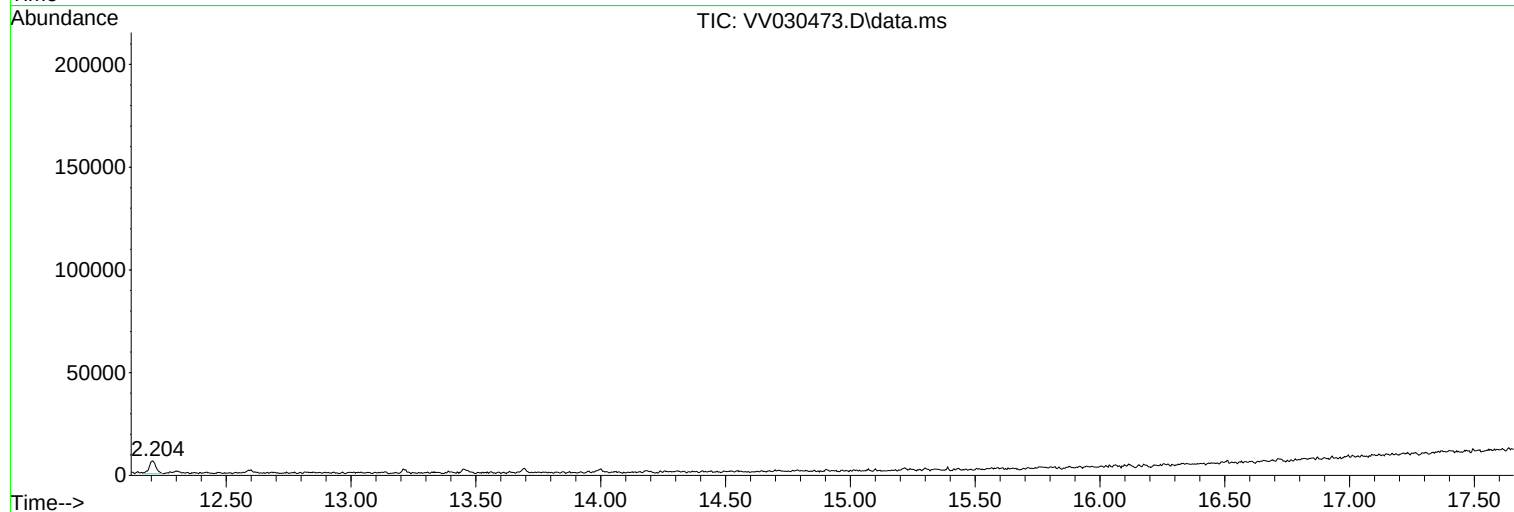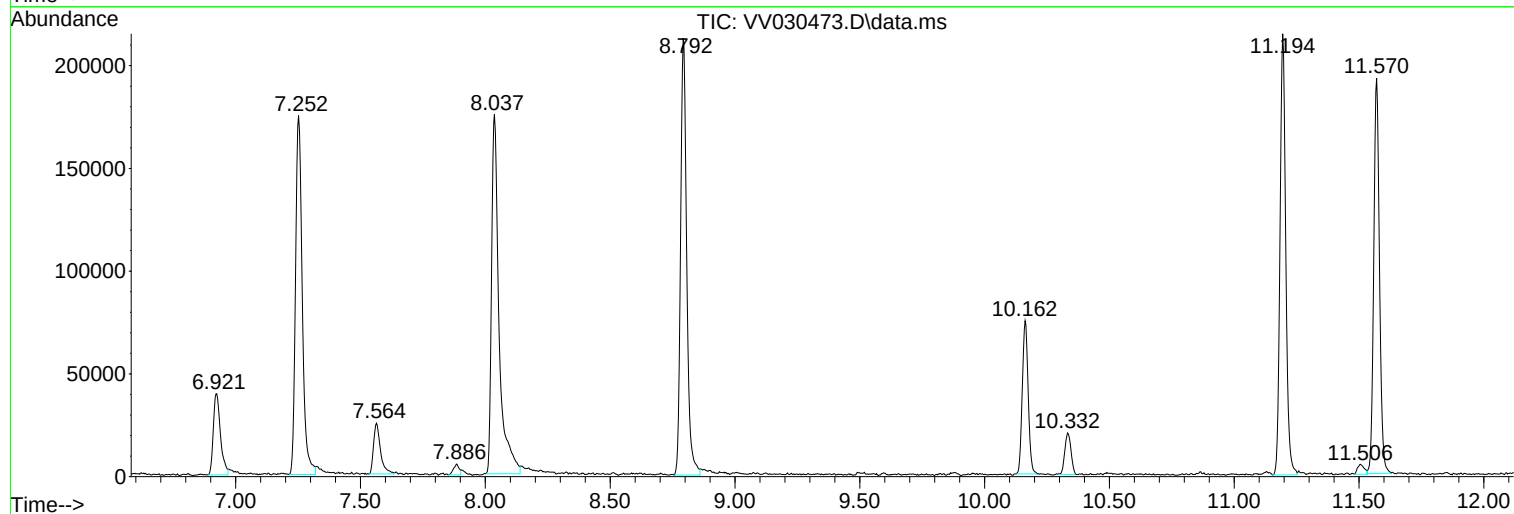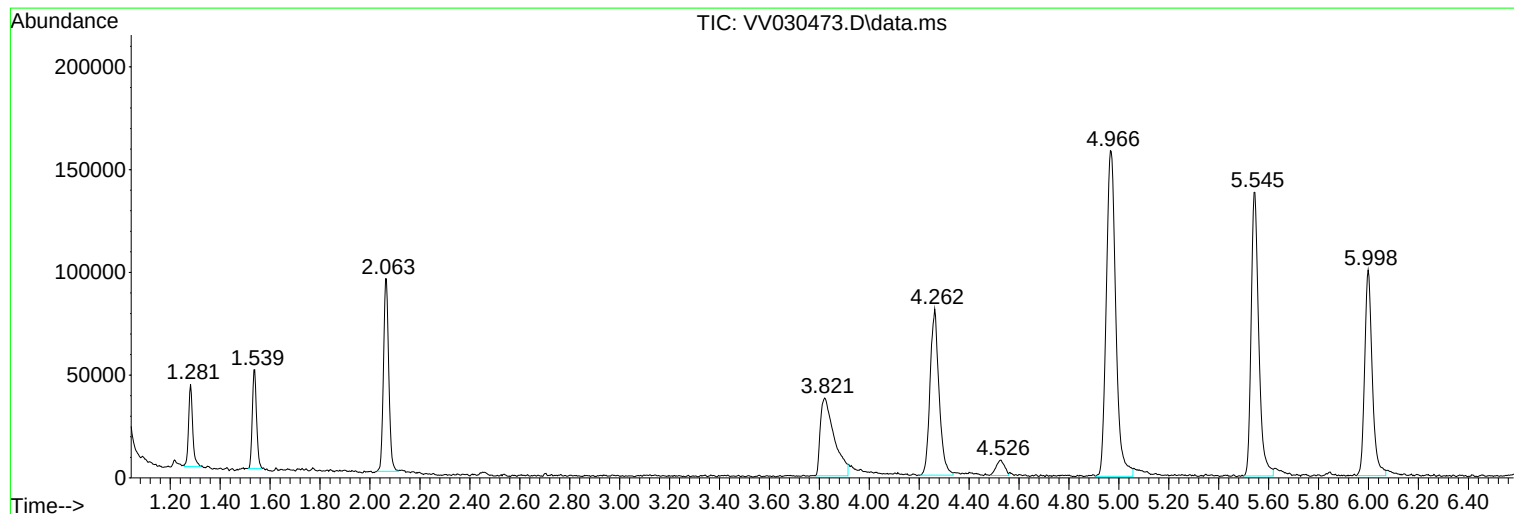

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030473.D
Acq On : 10 Apr 2023 17:24
Operator : SY/MD
Sample : 02225-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030473.D
Acq On : 10 Apr 2023 17:24
Operator : SY/MD
Sample : 02225-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------