

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
 Data File : VV030475.D
 Acq On : 10 Apr 2023 18:13
 Operator : SY/MD
 Sample : 02254-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.076	309	322	359	rBV	9467521	13711429	30.35%	20.737%
2	3.118	628	646	681	rBV	3037575	6293841	13.93%	9.519%
3	4.529	1058	1085	1111	rBV	17874454	45181457	100.00%	68.333%
4	5.841	1479	1493	1515	rBV	230304	470228	1.04%	0.711%
5	11.477	3235	3246	3264	rBV	285253	462233	1.02%	0.699%




Sum of corrected areas: 66119188

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030475.D
Acq On : 10 Apr 2023 18:13
Operator : SY/MD
Sample : 02254-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

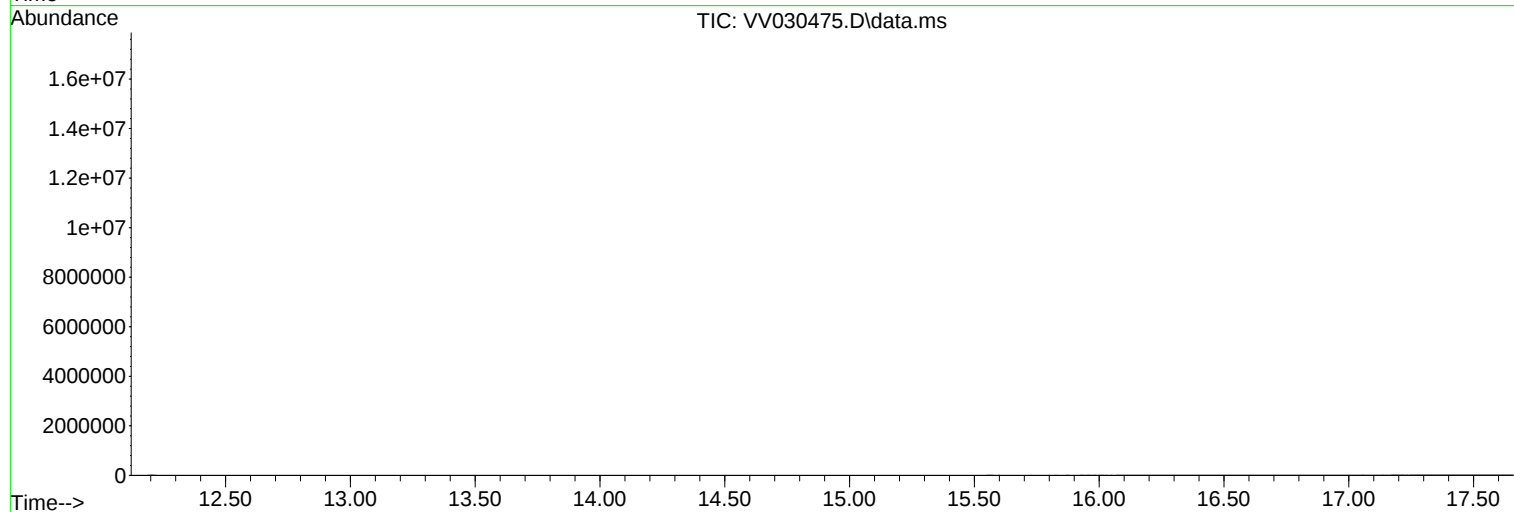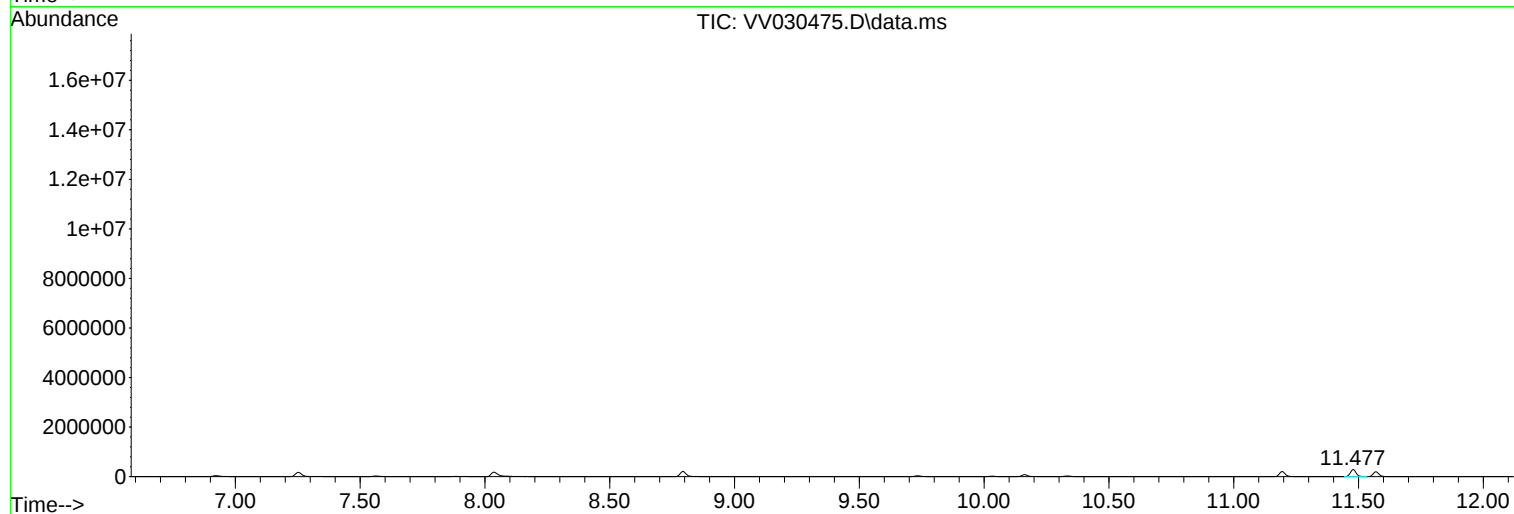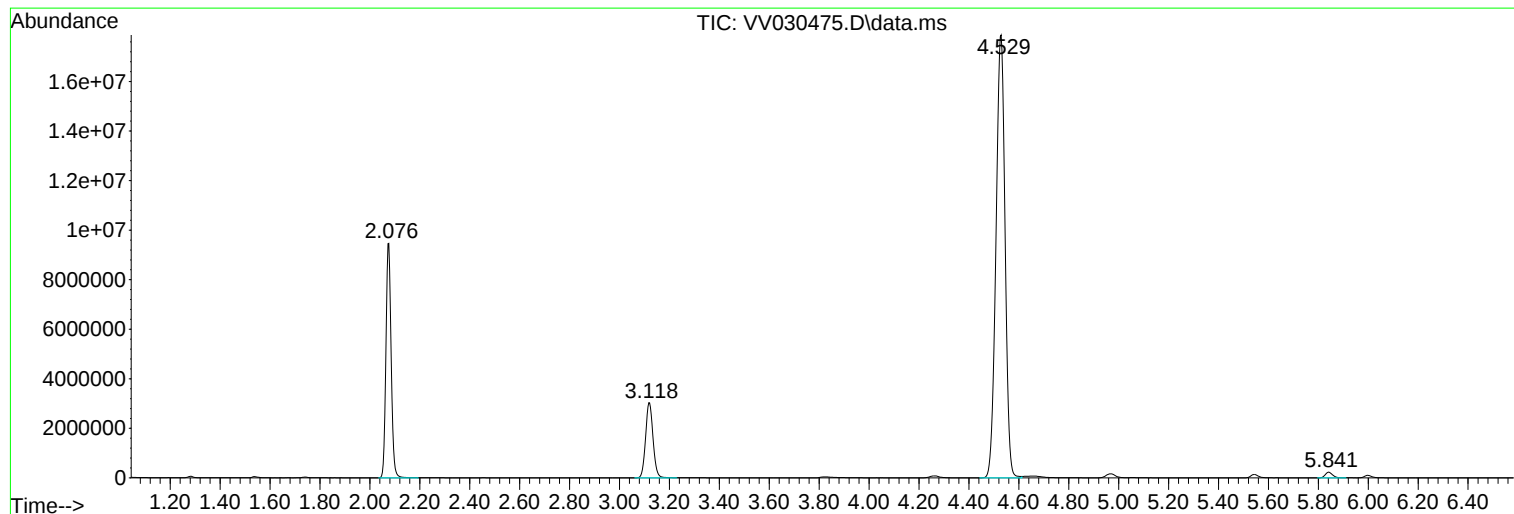

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030475.D
Acq On : 10 Apr 2023 18:13
Operator : SY/MD
Sample : 02254-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.477	5.00 ug/L	462233	1,4-Dichlorobenzene-d4	11.194

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopropane, 1,1-dichloro-2-chl...	172	C5H7Cl3	015997-19-0	35
2			Methyl 3,3-dichloropropenoate	154	C4H4Cl2O2	002257-46-7	27
3			2,2-Dichloroethyl ethyl carbonate	186	C5H8Cl2O3	1010373-78-3	16
4			1-Propene, 3,3,3-trichloro-2-met...	158	C4H5Cl3	004749-27-3	16
5			5-(4-Chlorobenzylidene)-3-(4-flu...	377	C17H9Cl1FN02S2	1000223-15-4	12

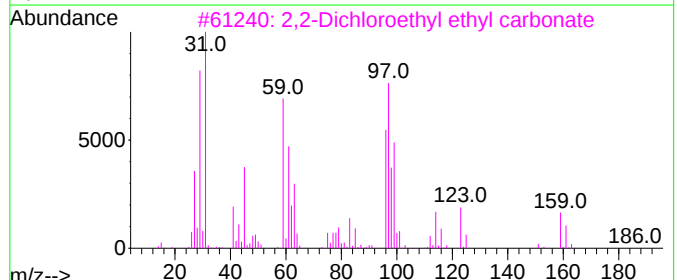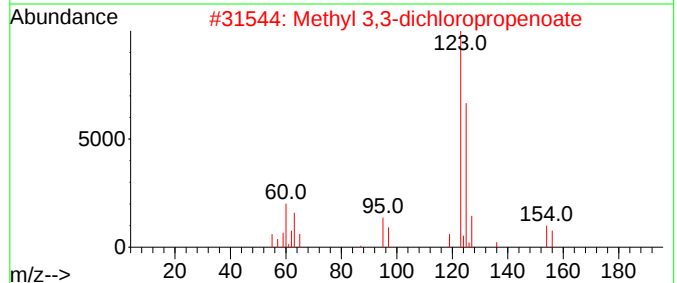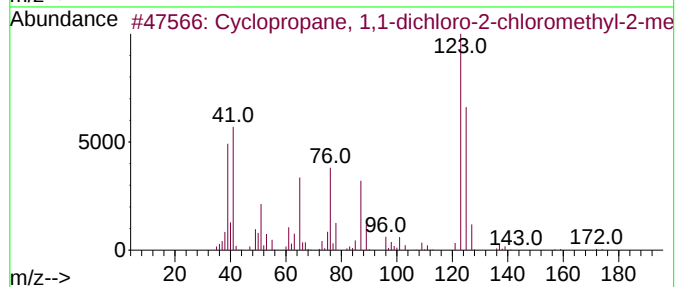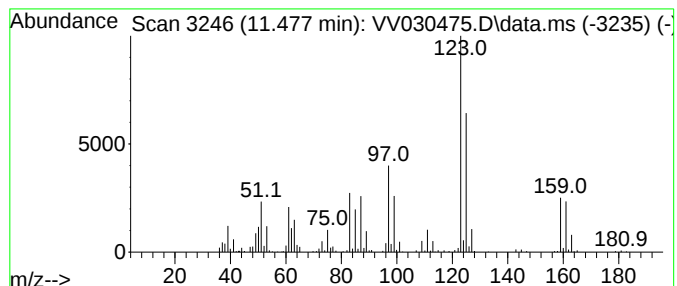

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030475.D
Acq On : 10 Apr 2023 18:13
Operator : SY/MD
Sample : 02254-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	11.477	5.0	ug/L	462233	3	11.194	462233	5.0