

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
 Data File : VV030477.D
 Acq On : 10 Apr 2023 19:02
 Operator : SY/MD
 Sample : 02254-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	90	rVB3	59044	74680	1.34%	0.435%
2	1.535	147	154	172	rVB	49155	67101	1.21%	0.391%
3	2.072	308	321	349	rBV	3150925	4649874	83.71%	27.112%
4	3.117	629	646	676	rBV	2668519	5554946	100.00%	32.389%
5	3.834	856	869	885	rBV2	31771	115109	2.07%	0.671%
6	4.259	984	1001	1028	rBV	75869	198902	3.58%	1.160%
7	4.522	1061	1083	1106	rBV	1300332	3307366	59.54%	19.284%
8	4.966	1202	1221	1243	rBV2	158215	414825	7.47%	2.419%
9	5.542	1385	1400	1424	rBV	137184	295810	5.33%	1.725%
10	5.841	1476	1493	1516	rBV2	132925	277618	5.00%	1.619%
11	5.998	1529	1542	1563	rBV	97730	206820	3.72%	1.206%
12	6.924	1817	1830	1849	rBV	39156	77496	1.40%	0.452%
13	7.252	1921	1932	1950	rBV	171292	311509	5.61%	1.816%
14	8.037	2164	2176	2210	rBV	169927	379800	6.84%	2.214%
15	8.792	2398	2411	2432	rBV	214850	362355	6.52%	2.113%
16	10.162	2827	2837	2850	rBV	76872	124963	2.25%	0.729%
17	11.194	3147	3158	3174	rBV	212499	335891	6.05%	1.958%
18	11.477	3237	3246	3263	rBV	54409	94450	1.70%	0.551%
19	11.570	3264	3275	3291	rVB	186446	301349	5.42%	1.757%




Sum of corrected areas: 17150864

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030477.D
Acq On : 10 Apr 2023 19:02
Operator : SY/MD
Sample : 02254-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

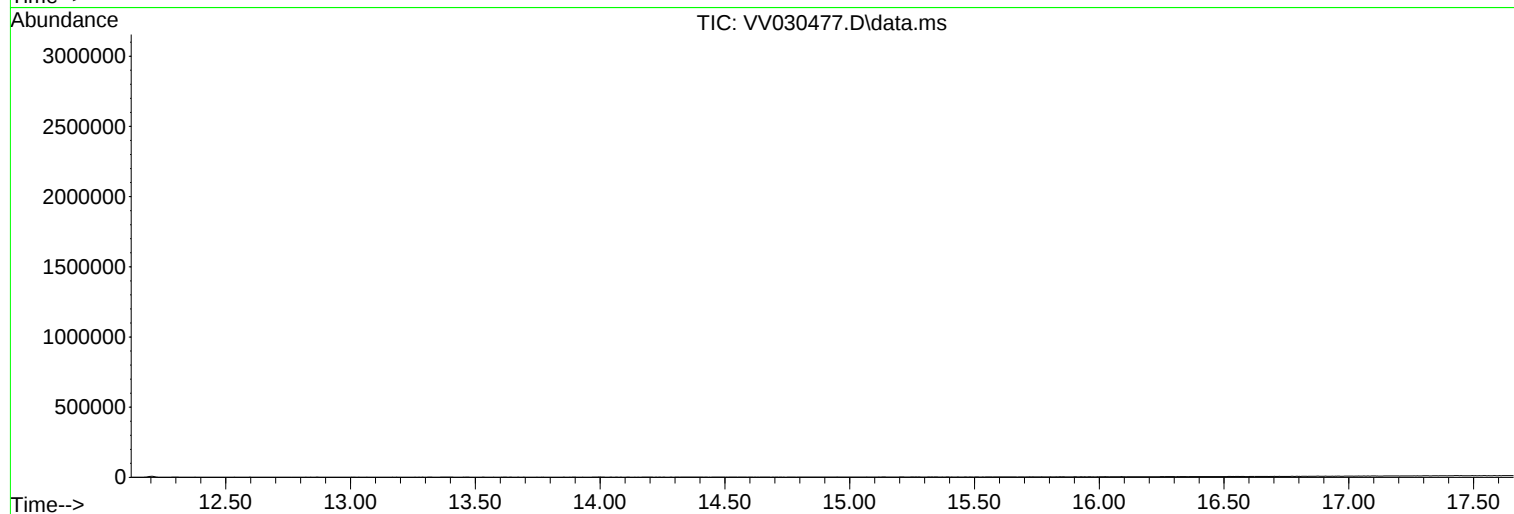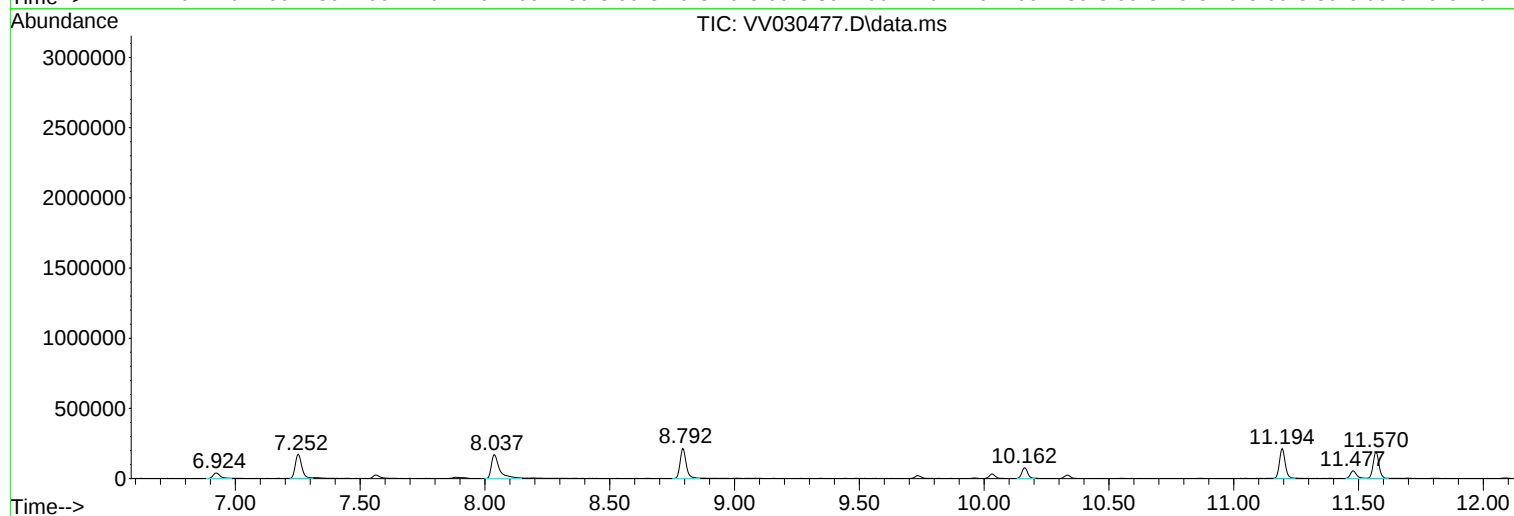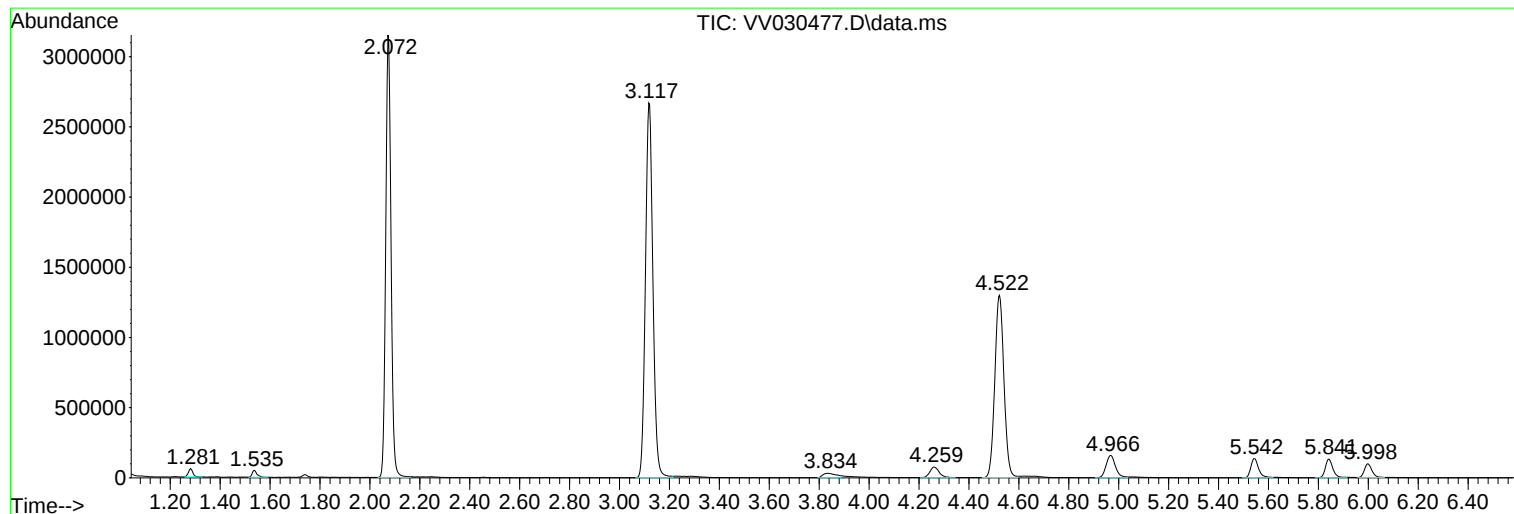

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030477.D
Acq On : 10 Apr 2023 19:02
Operator : SY/MD
Sample : 02254-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.477	1.41 ug/L	94450	1,4-Dichlorobenzene-d4	11.194

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopropane, 1,1-dichloro-2-chl...	172	C5H7Cl3	015997-19-0	35
2			2,2-Dichloroethyl ethyl carbonate	186	C5H8Cl2O3	1010373-78-3	25
3			4-Pyridinecarboxaldehyde N-oxide	123	C6H5NO2	007216-42-4	22
4			Phenol, 4-nitroso-	123	C6H5NO2	000104-91-6	16
5			1-Propene, 3,3,3-trichloro-2-met...	158	C4H5Cl3	004749-27-3	16

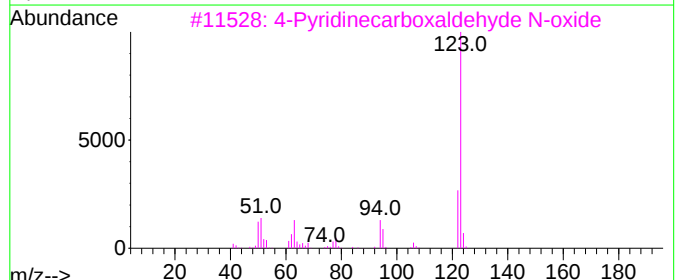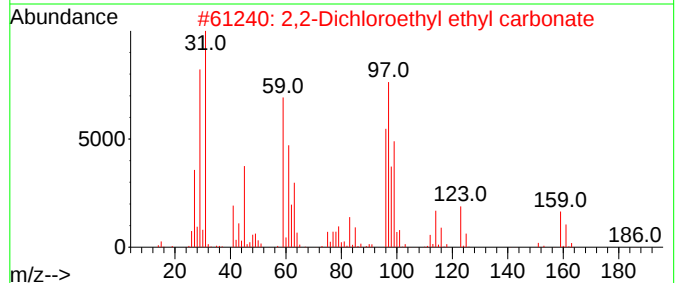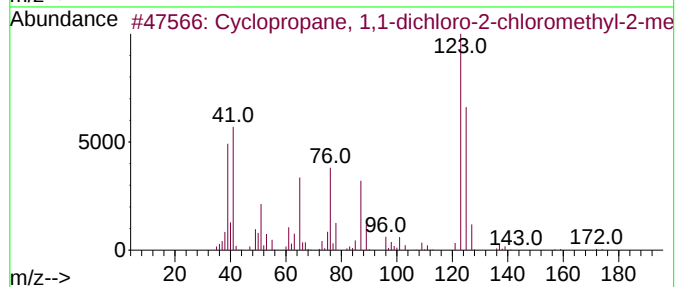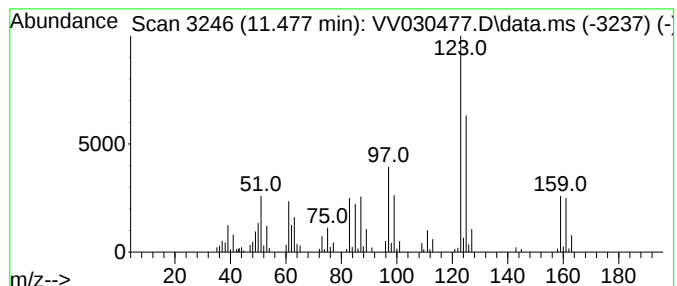

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030477.D
Acq On : 10 Apr 2023 19:02
Operator : SY/MD
Sample : 02254-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	11.477	1.4	ug/L	94450	3	11.194	335891	5.0