

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030482.D
Acq On : 10 Apr 2023 21:02
Operator : SY/MD
Sample : 02250-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.072	308	321	337	rBV3	199630	353628	1.44%	1.027%
2	3.825	850	866	896	rBV3	119075	351964	1.43%	1.023%
3	4.969	1205	1222	1247	rBV2	155037	409020	1.66%	1.188%
4	5.542	1386	1400	1422	rBV	134610	283352	1.15%	0.823%
5	5.841	1472	1493	1530	rBV	3517394	6786520	27.62%	19.719%
6	7.252	1918	1932	1951	rBV	176517	316527	1.29%	0.920%
7	7.918	2120	2139	2166	rBV	15161334	24569490	100.00%	71.388%
8	8.034	2167	2175	2208	rVB	200128	410547	1.67%	1.193%
9	8.792	2400	2411	2437	rBV	192843	337099	1.37%	0.979%
10	11.194	3146	3158	3173	rBV	196045	313448	1.28%	0.911%
11	11.570	3263	3275	3293	rBV	177641	285099	1.16%	0.828%




Sum of corrected areas: 34416694

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030482.D
Acq On : 10 Apr 2023 21:02
Operator : SY/MD
Sample : 02250-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

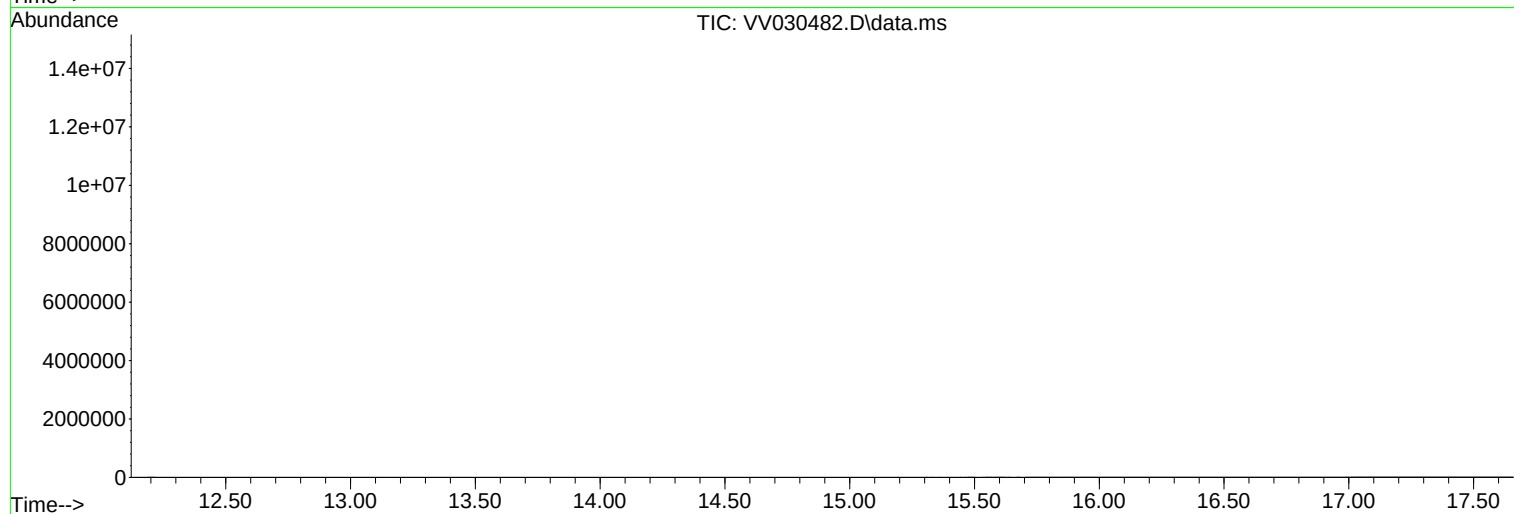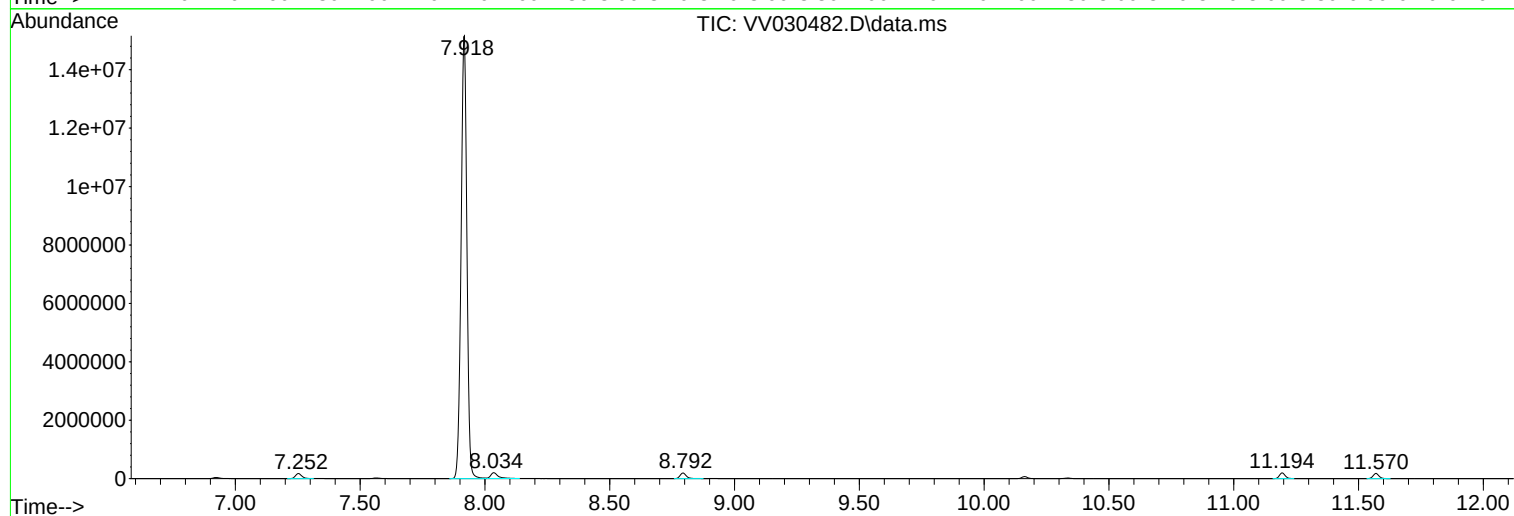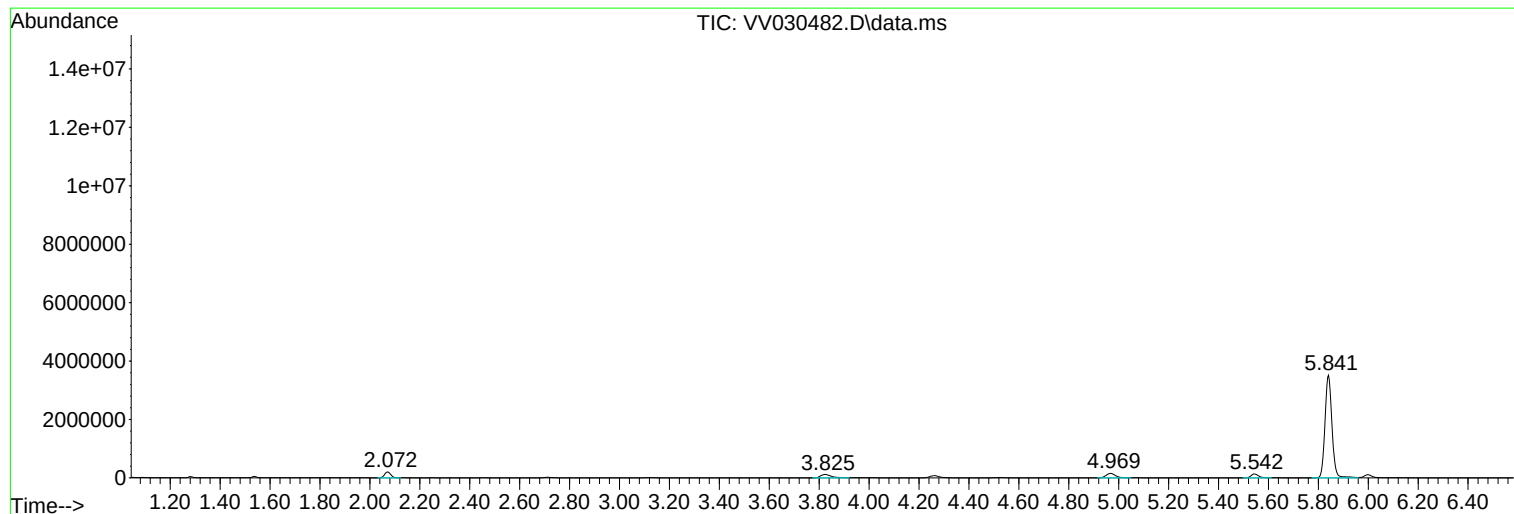

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030482.D
Acq On : 10 Apr 2023 21:02
Operator : SY/MD
Sample : 02250-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030482.D
Acq On : 10 Apr 2023 21:02
Operator : SY/MD
Sample : 02250-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc