

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
 Data File : VV030483.D
 Acq On : 10 Apr 2023 21:27
 Operator : SY/MD
 Sample : 02194-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	88	rBV	45068	48197	10.83%	1.232%
2	1.539	147	155	164	rBV	51031	60155	13.52%	1.537%
3	2.066	309	319	335	rBV2	102858	154423	34.70%	3.947%
4	2.455	428	440	448	rVB9	3303	6957	1.56%	0.178%
5	3.815	850	863	896	rBV2	43659	158145	35.53%	4.042%
6	4.259	987	1001	1028	rBV	81760	214352	48.16%	5.478%
7	4.529	1074	1085	1094	rVB10	2447	5713	1.28%	0.146%
8	4.969	1199	1222	1246	rBV2	169576	445060	100.00%	11.375%
9	5.545	1387	1401	1421	rBV	134169	283573	63.72%	7.248%
10	5.850	1485	1496	1505	rBV10	6667	12856	2.89%	0.329%
11	5.998	1528	1542	1564	rBV	107366	231078	51.92%	5.906%
12	6.924	1818	1830	1846	rBV	40511	81466	18.30%	2.082%
13	7.252	1919	1932	1945	rBV	184518	336275	75.56%	8.595%
14	7.323	1945	1954	1974	rVB	88944	166009	37.30%	4.243%
15	7.564	2018	2029	2045	rBV	26319	51211	11.51%	1.309%
16	7.915	2116	2138	2148	rBV5	22221	51399	11.55%	1.314%
17	8.034	2165	2175	2211	rBV	193133	401539	90.22%	10.263%
18	8.792	2400	2411	2432	rBV	203886	354957	79.75%	9.072%
19	9.085	2493	2502	2512	rBV8	3976	6651	1.49%	0.170%
20	9.509	2626	2634	2647	rVB8	4654	9430	2.12%	0.241%
21	10.162	2825	2837	2854	rBV	80135	129643	29.13%	3.313%
22	10.336	2878	2891	2900	rBV	15780	27118	6.09%	0.693%
23	11.194	3144	3158	3176	rBV	206062	329820	74.11%	8.430%
24	11.570	3264	3275	3292	rVV	196292	321076	72.14%	8.206%
25	12.204	3463	3472	3480	rVB3	5527	8311	1.87%	0.212%
26	12.297	3489	3501	3509	rBV7	10703	17231	3.87%	0.440%




Sum of corrected areas: 3912645

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030483.D
Acq On : 10 Apr 2023 21:27
Operator : SY/MD
Sample : 02194-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

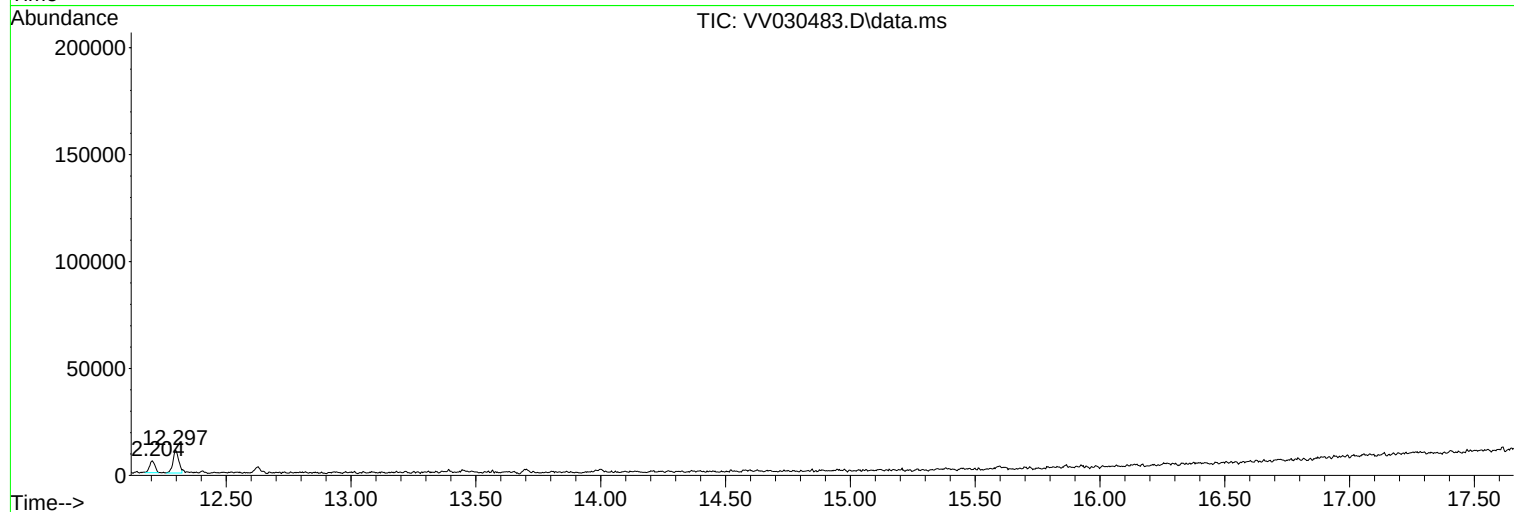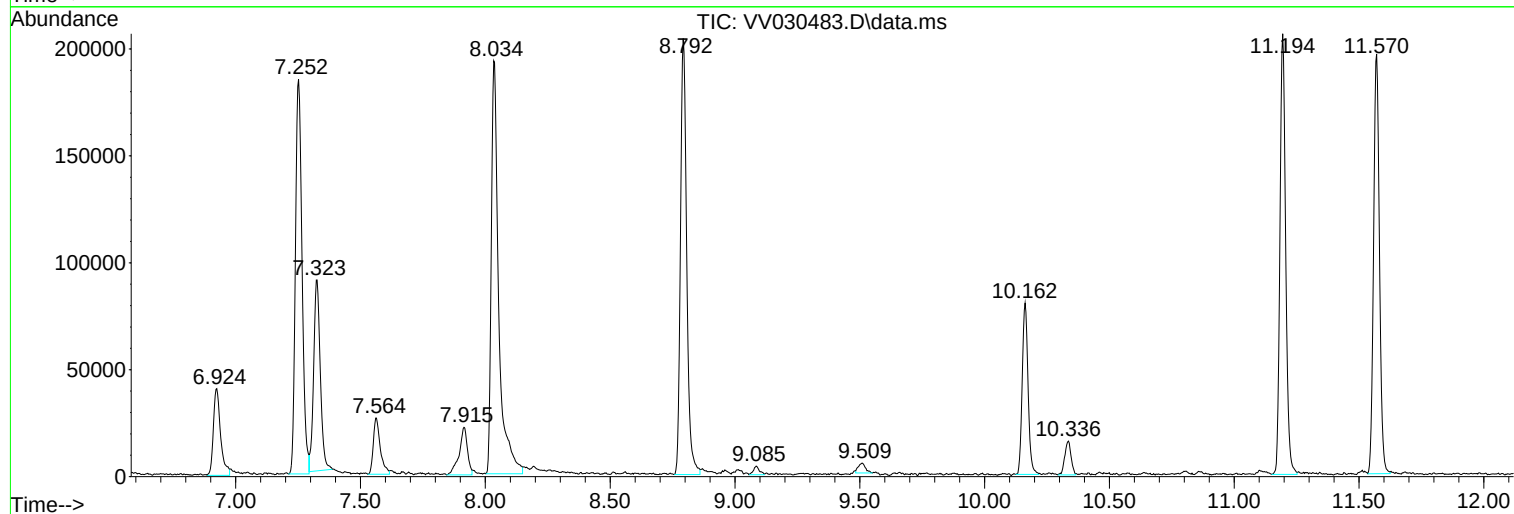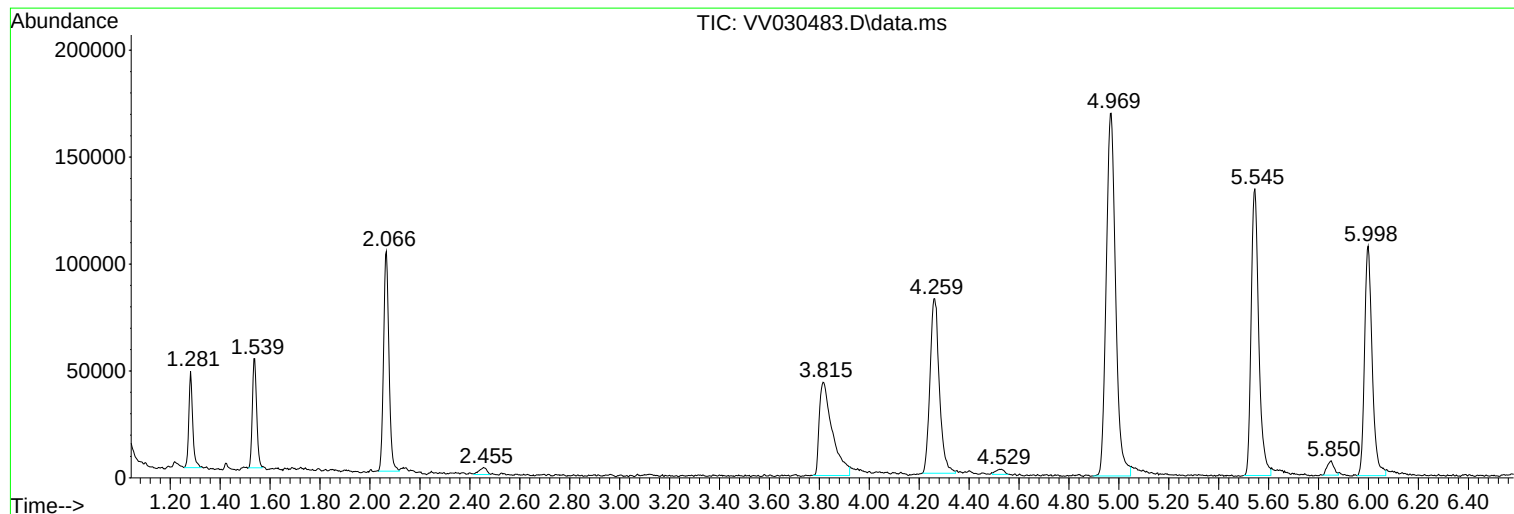

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030483.D
Acq On : 10 Apr 2023 21:27
Operator : SY/MD
Sample : 02194-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030483.D
Acq On : 10 Apr 2023 21:27
Operator : SY/MD
Sample : 02194-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------