
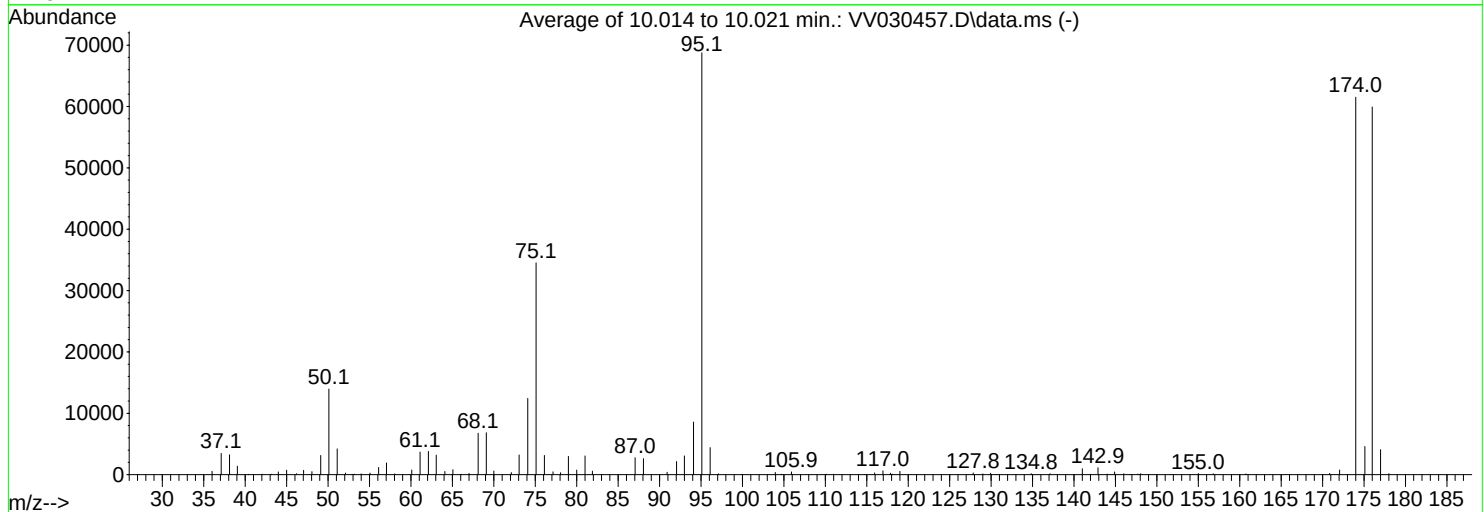


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041023\
Data File : VV030457.D
Acq On : 10 Apr 2023 09:59
Operator : SY/MD
Sample : BFB245
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB245

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Apr 11 06:24:59 2023

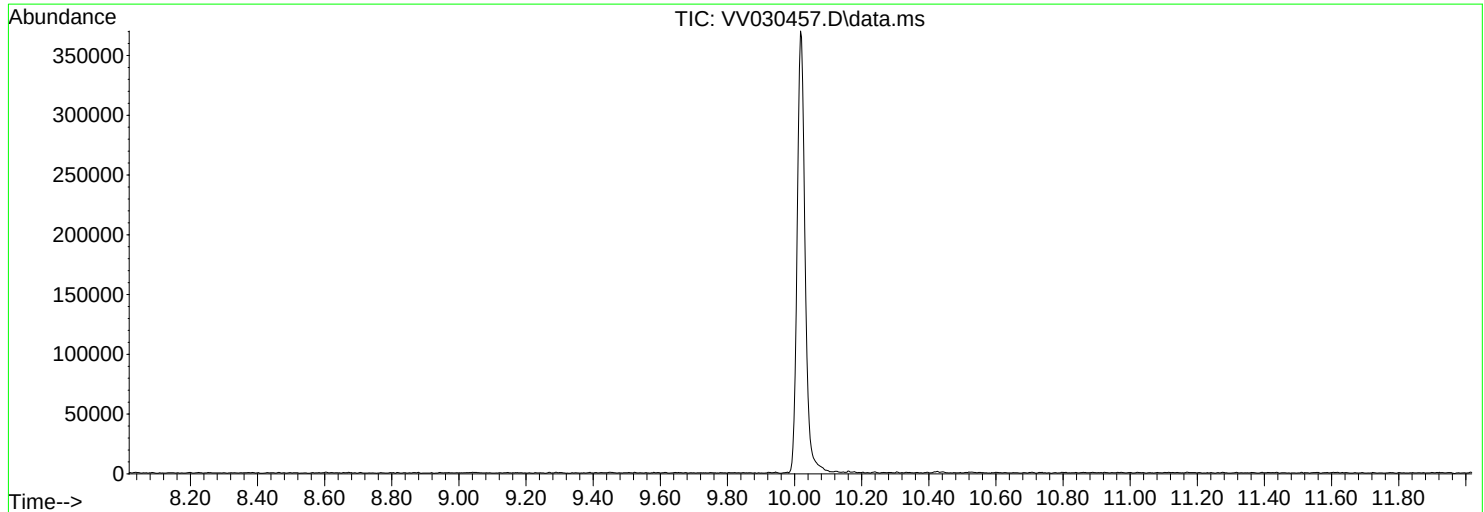

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	13944	PASS
75	95	30	80	50.2	34539	PASS
95	95	100	100	100.0	68744	PASS
96	95	5	9	6.4	4410	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.5	61512	PASS
175	174	5	9	7.5	4595	PASS
176	174	95	105	97.4	59920	PASS
177	176	5	10	6.8	4072	PASS

m/z	Abundance
36.00	123.0
37.20	110.0
39.00	122.0
39.90	246.0
44.00	442.0
68.20	119.0
76.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.00	582.0
37.10	3338.0
38.10	2991.0
39.10	1471.0
39.90	202.0
40.40	128.0
43.20	123.0
44.00	864.0
45.00	671.0
46.20	160.0
47.00	689.0
48.10	551.0
49.10	2976.0
50.10	13175.0
51.10	4135.0
52.10	269.0
52.90	154.0
54.00	140.0
55.00	273.0
56.10	1204.0
57.10	1786.0
58.00	144.0
60.10	718.0
61.10	3446.0
62.10	3650.0
63.00	3037.0
64.10	514.0
65.00	710.0
66.90	239.0
68.10	6392.0
69.10	6562.0
70.00	597.0
72.10	281.0
73.00	2983.0
74.10	11832.0
75.10	32880.0
76.10	3072.0
77.10	501.0
78.10	298.0
79.00	2794.0
80.00	748.0
81.00	2986.0
81.90	580.0
87.10	2666.0
88.00	2524.0
90.90	377.0
92.10	2131.0
93.00	2765.0
94.10	8298.0
95.10	65592.0
96.10	4285.0
97.10	143.0
103.90	353.0
104.70	121.0
105.90	432.0
110.10	117.0
114.70	103.0
115.90	321.0
116.90	623.0
117.90	238.0
119.00	518.0
127.80	230.0
129.00	130.0
130.00	238.0
131.00	123.0
134.80	133.0
137.10	166.0
141.00	929.0
142.90	1085.0
144.00	120.0
144.90	434.0
146.00	157.0
147.70	164.0
148.10	126.0
155.00	202.0
156.80	128.0
160.70	107.0
170.80	162.0
172.00	718.0
174.00	57776.0
175.10	4271.0
176.00	55704.0
177.00	3825.0
178.00	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.00	681.0
37.10	3736.0
38.10	3373.0
39.10	1559.0
39.90	189.0
42.10	102.0
44.00	938.0
45.00	779.0
46.20	165.0
47.00	697.0
48.10	510.0
49.10	3176.0
50.10	14566.0
51.10	4320.0
52.10	260.0
53.20	140.0
54.00	149.0
55.10	258.0
56.10	1189.0
57.10	1971.0
58.10	133.0
60.10	803.0
61.10	3812.0
62.10	3887.0
63.10	3264.0
64.10	529.0
65.10	826.0
66.00	114.0
67.00	195.0
68.10	7105.0
69.10	7084.0
70.00	635.0
72.10	358.0
73.10	3289.0
74.10	12826.0
75.10	35832.0
76.10	3191.0
77.20	500.0
78.10	329.0
79.00	3046.0
80.00	796.0
81.00	3152.0
81.90	586.0
87.10	2823.0
88.10	2654.0
90.90	385.0
92.00	2228.0
93.00	3129.0
94.10	8937.0
95.10	71104.0
96.10	4553.0
97.10	128.0
103.90	366.0
104.70	106.0
105.90	449.0
110.10	124.0
111.00	111.0
115.90	288.0
116.90	649.0
117.80	241.0
119.00	585.0
127.90	305.0
129.00	145.0
130.00	258.0
134.90	175.0
137.10	179.0
141.00	1007.0
142.00	103.0
142.90	1128.0
144.00	121.0
144.90	472.0
146.00	149.0
147.70	173.0
148.10	173.0
155.00	188.0
156.80	153.0
160.80	128.0
170.90	212.0
172.10	764.0
174.00	63520.0
175.10	4708.0
176.00	62104.0
177.00	4227.0
178.00	174.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.00	715.0
37.10	3684.0
38.10	3372.0
39.10	1469.0
40.00	186.0
41.00	114.0
42.00	106.0
43.10	106.0
44.00	895.0
45.00	765.0
46.20	151.0
47.10	695.0
48.00	455.0
49.10	3219.0
50.10	14092.0
51.10	4179.0
52.10	240.0
53.20	140.0
54.00	144.0
55.10	240.0
56.10	1103.0
57.00	1961.0
58.10	133.0
60.10	776.0
61.10	3780.0
62.10	3784.0
63.00	3229.0
64.10	495.0
65.10	875.0
66.10	138.0
67.10	185.0
68.10	7123.0
69.10	6877.0
70.00	600.0
72.10	396.0
73.10	3319.0
74.10	12576.0
75.10	34904.0
76.10	3098.0
77.20	443.0
78.00	329.0
79.00	3064.0
80.00	729.0
81.00	3040.0
81.90	593.0
87.00	2781.0
88.00	2609.0
90.90	382.0
92.00	2063.0
93.00	3256.0
94.10	8504.0
95.10	69536.0
96.10	4391.0
97.10	112.0
104.00	363.0
105.90	419.0
111.00	126.0
116.00	258.0
117.00	618.0
117.80	222.0
118.10	210.0
119.00	581.0
127.90	345.0
129.00	160.0
129.90	258.0
130.70	111.0
134.90	184.0
137.10	149.0
141.00	937.0
142.00	102.0
142.90	1133.0
144.00	115.0
144.90	454.0
146.00	139.0
146.80	105.0
148.00	213.0
151.70	109.0
155.00	165.0
156.80	205.0
160.70	131.0
170.90	245.0
172.10	814.0
174.00	63240.0
175.10	4806.0
176.00	61952.0
177.00	4165.0
178.00	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245