

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035097.D
 Acq On : 10 Apr 2024 10:28
 Operator : SY/MD
 Sample : P1979-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 11 06:56:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:53:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	332736	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	314244	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	132135	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	123793	38.524	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.040%
7) Chloroethane-d5	1.526	69	115633	41.430	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.860%
11) 1,1-Dichloroethene-d2	2.056	65	56851	40.360	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.720%
21) 2-Butanone-d5	3.783	46	199102	104.471	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.470%
24) Chloroform-d	4.243	84	251724	46.592	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.180%
26) 1,2-Dichloroethane-d4	4.937	65	167050	48.700	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.400%
32) Benzene-d6	4.957	84	486650	46.104	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.200%
36) 1,2-Dichloropropane-d6	5.986	67	169180	50.472	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.940%
41) Toluene-d8	7.240	98	403369	42.432	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.860%
43) trans-1,3-Dichloroprop...	7.551	79	64130	39.355	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.720%
47) 2-Hexanone-d5	8.024	63	115785	91.363	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.360%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	235012	50.914	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.820%
66) 1,2-Dichlorobenzene-d4	11.558	152	145749	49.128	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.260%
Target Compounds						
13) Acetone	2.118	43	9477	5.416	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035097.D
Acq On : 10 Apr 2024 10:28
Operator : SY/MD
Sample : P1979-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Apr 11 06:56:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

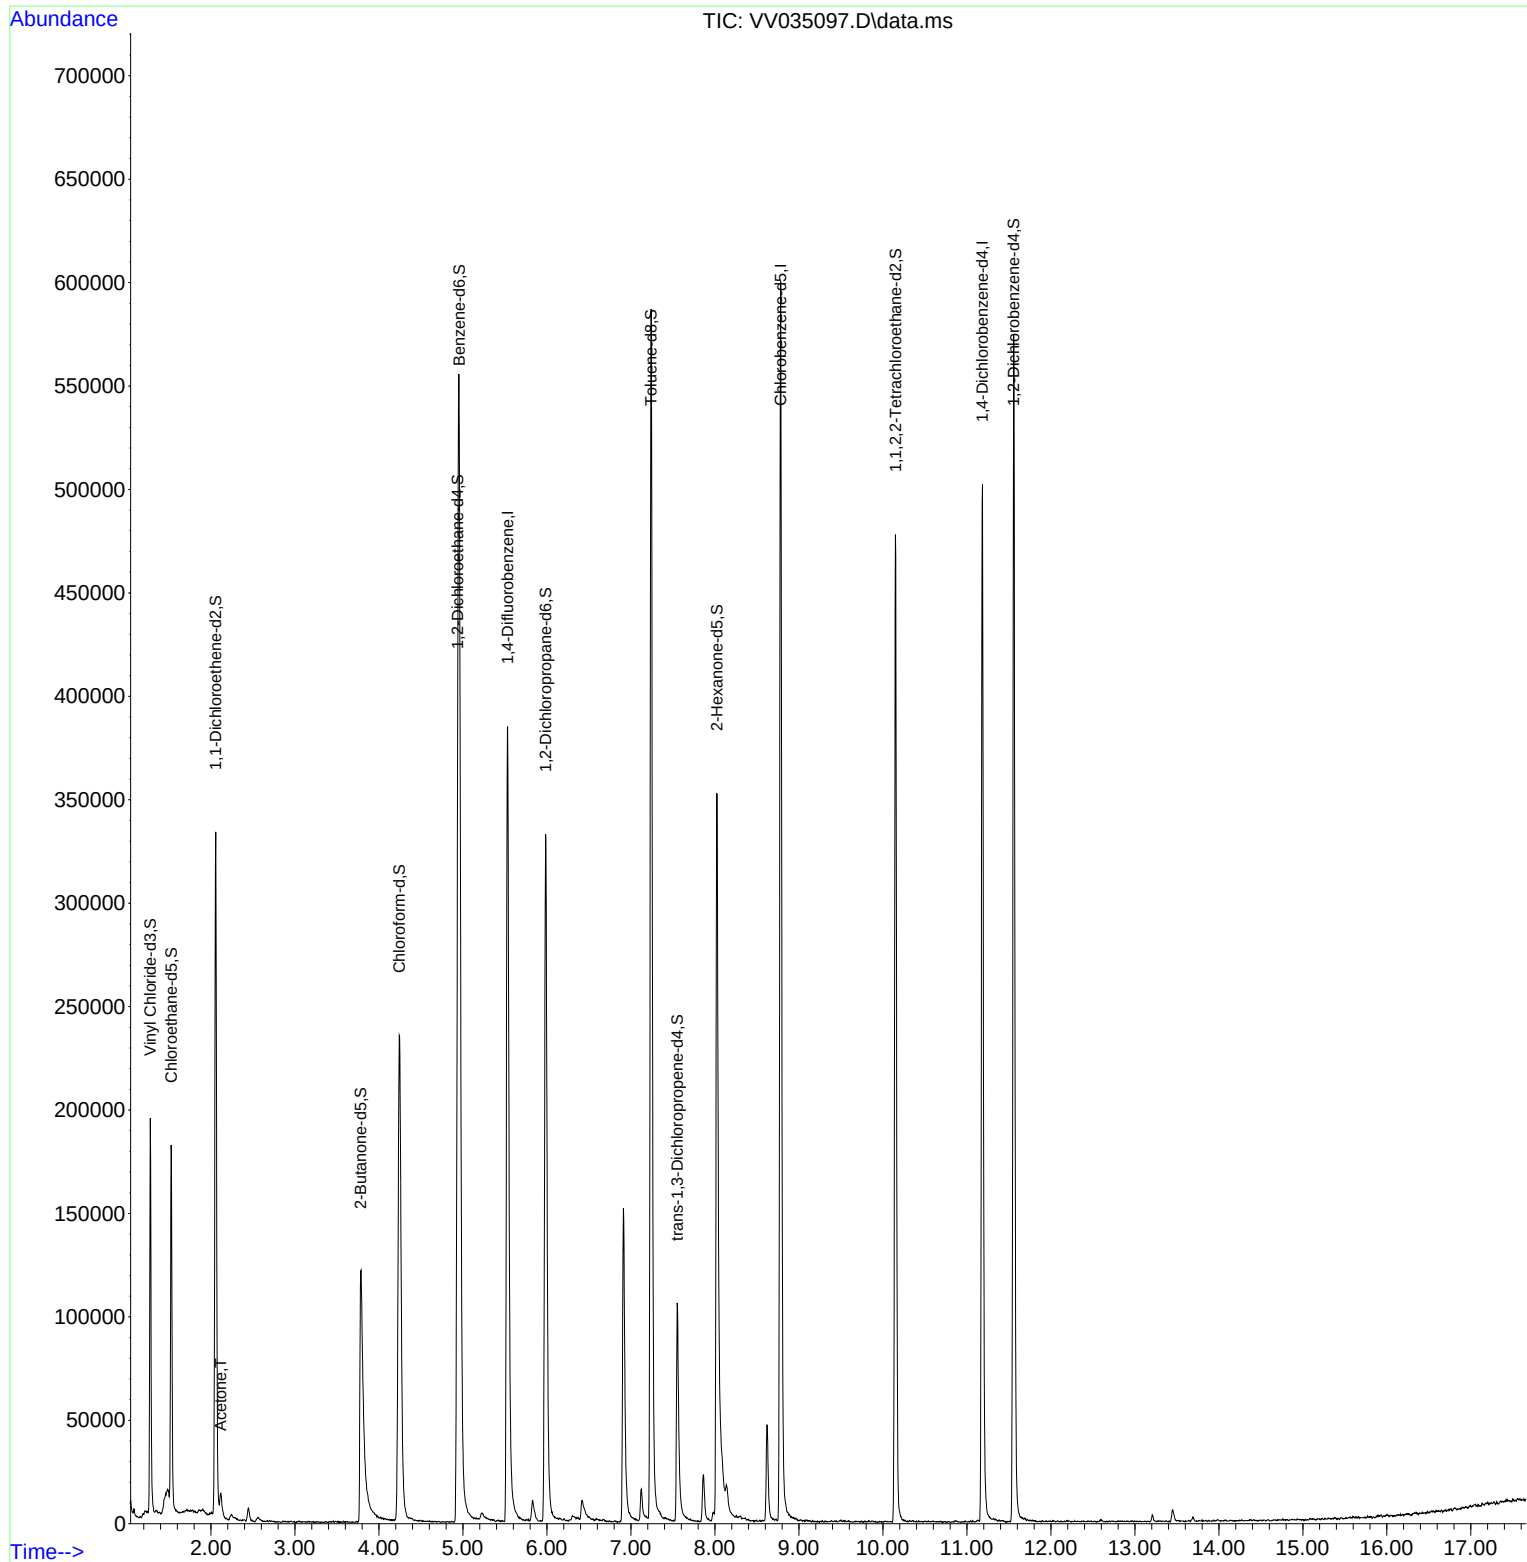

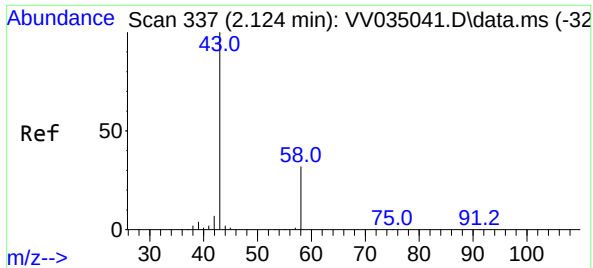

#13
 Acetone
 Concen: 5.416 ug/L
 RT: 2.118 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VV035097.D
 Acq: 10 Apr 2024 10:28

Instrument :
 MSVOA_V
 ClientSampleId :

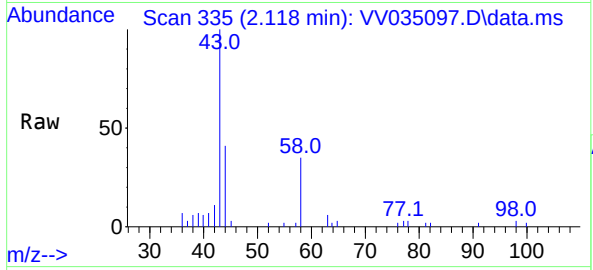

Tgt Ion: 43 Resp: 9477
 Ion Ratio Lower Upper
 43 100
 58 37.1 0.0 66.0

