

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035106.D
 Acq On : 10 Apr 2024 14:04
 Operator : SY/MD
 Sample : P2007-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2N8

Quant Time: Apr 11 06:57:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:53:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	343317	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	334164	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.184	152	143997	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	177367	53.495	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	106.980%	
7) Chloroethane-d5	1.532	69	155476	53.988	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	107.980%	
11) 1,1-Dichloroethene-d2	2.056	65	75217	51.753	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	103.500%	
21) 2-Butanone-d5	3.792	46	213199	108.420	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	108.420%	
24) Chloroform-d	4.246	84	289349	51.905	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	103.820%	
26) 1,2-Dichloroethane-d4	4.940	65	189181	53.452	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	106.900%	
32) Benzene-d6	4.960	84	591088	52.660	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.320%	
36) 1,2-Dichloropropane-d6	5.989	67	193386	54.255	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	108.500%	
41) Toluene-d8	7.242	98	504938	49.950	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	99.900%	
43) trans-1,3-Dichloroprop...	7.554	79	81307	46.922	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	93.840%	
47) 2-Hexanone-d5	8.024	63	122623	90.991	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	90.990%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	250063	50.945	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	101.900%	
66) 1,2-Dichlorobenzene-d4	11.557	152	175562	54.302	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	108.600%	
Target Compounds					Qvalue	
25) Chloroform	4.275	83	22413	4.438	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035106.D
Acq On : 10 Apr 2024 14:04
Operator : SY/MD
Sample : P2007-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2N8

Quant Time: Apr 11 06:57:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:53:36 2024
Response via : Initial Calibration

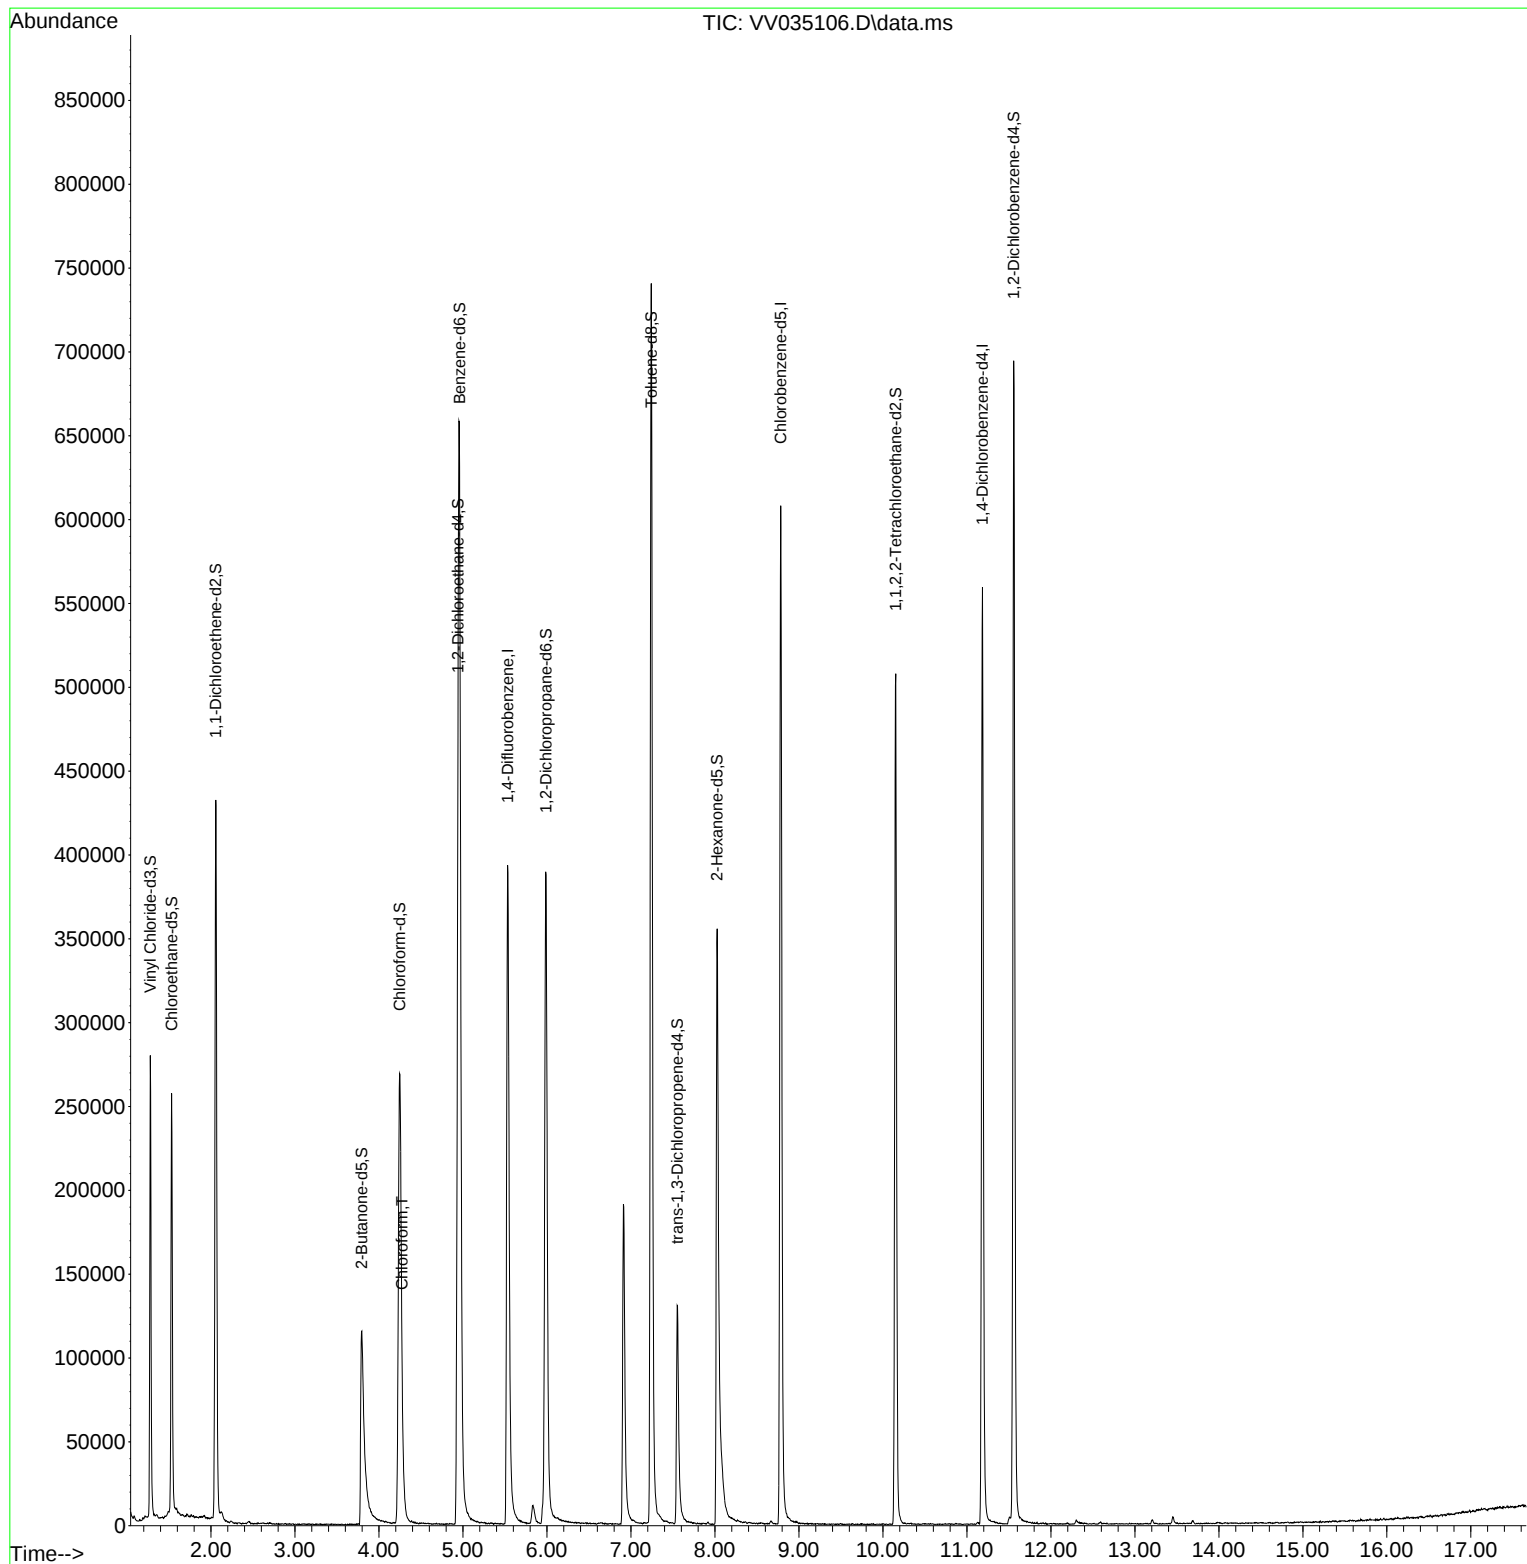

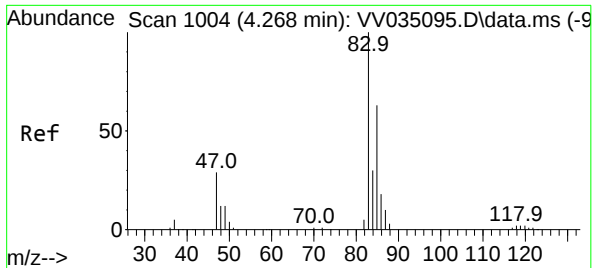

#25
 Chloroform
 Concen: 4.438 ug/L
 RT: 4.275 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV035106.D
 Acq: 10 Apr 2024 14:04

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2N8

Tgt Ion: 83 Resp: 22413
 Ion Ratio Lower Upper
 83 100
 85 64.2 46.0 85.4

