

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035096.D
 Acq On : 10 Apr 2024 09:56
 Operator : SY/MD
 Sample : VV0410WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	264504	271020	16.21%	2.322%
2	1.526	144	151	170	rVB	207961	253740	15.18%	2.174%
3	2.056	307	316	338	rVB	407767	589899	35.29%	5.054%
4	2.745	528	530	533	rVB2	332	126	0.01%	0.001%
5	2.809	547	550	551	rBV	290	171	0.01%	0.001%
6	2.854	559	564	566	rBV2	355	273	0.02%	0.002%
7	2.880	571	572	575	rVV	360	156	0.01%	0.001%
8	2.896	575	577	579	rVV2	433	150	0.01%	0.001%
9	2.921	582	585	588	rVB3	367	177	0.01%	0.002%
10	3.060	624	628	632	rVB	194	181	0.01%	0.002%
11	3.085	632	636	637	rBV2	529	276	0.02%	0.002%
12	3.140	651	653	659	rVB3	362	326	0.02%	0.003%
13	3.175	659	664	667	rBV4	291	310	0.02%	0.003%
14	3.195	667	670	673	rVB2	296	138	0.01%	0.001%
15	3.220	674	678	679	rBV2	343	213	0.01%	0.002%
16	3.282	695	697	702	rBV2	338	257	0.02%	0.002%
17	3.446	744	748	751	rBV3	258	217	0.01%	0.002%
18	3.468	751	755	758	rVV2	422	372	0.02%	0.003%
19	3.552	778	781	785	rBV3	445	277	0.02%	0.002%
20	3.597	793	795	800	rVB2	346	197	0.01%	0.002%
21	3.629	800	805	808	rBV4	254	274	0.02%	0.002%
22	3.651	809	812	817	rVB2	383	303	0.02%	0.003%
23	3.783	844	853	895	rBV	122832	353968	21.17%	3.033%
24	4.246	983	997	1029	rVB	251992	643672	38.50%	5.515%
25	4.564	1092	1096	1099	rBV3	815	661	0.04%	0.006%
26	4.664	1124	1127	1133	rBV4	550	405	0.02%	0.003%
27	4.790	1164	1166	1171	rVB3	388	164	0.01%	0.001%
28	4.835	1178	1180	1184	rVB2	313	126	0.01%	0.001%
29	4.867	1188	1190	1194	rBV	337	172	0.01%	0.001%
30	4.953	1201	1217	1260	rBV2	634031	1671795	100.00%	14.324%
31	5.371	1345	1347	1349	rBV3	433	210	0.01%	0.002%
32	5.478	1377	1380	1382	rBV	353	271	0.02%	0.002%
33	5.532	1386	1397	1424	rBV	376072	790551	47.29%	6.773%
34	5.831	1480	1490	1510	rBV2	10527	25508	1.53%	0.219%
35	5.986	1526	1538	1576	rBV	370283	767478	45.91%	6.576%
36	6.285	1628	1631	1633	rBV3	483	267	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035096.D
 Acq On : 10 Apr 2024 09:56
 Operator : SY/MD
 Sample : VV0410WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.323	1642	1643	1646	rVB2	580	226	0.01%	0.002%
38	6.346	1646	1650	1652	rBV3	373	256	0.02%	0.002%
39	6.378	1656	1660	1665	rVB4	584	575	0.03%	0.005%
40	6.410	1667	1670	1672	rBV2	472	275	0.02%	0.002%
41	6.439	1676	1679	1684	rBV3	425	336	0.02%	0.003%
42	6.487	1691	1694	1696	rBV2	336	189	0.01%	0.002%
43	6.506	1699	1700	1703	rBV	242	130	0.01%	0.001%
44	6.577	1715	1722	1726	rBV2	328	354	0.02%	0.003%
45	6.600	1726	1729	1730	rBV	298	151	0.01%	0.001%
46	6.625	1735	1737	1740	rBV3	490	315	0.02%	0.003%
47	6.645	1740	1743	1746	rBV3	502	282	0.02%	0.002%
48	6.661	1746	1748	1749	rBV	387	167	0.01%	0.001%
49	6.741	1767	1773	1778	rVB3	623	673	0.04%	0.006%
50	6.764	1778	1780	1783	rVB	218	125	0.01%	0.001%
51	6.825	1798	1799	1802	rBV	223	137	0.01%	0.001%
52	6.863	1808	1811	1814	rBV	545	305	0.02%	0.003%
53	6.912	1815	1826	1856	rBV	182027	349628	20.91%	2.996%
54	7.243	1918	1929	1957	rBV	705831	1256137	75.14%	10.763%
55	7.551	2016	2025	2053	rBV2	124493	233301	13.96%	1.999%
56	7.857	2119	2120	2121	rBV2	454	161	0.01%	0.001%
57	7.912	2128	2137	2138	rBV4	656	712	0.04%	0.006%
58	7.947	2146	2148	2150	rVB2	353	133	0.01%	0.001%
59	7.963	2150	2153	2155	rBV4	380	252	0.02%	0.002%
60	8.024	2163	2172	2218	rBV2	344215	742097	44.39%	6.358%
61	8.436	2298	2300	2303	rVB3	608	276	0.02%	0.002%
62	8.548	2333	2335	2337	rBV3	518	296	0.02%	0.003%
63	8.590	2344	2348	2350	rBV4	423	296	0.02%	0.003%
64	8.651	2365	2367	2371	rBV4	545	298	0.02%	0.003%
65	8.683	2375	2377	2379	rBV	461	213	0.01%	0.002%
66	8.735	2390	2393	2397	rBV2	763	592	0.04%	0.005%
67	8.783	2397	2408	2440	rBV	596892	991150	59.29%	8.492%
68	9.384	2587	2595	2600	rBV3	509	544	0.03%	0.005%
69	9.423	2605	2607	2611	rBV2	296	169	0.01%	0.001%
70	9.452	2611	2616	2619	rBV3	456	467	0.03%	0.004%
71	9.529	2638	2640	2644	rBV2	210	158	0.01%	0.001%
72	9.606	2661	2664	2665	rBV2	315	133	0.01%	0.001%
73	9.805	2723	2726	2728	rBV2	230	131	0.01%	0.001%
74	9.847	2737	2739	2741	rBV	275	134	0.01%	0.001%
75	9.918	2759	2761	2765	rVB3	489	240	0.01%	0.002%
76	10.072	2808	2809	2812	rVB2	731	235	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035096.D
 Acq On : 10 Apr 2024 09:56
 Operator : SY/MD
 Sample : VV0410WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.108	2817	2820	2821	rBV	542	346	0.02%	0.003%
78	10.149	2822	2833	2859	rVV	493465	781612	46.75%	6.697%
79	10.387	2904	2907	2909	rBV2	368	210	0.01%	0.002%
80	10.677	2995	2997	2999	rBV2	307	146	0.01%	0.001%
81	10.947	3078	3081	3083	rBV2	341	240	0.01%	0.002%
82	11.024	3103	3105	3111	rVB3	302	228	0.01%	0.002%
83	11.072	3117	3120	3123	rBV2	353	233	0.01%	0.002%
84	11.111	3129	3132	3133	rBV2	451	259	0.02%	0.002%
85	11.133	3133	3139	3144	rVV7	1433	1899	0.11%	0.016%
86	11.185	3144	3155	3180	rBV	525065	846911	50.66%	7.256%
87	11.436	3230	3233	3234	rBV2	424	201	0.01%	0.002%
88	11.558	3260	3271	3301	rBV	653949	1052478	62.95%	9.018%
89	11.857	3363	3364	3365	rBV	399	134	0.01%	0.001%
90	11.905	3376	3379	3382	rBV2	406	323	0.02%	0.003%
91	12.111	3439	3443	3444	rBV2	475	295	0.02%	0.003%
92	12.159	3456	3458	3463	rVB2	452	308	0.02%	0.003%
93	12.181	3463	3465	3469	rBV4	484	435	0.03%	0.004%
94	12.291	3497	3499	3502	rBV2	468	242	0.01%	0.002%
95	12.548	3577	3579	3582	rBV	382	185	0.01%	0.002%
96	12.635	3603	3606	3607	rBV	331	157	0.01%	0.001%
97	12.911	3690	3692	3696	rBV	598	407	0.02%	0.003%
98	13.358	3828	3831	3834	rBV3	630	490	0.03%	0.004%
99	13.445	3850	3858	3872	rBV	15069	26840	1.61%	0.230%
100	14.053	4043	4047	4048	rBV2	420	286	0.02%	0.002%




Sum of corrected areas: 11671415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035096.D
Acq On : 10 Apr 2024 09:56
Operator : SY/MD
Sample : VV0410WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

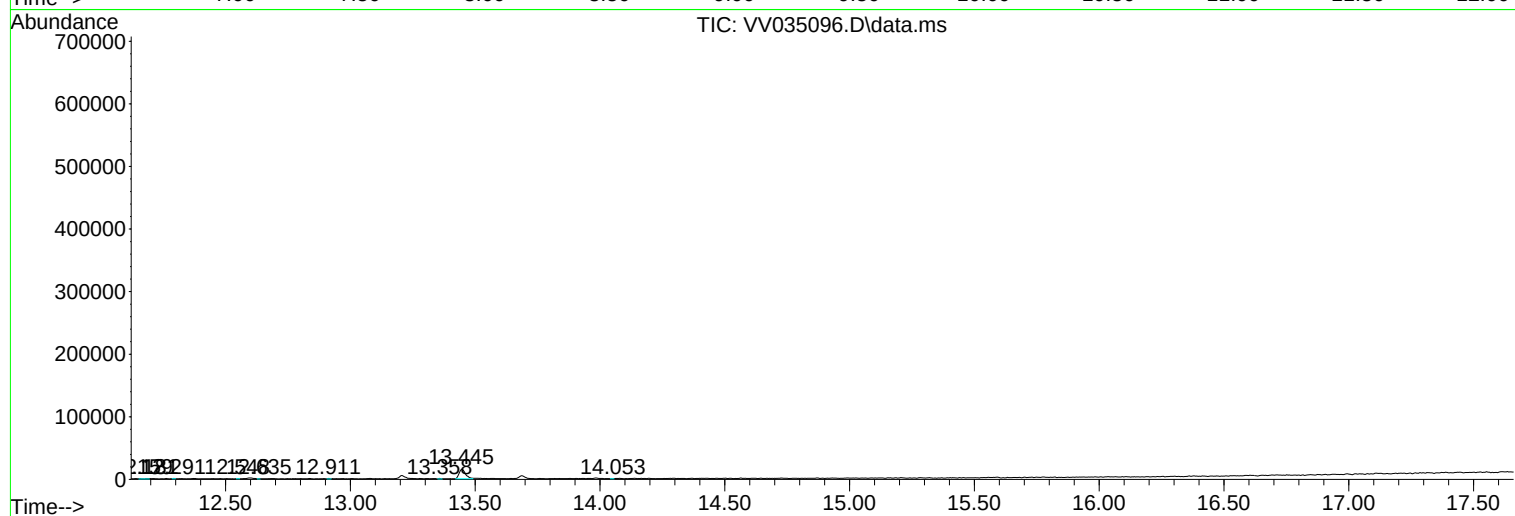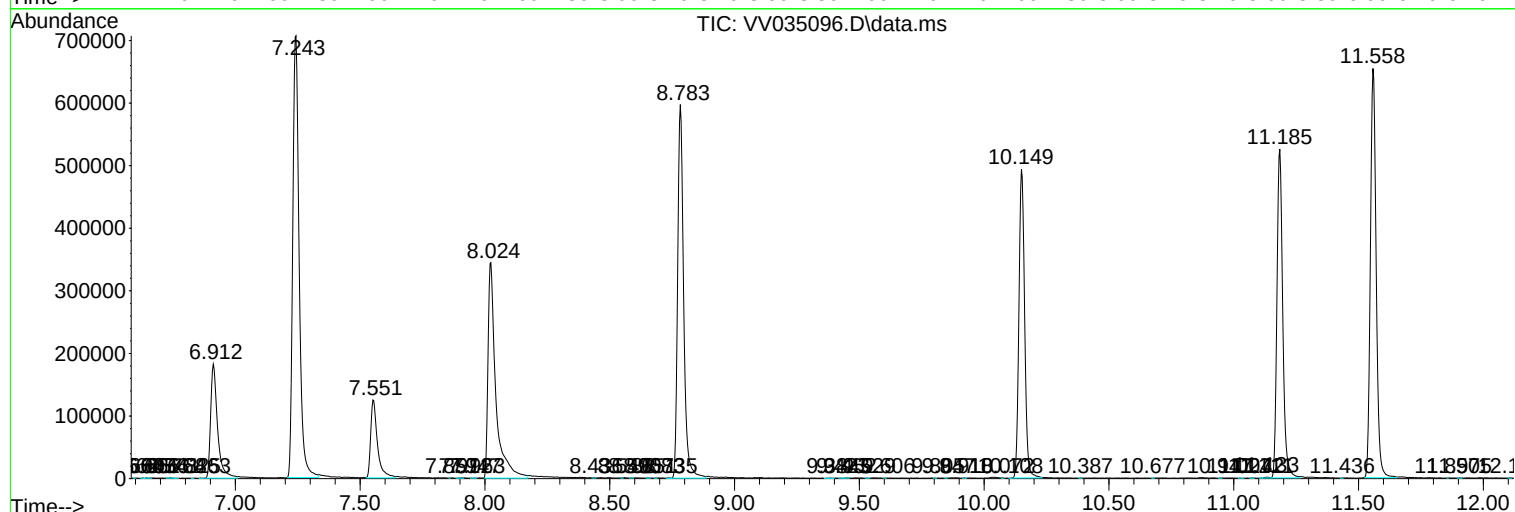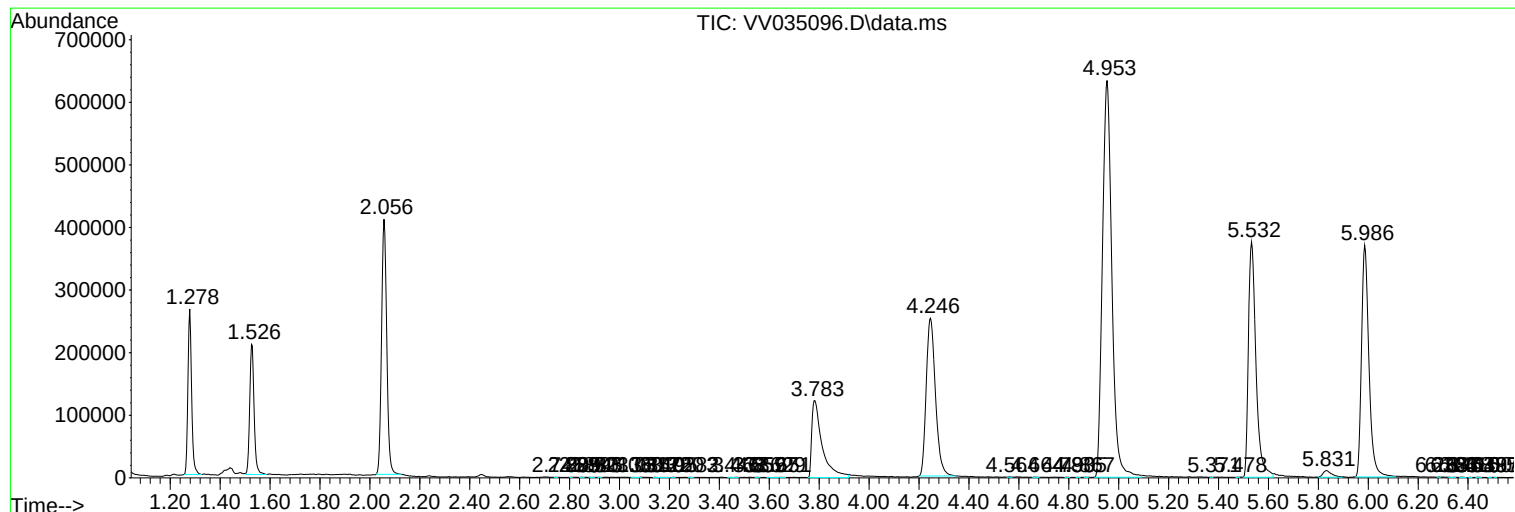

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035096.D
Acq On : 10 Apr 2024 09:56
Operator : SY/MD
Sample : VV0410WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035096.D
Acq On : 10 Apr 2024 09:56
Operator : SY/MD
Sample : VV0410WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------