

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035103.D
 Acq On : 10 Apr 2024 12:52
 Operator : SY/MD
 Sample : P1968-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	222724	242290	14.72%	2.101%
2	1.529	146	152	167	rVB	207477	246929	15.00%	2.142%
3	2.060	308	317	334	rVB	371690	535680	32.54%	4.646%
4	2.449	430	438	449	rVB4	4310	7985	0.49%	0.069%
5	2.700	511	516	524	rVB4	1038	1506	0.09%	0.013%
6	2.873	567	570	571	rBV4	228	123	0.01%	0.001%
7	2.979	599	603	605	rBV2	682	616	0.04%	0.005%
8	3.063	626	629	633	rBV4	403	347	0.02%	0.003%
9	3.095	637	639	641	rBV2	284	126	0.01%	0.001%
10	3.146	651	655	657	rBV2	409	286	0.02%	0.002%
11	3.298	695	702	705	rBV5	509	559	0.03%	0.005%
12	3.317	707	708	710	rBV	311	105	0.01%	0.001%
13	3.336	710	714	718	rVV3	233	239	0.01%	0.002%
14	3.359	718	721	723	rBV3	383	181	0.01%	0.002%
15	3.410	732	737	744	rVB6	510	645	0.04%	0.006%
16	3.510	765	768	770	rBV2	488	344	0.02%	0.003%
17	3.548	776	780	781	rBV2	294	185	0.01%	0.002%
18	3.645	807	810	816	rVB3	248	191	0.01%	0.002%
19	3.690	822	824	826	rBV	333	152	0.01%	0.001%
20	3.706	826	829	833	rVB2	362	206	0.01%	0.002%
21	3.790	846	855	894	rBV	132224	390649	23.73%	3.388%
22	4.249	981	998	1029	rBV	252432	653213	39.68%	5.665%
23	4.748	1148	1153	1155	rBV3	513	412	0.03%	0.004%
24	4.812	1171	1173	1174	rBV	359	134	0.01%	0.001%
25	4.953	1201	1217	1251	rBV2	615707	1646122	100.00%	14.276%
26	5.442	1367	1369	1370	rBV	353	173	0.01%	0.002%
27	5.535	1387	1398	1428	rBV	363298	766511	46.56%	6.648%
28	5.834	1482	1491	1509	rBV4	11648	24472	1.49%	0.212%
29	5.989	1526	1539	1568	rBV	363975	765392	46.50%	6.638%
30	6.420	1671	1673	1674	rBV	293	116	0.01%	0.001%
31	6.535	1706	1709	1712	rVB3	531	209	0.01%	0.002%
32	6.551	1712	1714	1715	rBV	398	131	0.01%	0.001%
33	6.600	1728	1729	1734	rVB3	369	248	0.02%	0.002%
34	6.632	1734	1739	1742	rBV3	496	514	0.03%	0.004%
35	6.648	1742	1744	1745	rBV2	401	168	0.01%	0.001%
36	6.722	1761	1767	1769	rBV3	607	492	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035103.D
 Acq On : 10 Apr 2024 12:52
 Operator : SY/MD
 Sample : P1968-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.760	1775	1779	1782	rBV2	292	210	0.01%	0.002%
38	6.796	1787	1790	1795	rVB2	416	234	0.01%	0.002%
39	6.822	1795	1798	1800	rBV2	389	200	0.01%	0.002%
40	6.863	1807	1811	1812	rBV	196	114	0.01%	0.001%
41	6.912	1815	1826	1854	rBV	179900	354902	21.56%	3.078%
42	7.124	1890	1892	1894	rBV3	520	276	0.02%	0.002%
43	7.243	1918	1929	1971	rBV	677056	1206459	73.29%	10.463%
44	7.555	2016	2026	2055	rBV	126322	238700	14.50%	2.070%
45	7.834	2111	2113	2115	rVB2	686	328	0.02%	0.003%
46	7.886	2127	2129	2134	rBV3	476	345	0.02%	0.003%
47	7.918	2136	2139	2143	rVB3	799	506	0.03%	0.004%
48	7.957	2148	2151	2155	rVB4	384	252	0.02%	0.002%
49	8.024	2163	2172	2223	rBV2	377201	812821	49.38%	7.049%
50	8.744	2393	2396	2397	rBV3	502	323	0.02%	0.003%
51	8.783	2397	2408	2436	rVV	561146	950487	57.74%	8.243%
52	9.014	2478	2480	2481	rBV2	527	216	0.01%	0.002%
53	9.178	2529	2531	2536	rVB4	510	358	0.02%	0.003%
54	9.204	2536	2539	2542	rVB3	448	310	0.02%	0.003%
55	9.223	2542	2545	2549	rBV4	648	486	0.03%	0.004%
56	9.262	2554	2557	2561	rBV4	643	526	0.03%	0.005%
57	9.294	2564	2567	2569	rBV	376	197	0.01%	0.002%
58	9.436	2609	2611	2614	rBV2	367	240	0.01%	0.002%
59	9.481	2623	2625	2628	rBV3	374	293	0.02%	0.003%
60	9.526	2637	2639	2641	rBV	797	314	0.02%	0.003%
61	9.641	2672	2675	2677	rBV3	374	262	0.02%	0.002%
62	9.674	2682	2685	2688	rBV2	535	308	0.02%	0.003%
63	9.776	2715	2717	2720	rBV3	532	302	0.02%	0.003%
64	9.834	2732	2735	2736	rBV2	251	141	0.01%	0.001%
65	10.030	2794	2796	2797	rBV2	295	123	0.01%	0.001%
66	10.069	2805	2808	2810	rBV2	286	158	0.01%	0.001%
67	10.085	2810	2813	2815	rVB3	447	252	0.02%	0.002%
68	10.149	2822	2833	2852	rBV	498195	792906	48.17%	6.877%
69	10.397	2907	2910	2914	rBV2	340	287	0.02%	0.002%
70	10.484	2930	2937	2946	rBV6	814	1422	0.09%	0.012%
71	10.583	2961	2968	2972	rBV3	611	675	0.04%	0.006%
72	10.651	2986	2989	2993	rVB2	422	232	0.01%	0.002%
73	10.670	2993	2995	2999	rVB	243	173	0.01%	0.002%
74	10.696	2999	3003	3006	rBV3	554	475	0.03%	0.004%
75	10.786	3027	3031	3033	rBV2	343	244	0.01%	0.002%
76	10.844	3046	3049	3050	rBV2	225	122	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035103.D
 Acq On : 10 Apr 2024 12:52
 Operator : SY/MD
 Sample : P1968-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.873	3050	3058	3063	rVV5	1204	1622	0.10%	0.014%
78	10.902	3065	3067	3068	rBV5	372	138	0.01%	0.001%
79	11.059	3114	3116	3118	rVB2	328	122	0.01%	0.001%
80	11.069	3118	3119	3120	rBV2	417	113	0.01%	0.001%
81	11.130	3131	3138	3145	rBV5	2176	3403	0.21%	0.030%
82	11.185	3145	3155	3178	rVV	497205	797446	48.44%	6.916%
83	11.558	3259	3271	3291	rBV	628138	1004774	61.04%	8.714%
84	11.931	3384	3387	3390	rBV3	378	310	0.02%	0.003%
85	12.046	3421	3423	3424	rBV	409	157	0.01%	0.001%
86	12.085	3432	3435	3436	rBV3	358	242	0.01%	0.002%
87	12.220	3474	3477	3480	rBV2	259	214	0.01%	0.002%
88	12.281	3494	3496	3499	rBV	399	247	0.02%	0.002%
89	12.374	3522	3525	3528	rBV3	741	507	0.03%	0.004%
90	12.593	3586	3593	3600	rBV6	2646	3960	0.24%	0.034%
91	12.927	3693	3697	3701	rBV2	664	507	0.03%	0.004%
92	13.005	3719	3721	3724	rBV	365	239	0.01%	0.002%
93	13.095	3745	3749	3751	rBV2	505	416	0.03%	0.004%
94	13.133	3759	3761	3765	rBV3	525	327	0.02%	0.003%
95	13.178	3773	3775	3776	rBV	578	248	0.02%	0.002%
96	13.204	3778	3783	3792	rVB5	5890	8675	0.53%	0.075%
97	13.316	3816	3818	3823	rBV2	429	341	0.02%	0.003%
98	13.445	3849	3858	3873	rBV2	22000	40677	2.47%	0.353%
99	13.683	3926	3932	3943	rVB4	6885	10353	0.63%	0.090%
100	13.844	3979	3982	3986	rBV3	536	432	0.03%	0.004%




Sum of corrected areas: 11530300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035103.D
Acq On : 10 Apr 2024 12:52
Operator : SY/MD
Sample : P1968-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

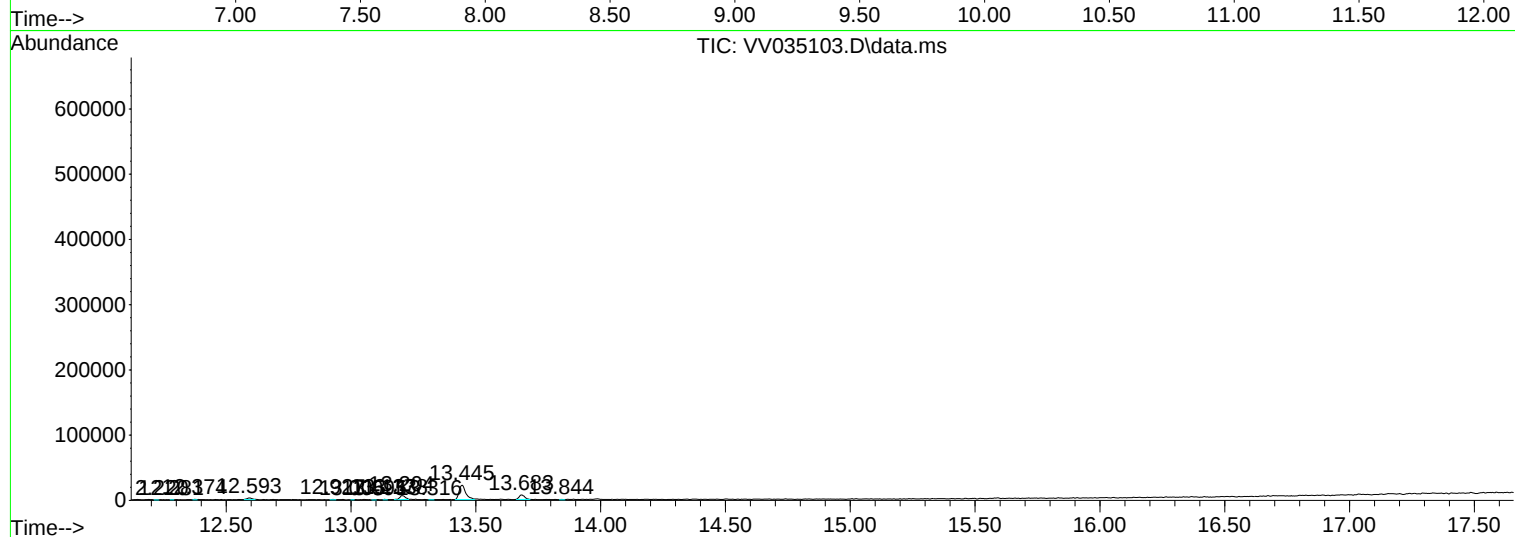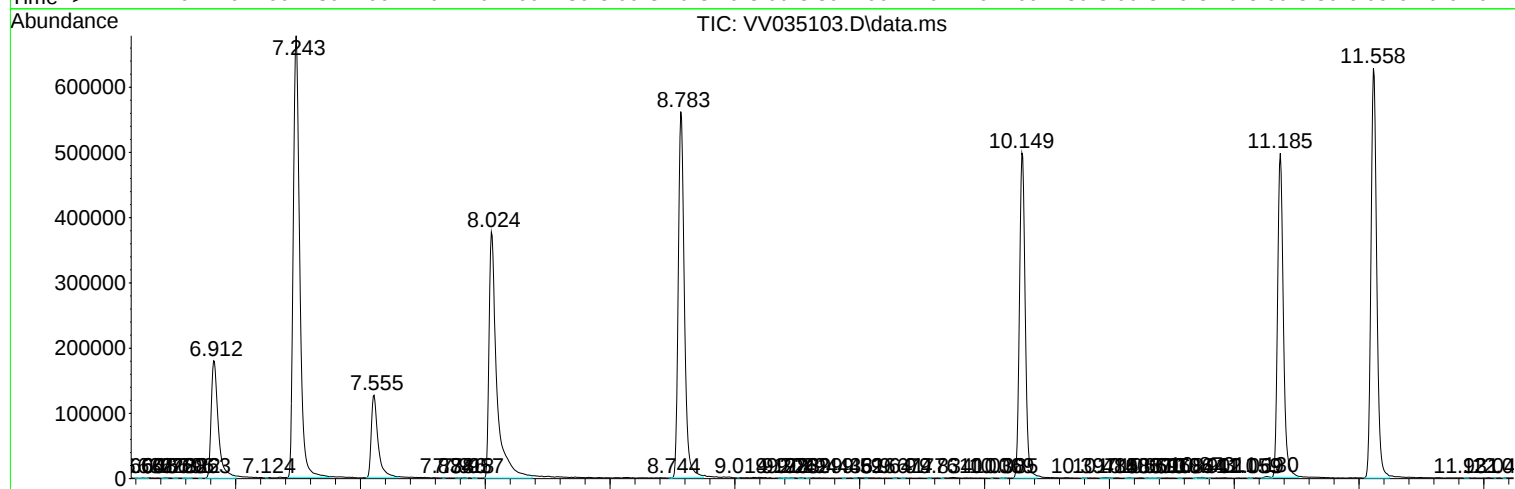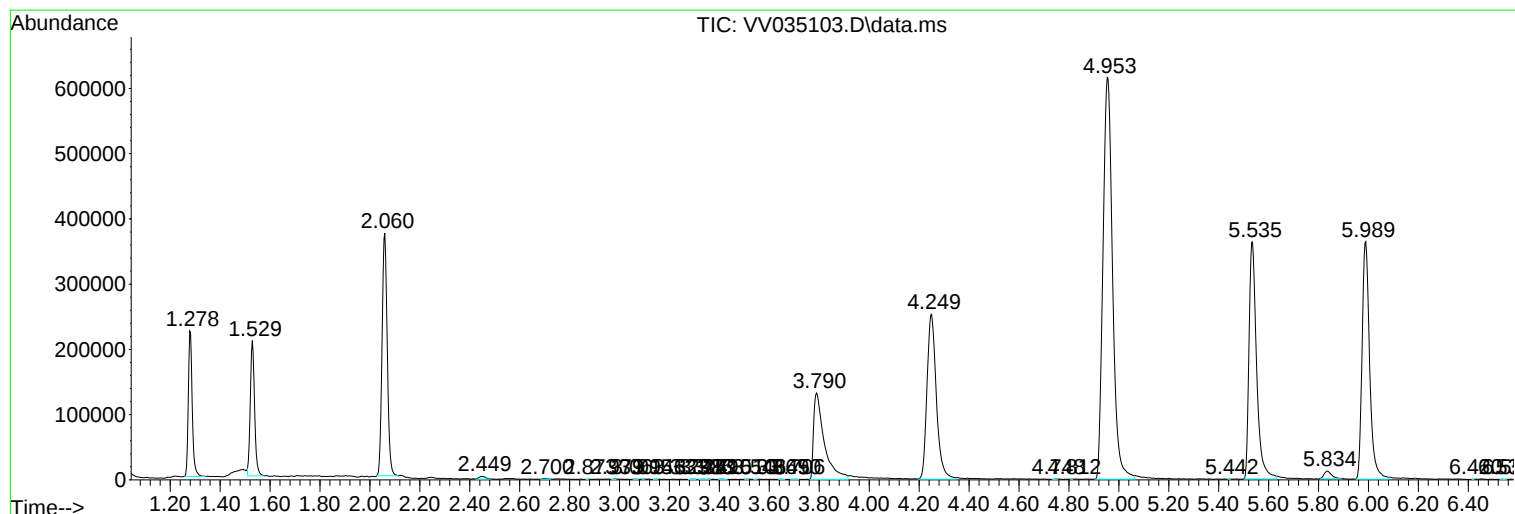

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035103.D
Acq On : 10 Apr 2024 12:52
Operator : SY/MD
Sample : P1968-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035103.D
Acq On : 10 Apr 2024 12:52
Operator : SY/MD
Sample : P1968-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc