

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035110.D
 Acq On : 10 Apr 2024 15:40
 Operator : SY/MD
 Sample : P2007-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	11	14	25	rVB2	18391	18419	0.97%	0.138%
2	1.278	67	74	91	rVB	299468	311048	16.36%	2.326%
3	1.529	146	152	168	rVB	277917	321811	16.93%	2.407%
4	2.056	307	316	330	rBV	463532	669774	35.23%	5.009%
5	2.532	462	464	467	rBV	325	159	0.01%	0.001%
6	2.773	537	539	541	rVB2	350	156	0.01%	0.001%
7	2.793	543	545	549	rVB3	383	254	0.01%	0.002%
8	2.812	549	551	553	rBV	417	184	0.01%	0.001%
9	2.870	566	569	573	rBV5	709	591	0.03%	0.004%
10	2.902	577	579	581	rBV2	378	180	0.01%	0.001%
11	2.941	589	591	594	rBV3	471	307	0.02%	0.002%
12	3.011	611	613	616	rBV	332	200	0.01%	0.001%
13	3.050	622	625	627	rBV2	384	234	0.01%	0.002%
14	3.118	642	646	648	rVB3	511	352	0.02%	0.003%
15	3.130	648	650	651	rBV3	367	171	0.01%	0.001%
16	3.166	659	661	663	rVB2	267	88	0.00%	0.001%
17	3.182	663	666	669	rVB2	404	292	0.02%	0.002%
18	3.211	669	675	678	rBV2	354	340	0.02%	0.003%
19	3.304	703	704	707	rBV2	367	168	0.01%	0.001%
20	3.330	710	712	714	rBV	208	109	0.01%	0.001%
21	3.445	743	748	750	rVV3	230	196	0.01%	0.001%
22	3.484	757	760	762	rBV	391	196	0.01%	0.001%
23	3.523	769	772	776	rBV2	355	255	0.01%	0.002%
24	3.574	786	788	790	rBV2	343	180	0.01%	0.001%
25	3.606	795	798	801	rVB3	533	279	0.01%	0.002%
26	3.626	801	804	807	rBV2	541	301	0.02%	0.002%
27	3.648	807	811	813	rVB3	236	143	0.01%	0.001%
28	3.667	813	817	819	rBV	668	528	0.03%	0.004%
29	3.790	846	855	890	rBV	125494	378480	19.91%	2.830%
30	4.246	983	997	1032	rVB	295768	808187	42.51%	6.044%
31	4.635	1116	1118	1122	rBV2	542	327	0.02%	0.002%
32	4.767	1157	1159	1164	rBV3	326	227	0.01%	0.002%
33	4.953	1201	1217	1258	rBV2	718680	1901329	100.00%	14.218%
34	5.452	1369	1372	1373	rBV2	432	269	0.01%	0.002%
35	5.532	1386	1397	1436	rBV	414746	866785	45.59%	6.482%
36	5.831	1479	1490	1506	rBV2	11251	26759	1.41%	0.200%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035110.D
 Acq On : 10 Apr 2024 15:40
 Operator : SY/MD
 Sample : P2007-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.928	1513	1520	1525	rBV4	17415	28865	1.52%	0.216%
38	5.986	1529	1538	1568	rVB	431948	893213	46.98%	6.679%
39	6.555	1713	1715	1717	rBV2	606	261	0.01%	0.002%
40	6.568	1717	1719	1721	rBV2	555	253	0.01%	0.002%
41	6.670	1749	1751	1753	rBV2	430	235	0.01%	0.002%
42	6.767	1779	1781	1785	rVV3	432	316	0.02%	0.002%
43	6.870	1811	1813	1814	rBV	453	192	0.01%	0.001%
44	6.912	1815	1826	1854	rVV	214486	407823	21.45%	3.050%
45	7.243	1917	1929	1955	rBV	825719	1451828	76.36%	10.857%
46	7.551	2016	2025	2061	rBV	145368	274606	14.44%	2.054%
47	8.024	2163	2172	2219	rBV2	386448	857937	45.12%	6.416%
48	8.529	2326	2329	2331	rBV3	666	470	0.02%	0.004%
49	8.712	2383	2386	2387	rBV2	484	243	0.01%	0.002%
50	8.783	2396	2408	2441	rBV	644086	1075212	56.55%	8.040%
51	9.085	2499	2502	2504	rBV4	770	508	0.03%	0.004%
52	9.217	2541	2543	2545	rBV2	314	148	0.01%	0.001%
53	9.281	2560	2563	2565	rBV2	303	184	0.01%	0.001%
54	9.297	2566	2568	2573	rVB3	699	476	0.03%	0.004%
55	9.320	2573	2575	2578	rBV	265	147	0.01%	0.001%
56	9.352	2582	2585	2588	rBV3	695	580	0.03%	0.004%
57	9.423	2600	2607	2610	rBV3	573	524	0.03%	0.004%
58	9.465	2612	2620	2628	rBV6	2475	4774	0.25%	0.036%
59	9.645	2673	2676	2678	rBV3	478	269	0.01%	0.002%
60	9.706	2691	2695	2700	rVB3	302	276	0.01%	0.002%
61	9.738	2700	2705	2709	rBV3	553	550	0.03%	0.004%
62	9.847	2737	2739	2741	rVB3	369	100	0.01%	0.001%
63	9.860	2741	2743	2746	rBV	352	143	0.01%	0.001%
64	9.876	2746	2748	2749	rBV	383	157	0.01%	0.001%
65	9.937	2763	2767	2768	rBV	249	179	0.01%	0.001%
66	9.966	2773	2776	2780	rBV2	417	304	0.02%	0.002%
67	9.998	2780	2786	2791	rBV4	427	496	0.03%	0.004%
68	10.043	2797	2800	2803	rBV3	432	251	0.01%	0.002%
69	10.149	2821	2833	2860	rBV	557800	886039	46.60%	6.626%
70	10.323	2882	2887	2891	rVB3	922	896	0.05%	0.007%
71	10.445	2923	2925	2926	rBV	296	147	0.01%	0.001%
72	10.490	2936	2939	2942	rVB4	723	437	0.02%	0.003%
73	10.526	2947	2950	2951	rBV	400	256	0.01%	0.002%
74	10.558	2958	2960	2963	rBV	365	151	0.01%	0.001%
75	10.574	2963	2965	2967	rVV2	399	227	0.01%	0.002%
76	10.590	2968	2970	2976	rVB3	711	447	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035110.D
 Acq On : 10 Apr 2024 15:40
 Operator : SY/MD
 Sample : P2007-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2N0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.648	2986	2988	2991	rVB	504	213	0.01%	0.002%
78	10.673	2992	2996	2997	rBV	389	247	0.01%	0.002%
79	10.866	3053	3056	3063	rVB5	993	709	0.04%	0.005%
80	10.989	3091	3094	3095	rBV	304	129	0.01%	0.001%
81	11.040	3106	3110	3113	rVB2	233	167	0.01%	0.001%
82	11.056	3113	3115	3119	rBV2	333	168	0.01%	0.001%
83	11.127	3131	3137	3139	rBV4	1195	1239	0.07%	0.009%
84	11.185	3143	3155	3176	rBV	592675	938981	49.39%	7.022%
85	11.513	3250	3257	3259	rBV6	3757	4796	0.25%	0.036%
86	11.558	3261	3271	3293	rVB	764364	1206252	63.44%	9.020%
87	12.056	3423	3426	3429	rBV2	695	373	0.02%	0.003%
88	12.117	3440	3445	3447	rBV4	611	597	0.03%	0.004%
89	12.252	3485	3487	3489	rBV2	383	157	0.01%	0.001%
90	12.355	3516	3519	3521	rBV3	557	447	0.02%	0.003%
91	12.670	3614	3617	3620	rBV2	412	319	0.02%	0.002%
92	12.747	3639	3641	3643	rBV2	454	249	0.01%	0.002%
93	12.879	3680	3682	3684	rBV	498	214	0.01%	0.002%
94	12.947	3702	3703	3707	rBV2	347	246	0.01%	0.002%
95	13.001	3718	3720	3722	rBV	639	369	0.02%	0.003%
96	13.120	3754	3757	3759	rBV2	456	342	0.02%	0.003%
97	13.204	3776	3783	3799	rVB3	7572	12187	0.64%	0.091%
98	13.561	3891	3894	3896	rBV2	371	284	0.01%	0.002%
99	13.632	3914	3916	3918	rVB2	528	239	0.01%	0.002%
100	13.683	3927	3932	3940	rBV6	2880	4217	0.22%	0.032%




Sum of corrected areas: 13372539

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035110.D
Acq On : 10 Apr 2024 15:40
Operator : SY/MD
Sample : P2007-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

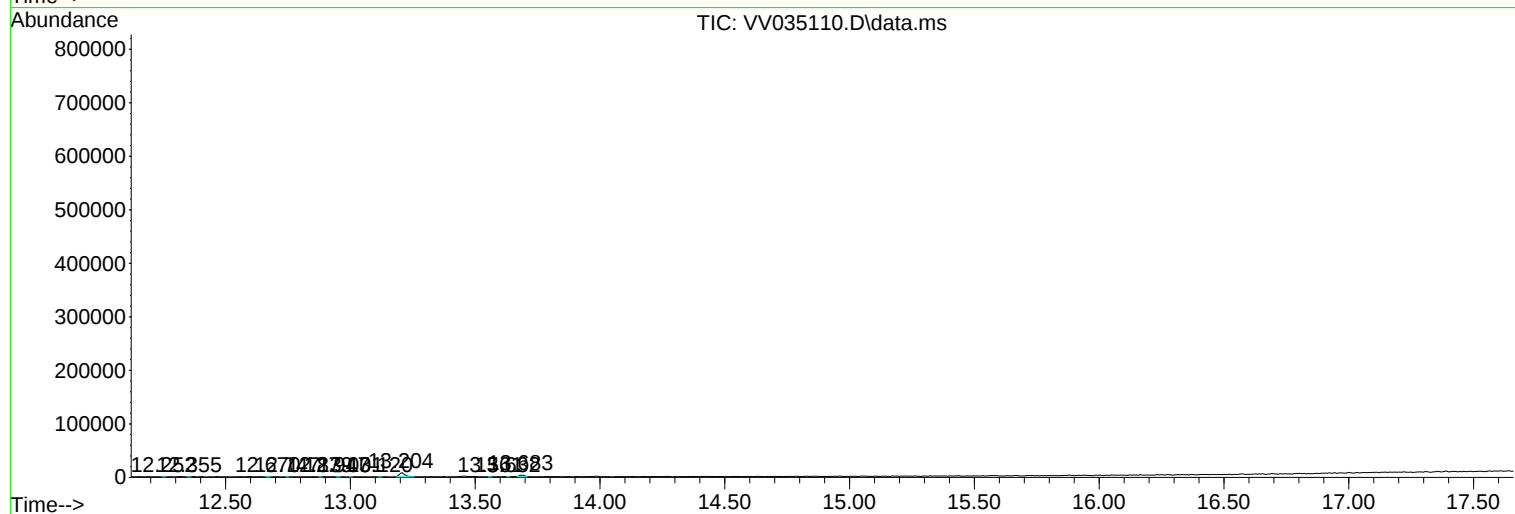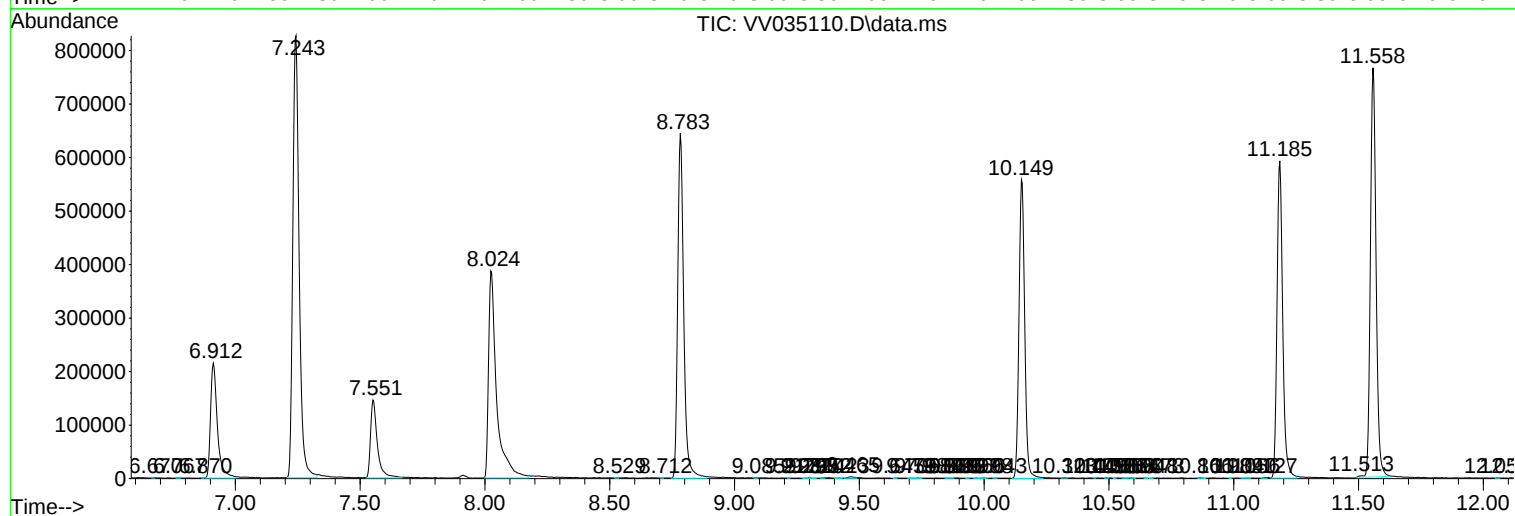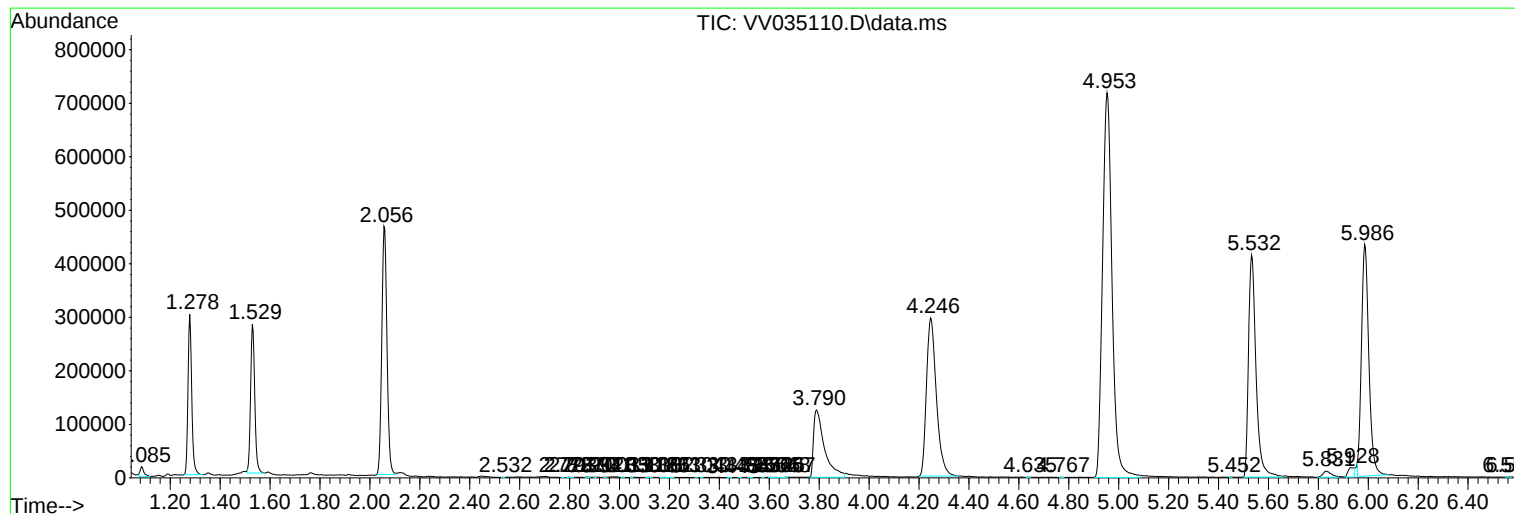

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035110.D
Acq On : 10 Apr 2024 15:40
Operator : SY/MD
Sample : P2007-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035110.D
Acq On : 10 Apr 2024 15:40
Operator : SY/MD
Sample : P2007-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2N0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------