

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035113.D
 Acq On : 10 Apr 2024 16:52
 Operator : SY/MD
 Sample : P2007-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rBV	258346	270342	16.13%	2.285%
2	1.532	146	153	169	rVB	242015	284668	16.99%	2.406%
3	2.057	306	316	333	rBV	415064	602928	35.98%	5.096%
4	2.806	545	549	553	rBV	215	193	0.01%	0.002%
5	2.886	571	574	576	rBV2	416	272	0.02%	0.002%
6	2.931	583	588	591	rBV3	385	387	0.02%	0.003%
7	2.947	591	593	596	rVB2	401	196	0.01%	0.002%
8	2.966	596	599	604	rBV3	462	318	0.02%	0.003%
9	3.134	649	651	654	rVB	180	80	0.00%	0.001%
10	3.153	654	657	659	rBV2	215	120	0.01%	0.001%
11	3.256	684	689	690	rBV	314	244	0.01%	0.002%
12	3.320	707	709	710	rBV	238	118	0.01%	0.001%
13	3.349	713	718	723	rBV2	271	303	0.02%	0.003%
14	3.375	723	726	728	rBV3	358	203	0.01%	0.002%
15	3.420	734	740	745	rVB4	317	455	0.03%	0.004%
16	3.446	745	748	750	rBV2	252	163	0.01%	0.001%
17	3.468	752	755	758	rVB	544	259	0.02%	0.002%
18	3.484	758	760	761	rVB	290	80	0.00%	0.001%
19	3.500	761	765	767	rBV3	365	199	0.01%	0.002%
20	3.510	767	768	772	rVB	234	94	0.01%	0.001%
21	3.638	800	808	812	rBV2	414	513	0.03%	0.004%
22	3.674	816	819	821	rBV	238	149	0.01%	0.001%
23	3.719	831	833	834	rBV2	286	142	0.01%	0.001%
24	3.793	848	856	904	rBV	109974	355953	21.24%	3.008%
25	4.246	981	997	1026	rBV	254656	660247	39.40%	5.580%
26	4.683	1129	1133	1136	rBV4	599	413	0.02%	0.003%
27	4.748	1151	1153	1154	rBV	258	120	0.01%	0.001%
28	4.828	1176	1178	1181	rBV2	269	112	0.01%	0.001%
29	4.880	1191	1194	1195	rBV2	262	177	0.01%	0.001%
30	4.954	1201	1217	1268	rBV2	631952	1675642	100.00%	14.162%
31	5.420	1358	1362	1366	rBV3	456	438	0.03%	0.004%
32	5.532	1386	1397	1428	rBV	381962	802404	47.89%	6.782%
33	5.831	1480	1490	1501	rBV4	13829	30774	1.84%	0.260%
34	5.986	1519	1538	1563	rBV	380112	819378	48.90%	6.925%
35	6.391	1662	1664	1667	rBV3	730	506	0.03%	0.004%
36	6.561	1716	1717	1718	rBV	455	151	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035113.D
 Acq On : 10 Apr 2024 16:52
 Operator : SY/MD
 Sample : P2007-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.706	1758	1762	1765	rBV2	709	490	0.03%	0.004%
38	6.748	1772	1775	1778	rVB2	556	342	0.02%	0.003%
39	6.773	1778	1783	1786	rVB3	678	571	0.03%	0.005%
40	6.789	1786	1788	1790	rBV	367	207	0.01%	0.002%
41	6.812	1793	1795	1797	rBV2	178	93	0.01%	0.001%
42	6.828	1797	1800	1802	rVB4	347	236	0.01%	0.002%
43	6.844	1802	1805	1809	rBV2	603	429	0.03%	0.004%
44	6.876	1814	1815	1816	rBV	387	94	0.01%	0.001%
45	6.912	1816	1826	1859	rBV	183556	354326	21.15%	2.995%
46	7.243	1918	1929	1968	rBV	726289	1272756	75.96%	10.757%
47	7.551	2017	2025	2054	rBV	121902	228961	13.66%	1.935%
48	7.960	2150	2152	2158	rVB3	373	318	0.02%	0.003%
49	8.027	2163	2173	2215	rBV2	332668	760581	45.39%	6.428%
50	8.667	2367	2372	2374	rBV4	521	461	0.03%	0.004%
51	8.783	2397	2408	2439	rBV	600103	998080	59.56%	8.435%
52	9.076	2495	2499	2502	rBV5	765	752	0.04%	0.006%
53	9.149	2521	2522	2523	rBV5	327	109	0.01%	0.001%
54	9.204	2537	2539	2541	rBV	595	373	0.02%	0.003%
55	9.336	2578	2580	2583	rVB	339	106	0.01%	0.001%
56	9.368	2586	2590	2591	rBV	258	143	0.01%	0.001%
57	9.436	2609	2611	2614	rVB3	212	79	0.00%	0.001%
58	9.577	2651	2655	2658	rBV2	588	499	0.03%	0.004%
59	9.619	2667	2668	2672	rVB2	366	213	0.01%	0.002%
60	9.641	2673	2675	2676	rVV	276	97	0.01%	0.001%
61	9.648	2676	2677	2681	rVB3	537	256	0.02%	0.002%
62	9.686	2686	2689	2694	rVB4	600	583	0.03%	0.005%
63	9.712	2694	2697	2700	rVB3	692	394	0.02%	0.003%
64	9.751	2705	2709	2713	rBV3	916	652	0.04%	0.006%
65	9.776	2713	2717	2720	rBV2	534	406	0.02%	0.003%
66	9.799	2721	2724	2728	rBV4	527	440	0.03%	0.004%
67	9.860	2741	2743	2744	rBV	431	152	0.01%	0.001%
68	9.950	2768	2771	2775	rBV2	293	188	0.01%	0.002%
69	9.973	2776	2778	2781	rVV2	313	148	0.01%	0.001%
70	9.989	2781	2783	2787	rVV3	311	224	0.01%	0.002%
71	10.008	2787	2789	2793	rVB	388	253	0.02%	0.002%
72	10.072	2805	2809	2812	rBV2	517	355	0.02%	0.003%
73	10.149	2822	2833	2866	rBV	479658	767797	45.82%	6.489%
74	10.426	2916	2919	2923	rBV3	592	417	0.02%	0.004%
75	10.535	2951	2953	2956	rVB3	511	241	0.01%	0.002%
76	10.551	2956	2958	2959	rBV3	239	99	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
 Data File : VV035113.D
 Acq On : 10 Apr 2024 16:52
 Operator : SY/MD
 Sample : P2007-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH2P8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.686	2998	3000	3003	rBV3	317	153	0.01%	0.001%
78	10.702	3003	3005	3008	rVB2	350	178	0.01%	0.002%
79	10.719	3008	3010	3013	rVB2	289	118	0.01%	0.001%
80	10.744	3015	3018	3021	rBV	566	387	0.02%	0.003%
81	10.812	3037	3039	3040	rBV	430	198	0.01%	0.002%
82	10.873	3055	3058	3063	rVB3	1083	791	0.05%	0.007%
83	10.902	3064	3067	3068	rBV2	511	247	0.01%	0.002%
84	10.979	3089	3091	3093	rBV2	461	257	0.02%	0.002%
85	11.050	3109	3113	3115	rBV2	438	344	0.02%	0.003%
86	11.185	3144	3155	3183	rBV	548893	863623	51.54%	7.299%
87	11.513	3246	3257	3260	rBV6	4408	7330	0.44%	0.062%
88	11.558	3261	3271	3295	rVB	662920	1051922	62.78%	8.891%
89	11.908	3378	3380	3382	rVB2	435	128	0.01%	0.001%
90	12.098	3434	3439	3442	rBV3	599	486	0.03%	0.004%
91	12.194	3465	3469	3473	rBV4	717	755	0.05%	0.006%
92	12.339	3512	3514	3518	rVB2	868	509	0.03%	0.004%
93	12.468	3551	3554	3556	rBV2	564	367	0.02%	0.003%
94	12.513	3565	3568	3569	rBV2	388	196	0.01%	0.002%
95	12.542	3573	3577	3581	rVB3	835	729	0.04%	0.006%
96	12.561	3581	3583	3584	rBV3	447	180	0.01%	0.002%
97	12.583	3588	3590	3591	rBV	533	206	0.01%	0.002%
98	12.641	3605	3608	3611	rVB2	481	300	0.02%	0.003%
99	13.506	3875	3877	3880	rVB2	710	369	0.02%	0.003%
100	13.895	3996	3998	4004	rBV4	680	487	0.03%	0.004%




Sum of corrected areas: 11831922

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035113.D
Acq On : 10 Apr 2024 16:52
Operator : SY/MD
Sample : P2007-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

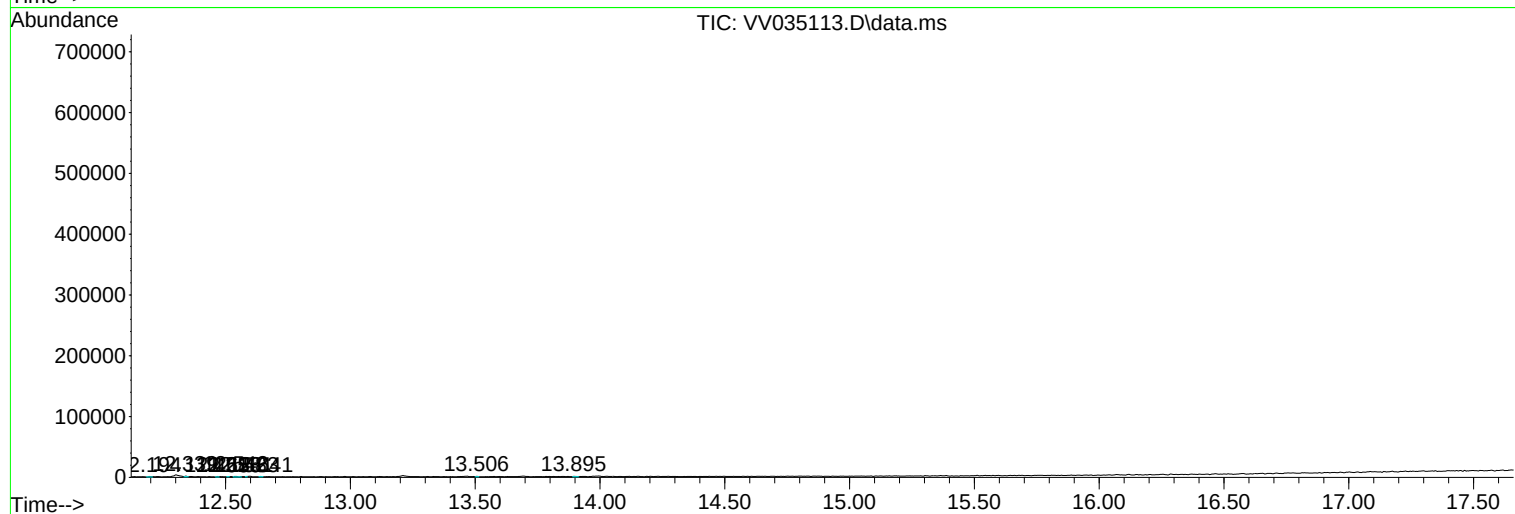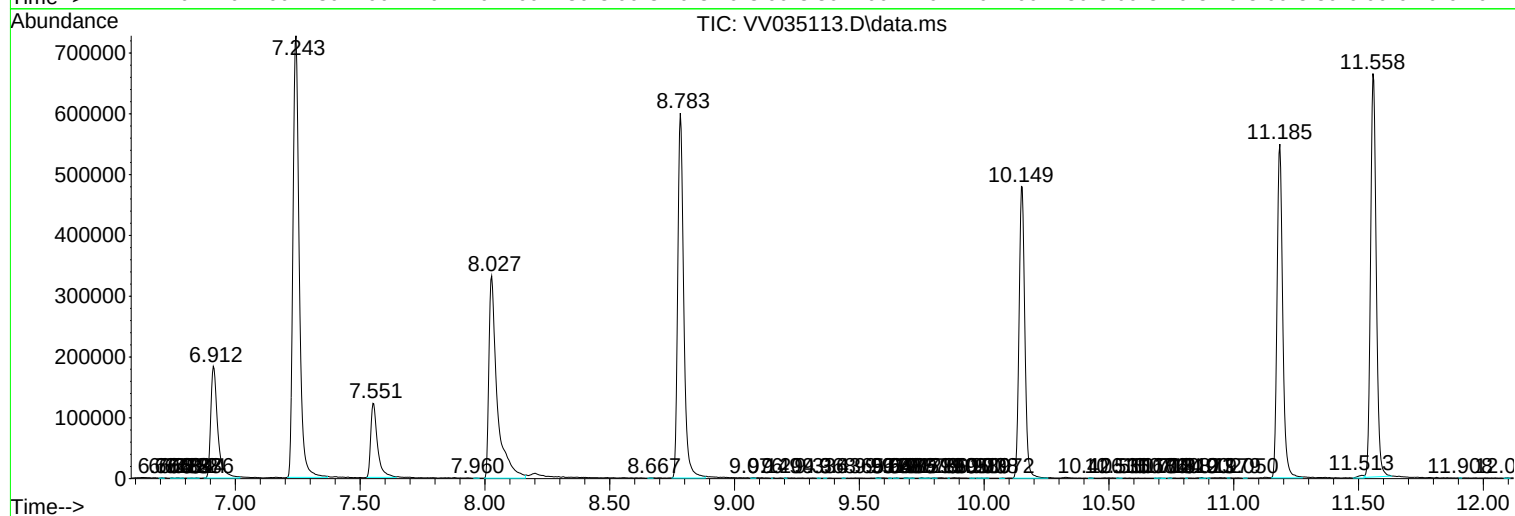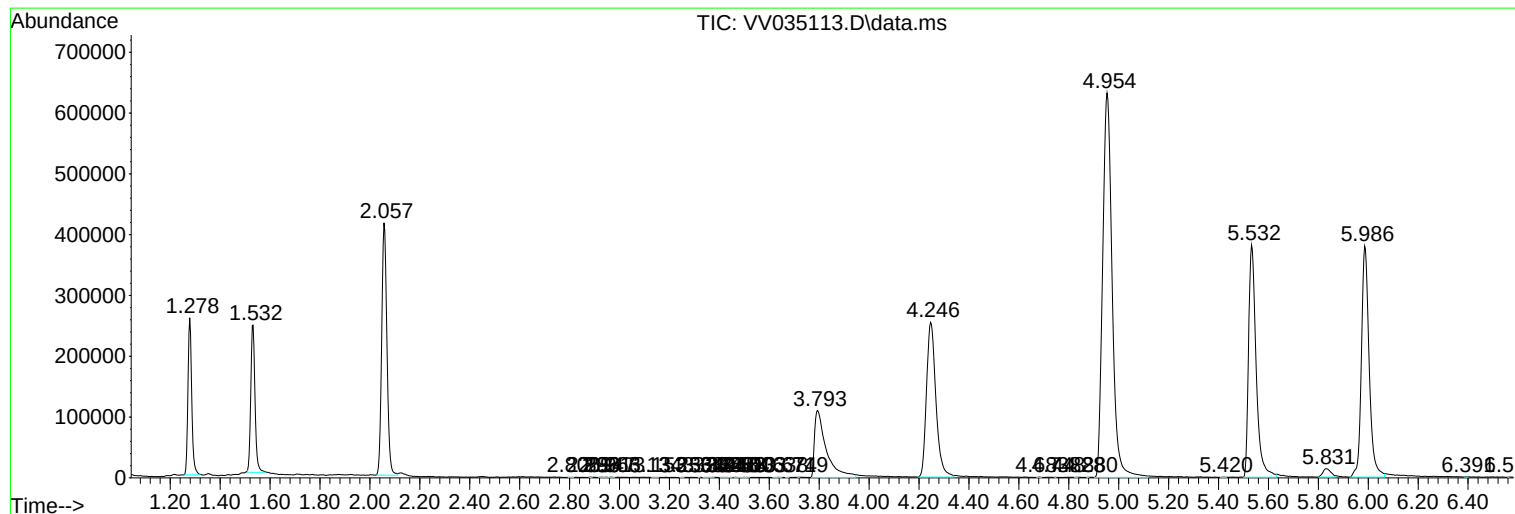

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035113.D
Acq On : 10 Apr 2024 16:52
Operator : SY/MD
Sample : P2007-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041024\
Data File : VV035113.D
Acq On : 10 Apr 2024 16:52
Operator : SY/MD
Sample : P2007-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH2P8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------